

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092122\
 Data File : VU050874.D
 Acq On : 21 Sep 2022 11:36
 Operator : JC/MD
 Sample : N4650-20DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ37DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M

Title : VOC Analysis

Signal : TIC: VU050874.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	74	80	92	rVB	103623	119790	13.60%	1.755%
2	1.909	170	177	197	rVB	87816	119475	13.56%	1.751%
3	2.488	354	357	363	rVB2	1086	1005	0.11%	0.015%
4	2.571	369	383	399	rBV3	240584	470740	53.44%	6.898%
5	2.793	444	452	461	rBV6	2140	3953	0.45%	0.058%
6	2.864	471	474	478	rVB2	745	507	0.06%	0.007%
7	2.961	501	504	507	rBV3	566	491	0.06%	0.007%
8	3.041	521	529	540	rBV6	3504	6541	0.74%	0.096%
9	3.189	557	575	592	rVB	18466	44486	5.05%	0.652%
10	3.272	597	601	604	rVV2	418	378	0.04%	0.006%
11	3.288	604	606	609	rVV3	432	345	0.04%	0.005%
12	3.356	613	627	640	rVB3	5548	11161	1.27%	0.164%
13	3.407	640	643	646	rBV	334	247	0.03%	0.004%
14	3.523	676	679	683	rVB2	456	299	0.03%	0.004%
15	3.870	769	787	806	rBV	118067	281324	31.94%	4.123%
16	3.993	822	825	828	rVB2	491	336	0.04%	0.005%
17	4.134	864	869	872	rBV	476	451	0.05%	0.007%
18	4.186	882	885	888	rBV3	458	321	0.04%	0.005%
19	4.350	934	936	942	rVB2	226	228	0.03%	0.003%
20	4.385	942	947	953	rVB	293	332	0.04%	0.005%
21	4.427	955	960	965	rBV2	346	374	0.04%	0.005%
22	4.485	971	978	982	rBV3	365	456	0.05%	0.007%
23	4.629	1006	1023	1028	rBV3	95862	204026	23.16%	2.990%
24	4.989	1132	1135	1136	rBV3	356	220	0.02%	0.003%
25	5.063	1143	1158	1179	rBV	142051	316088	35.89%	4.632%
26	5.150	1184	1185	1191	rVB4	511	305	0.03%	0.004%
27	5.214	1202	1205	1209	rBV2	510	454	0.05%	0.007%
28	5.317	1219	1237	1256	rBV	390011	880807	100.00%	12.907%
29	5.478	1282	1287	1290	rVV3	500	390	0.04%	0.006%
30	5.504	1290	1295	1297	rVV3	355	369	0.04%	0.005%
31	5.584	1316	1320	1326	rBV3	409	370	0.04%	0.005%
32	5.639	1333	1337	1342	rVB	384	344	0.04%	0.005%
33	5.726	1342	1364	1386	rBV3	280978	766336	87.00%	11.230%
34	5.835	1395	1398	1403	rVB3	868	714	0.08%	0.010%
35	5.870	1406	1409	1414	rBV2	520	435	0.05%	0.006%
36	5.912	1420	1422	1424	rBV2	467	285	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092122\
 Data File : VU050874.D
 Acq On : 21 Sep 2022 11:36
 Operator : JC/MD
 Sample : N4650-20DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ37DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

37	5.970	1436	1440	1444	rBV2	323	349	0.04%	0.005%
38	6.031	1455	1459	1462	rVV3	372	363	0.04%	0.005%
39	6.250	1513	1527	1554	rBV	157591	299969	34.06%	4.396%
40	6.417	1577	1579	1585	rVB	551	385	0.04%	0.006%
41	6.542	1605	1618	1633	rVV3	73883	142089	16.13%	2.082%
42	6.690	1647	1664	1684	rBV2	180951	356690	40.50%	5.227%
43	6.787	1688	1694	1696	rVV3	503	495	0.06%	0.007%
44	6.800	1696	1698	1702	rVB3	414	341	0.04%	0.005%
45	7.047	1772	1775	1777	rBV	376	246	0.03%	0.004%
46	7.070	1780	1782	1792	rVV3	467	698	0.08%	0.010%
47	7.185	1811	1818	1819	rBV	642	609	0.07%	0.009%
48	7.292	1847	1851	1856	rBV2	350	428	0.05%	0.006%
49	7.353	1867	1870	1873	rVB	424	228	0.03%	0.003%
50	7.484	1908	1911	1914	rBV	337	247	0.03%	0.004%
51	7.565	1923	1936	1954	rBV	87442	156878	17.81%	2.299%
52	7.790	2001	2006	2007	rBV	462	307	0.03%	0.004%
53	7.899	2025	2040	2059	rVV	291046	503063	57.11%	7.372%
54	7.973	2059	2063	2072	rVB6	3592	4504	0.51%	0.066%
55	8.179	2115	2127	2148	rBV	62939	107194	12.17%	1.571%
56	8.404	2188	2197	2208	rVB8	3255	6010	0.68%	0.088%
57	8.462	2212	2215	2217	rBV2	402	316	0.04%	0.005%
58	8.475	2217	2219	2224	rVB3	607	458	0.05%	0.007%
59	8.497	2224	2226	2231	rVB	381	291	0.03%	0.004%
60	8.555	2231	2244	2257	rBV	114971	193678	21.99%	2.838%
61	8.636	2257	2269	2299	rBV2	190091	387900	44.04%	5.684%
62	8.976	2372	2375	2382	rVV3	265	371	0.04%	0.005%
63	9.195	2440	2443	2449	rVB	602	513	0.06%	0.008%
64	9.237	2453	2456	2459	rVV2	268	231	0.03%	0.003%
65	9.256	2459	2462	2466	rVV3	323	274	0.03%	0.004%
66	9.288	2466	2472	2478	rVB2	297	364	0.04%	0.005%
67	9.343	2486	2489	2495	rBV2	345	299	0.03%	0.004%
68	9.417	2500	2512	2534	rVV	215109	357339	40.57%	5.236%
69	9.574	2556	2561	2563	rBV2	483	479	0.05%	0.007%
70	9.693	2593	2598	2608	rBV4	786	1326	0.15%	0.019%
71	9.803	2629	2632	2636	rBV2	321	291	0.03%	0.004%
72	10.105	2723	2726	2730	rBV2	318	252	0.03%	0.004%
73	10.343	2794	2800	2803	rBV3	361	354	0.04%	0.005%
74	10.362	2803	2806	2811	rVV	376	273	0.03%	0.004%
75	10.430	2824	2827	2830	rVB2	412	295	0.03%	0.004%
76	10.481	2837	2843	2846	rBV2	678	665	0.08%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092122\
 Data File : VU050874.D
 Acq On : 21 Sep 2022 11:36
 Operator : JC/MD
 Sample : N4650-20DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXZ37DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

77	10.754	2917	2928	2945	rBV	248440	404659	45.94%	5.930%
78	10.999	2996	3004	3006	rBV	451	460	0.05%	0.007%
79	11.095	3027	3034	3036	rBV3	382	496	0.06%	0.007%
80	11.143	3046	3049	3054	rBV2	308	295	0.03%	0.004%
81	11.288	3091	3094	3100	rVB	525	476	0.05%	0.007%
82	11.504	3160	3161	3167	rVB2	630	368	0.04%	0.005%
83	11.751	3235	3238	3243	rVB2	973	879	0.10%	0.013%
84	11.812	3245	3257	3278	rBV	160230	259346	29.44%	3.800%
85	11.970	3304	3306	3314	rVB	517	387	0.04%	0.006%
86	12.192	3363	3375	3393	rBV	231805	384099	43.61%	5.629%
87	12.365	3426	3429	3431	rBV2	377	221	0.03%	0.003%
88	12.741	3543	3546	3551	rVV	301	228	0.03%	0.003%
89	13.066	3644	3647	3650	rVB2	432	271	0.03%	0.004%
90	13.131	3659	3667	3669	rBV3	472	583	0.07%	0.009%
91	13.198	3685	3688	3690	rBV2	538	356	0.04%	0.005%
92	13.269	3707	3710	3713	rBV2	417	250	0.03%	0.004%
93	13.690	3838	3841	3844	rBV3	382	276	0.03%	0.004%
94	13.790	3868	3872	3876	rBV2	744	672	0.08%	0.010%
95	13.848	3886	3890	3895	rVV4	1216	1026	0.12%	0.015%
96	13.883	3898	3901	3904	rBV2	461	374	0.04%	0.005%
97	13.960	3922	3925	3928	rBV	408	336	0.04%	0.005%
98	14.098	3962	3968	3978	rVB2	2828	4139	0.47%	0.061%
99	14.327	4035	4039	4044	rBV6	1964	2143	0.24%	0.031%
100	15.262	4328	4330	4332	rBV3	486	239	0.03%	0.004%




Sum of corrected areas: 6824024

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092122\
Data File : VU050874.D
Acq On : 21 Sep 2022 11:36
Operator : JC/MD
Sample : N4650-20DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ37DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

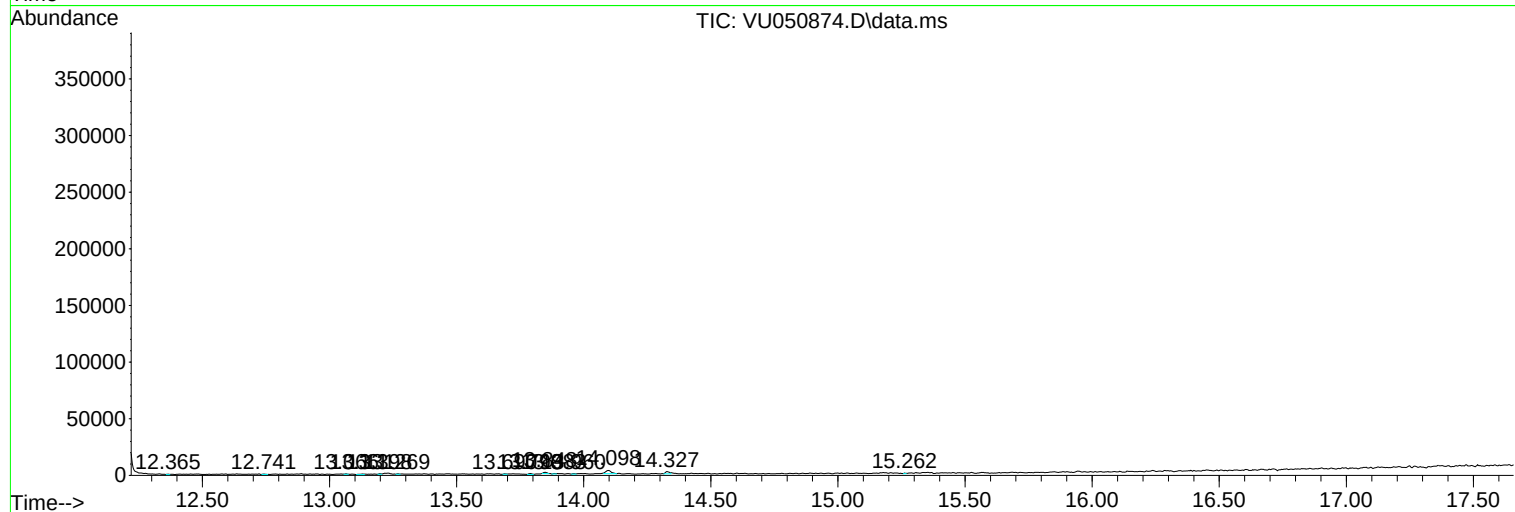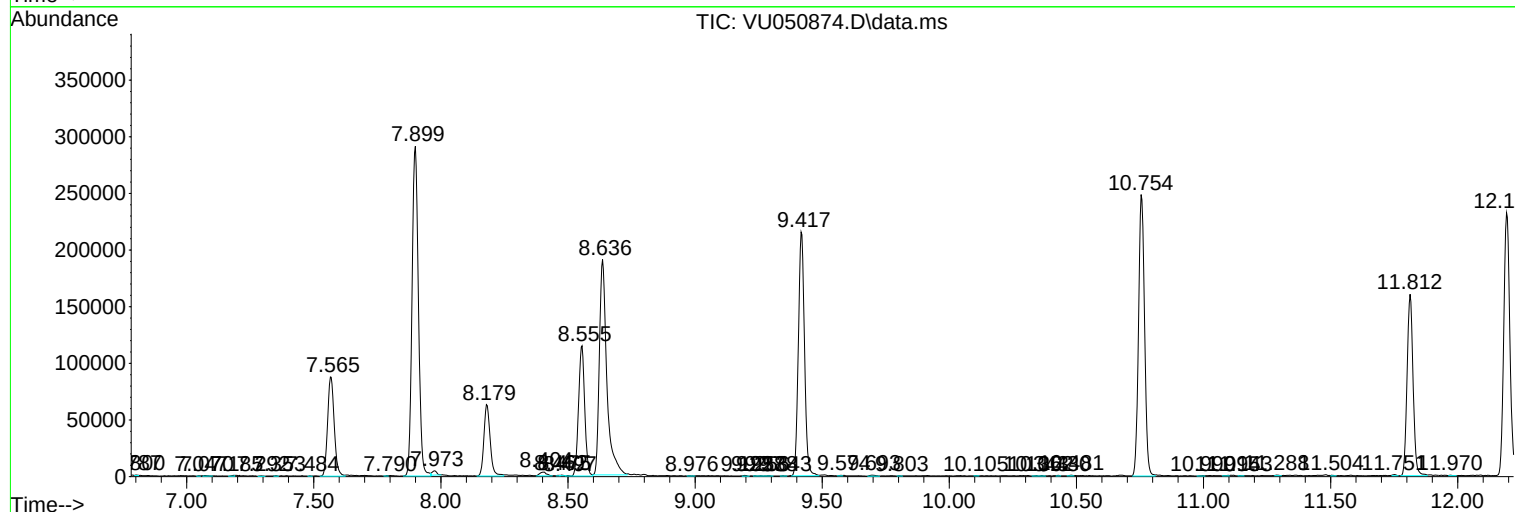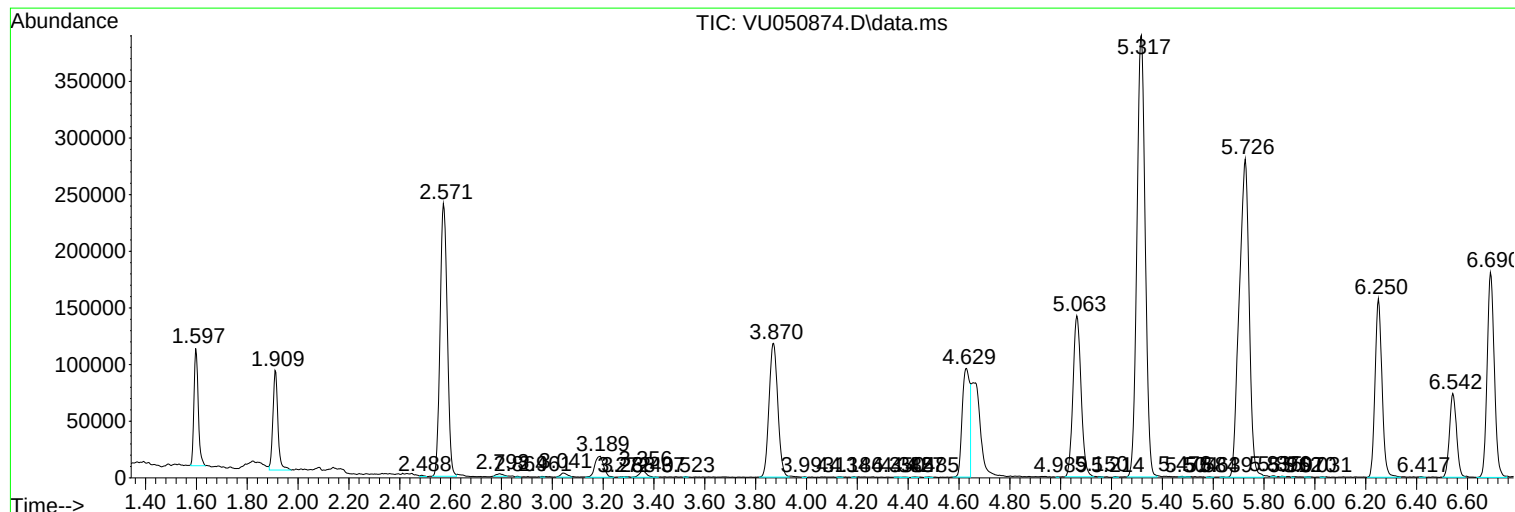

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092122\
Data File : VU050874.D
Acq On : 21 Sep 2022 11:36
Operator : JC/MD
Sample : N4650-20DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ37DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092122\
Data File : VU050874.D
Acq On : 21 Sep 2022 11:36
Operator : JC/MD
Sample : N4650-20DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXZ37DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc