

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092122\
 Data File : VU050881.D
 Acq On : 21 Sep 2022 17:36
 Operator : JC/MD
 Sample : VIBLK135
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK135

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VU050881.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.598	74	80	99	rVB	189064	232513	16.98%	2.199%
2	1.903	168	175	198	rVB2	143080	236753	17.29%	2.239%
3	2.562	369	380	397	rBV	281734	462449	33.77%	4.373%
4	2.942	496	498	500	rBV2	345	175	0.01%	0.002%
5	3.045	522	530	540	rVB5	3659	6804	0.50%	0.064%
6	3.090	542	544	547	rBV2	260	153	0.01%	0.001%
7	3.106	547	549	553	rVB	404	209	0.02%	0.002%
8	3.128	553	556	558	rVB	245	127	0.01%	0.001%
9	3.183	558	573	594	rBV2	34736	85665	6.26%	0.810%
10	3.353	618	626	637	rBV6	2655	5159	0.38%	0.049%
11	3.450	650	656	661	rBV2	390	474	0.03%	0.004%
12	3.623	705	710	712	rBV2	366	302	0.02%	0.003%
13	3.668	720	724	728	rBV	411	312	0.02%	0.003%
14	3.707	734	736	739	rVB	288	125	0.01%	0.001%
15	3.762	750	753	756	rBV	210	145	0.01%	0.001%
16	3.803	763	766	769	rBV2	282	182	0.01%	0.002%
17	3.868	769	786	803	rBV	67028	157417	11.49%	1.489%
18	4.006	828	829	830	rBV	127	38	0.00%	0.000%
19	4.077	848	851	853	rBV	250	178	0.01%	0.002%
20	4.138	868	870	875	rBV2	183	156	0.01%	0.001%
21	4.160	875	877	881	rVV2	153	94	0.01%	0.001%
22	4.183	881	884	886	rBV2	265	108	0.01%	0.001%
23	4.253	902	906	908	rBV	244	202	0.01%	0.002%
24	4.327	927	929	931	rBB2	88	32	0.00%	0.000%
25	4.347	931	935	936	rBV2	418	282	0.02%	0.003%
26	4.398	947	951	954	rVB2	290	191	0.01%	0.002%
27	4.417	954	957	960	rBV2	167	110	0.01%	0.001%
28	4.446	963	966	968	rBV	235	147	0.01%	0.001%
29	4.514	982	987	991	rBV2	327	353	0.03%	0.003%
30	4.623	1007	1021	1063	rBV2	216887	701610	51.23%	6.635%
31	5.061	1141	1157	1180	rBV	253645	556774	40.66%	5.265%
32	5.183	1191	1195	1199	rBV3	596	520	0.04%	0.005%
33	5.446	1275	1277	1280	rBV2	353	154	0.01%	0.001%
34	5.466	1280	1283	1284	rVV	137	63	0.00%	0.001%
35	5.488	1289	1290	1293	rBV	166	89	0.01%	0.001%
36	5.549	1306	1309	1312	rBV	181	105	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092122\
 Data File : VU050881.D
 Acq On : 21 Sep 2022 17:36
 Operator : JC/MD
 Sample : VIBLK135
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK135

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

37	5.639	1335	1337	1338	rBV	183	62	0.00%	0.001%
38	5.723	1339	1363	1389	rBV2	505972	1369453	100.00%	12.950%
39	6.099	1477	1480	1481	rBV	254	140	0.01%	0.001%
40	6.112	1481	1484	1487	rVV4	457	359	0.03%	0.003%
41	6.247	1511	1526	1547	rBV	397883	760409	55.53%	7.191%
42	6.533	1604	1615	1629	rVB6	11457	23836	1.74%	0.225%
43	6.597	1629	1635	1639	rVB2	473	485	0.04%	0.005%
44	6.623	1640	1643	1644	rBV	238	118	0.01%	0.001%
45	6.691	1649	1664	1686	rBV	328753	645421	47.13%	6.103%
46	6.880	1720	1723	1724	rBV	239	123	0.01%	0.001%
47	6.900	1727	1729	1730	rBV	352	139	0.01%	0.001%
48	6.913	1731	1733	1736	rVB	441	181	0.01%	0.002%
49	6.929	1736	1738	1739	rBV	191	91	0.01%	0.001%
50	6.964	1745	1749	1753	rBV3	852	844	0.06%	0.008%
51	7.109	1791	1794	1795	rBV2	176	109	0.01%	0.001%
52	7.189	1812	1819	1827	rBV6	1638	2613	0.19%	0.025%
53	7.244	1831	1836	1841	rVB2	501	494	0.04%	0.005%
54	7.321	1858	1860	1861	rBV2	120	54	0.00%	0.001%
55	7.334	1861	1864	1867	rVB2	314	198	0.01%	0.002%
56	7.350	1867	1869	1871	rVB	71	31	0.00%	0.000%
57	7.369	1871	1875	1879	rBV2	309	275	0.02%	0.003%
58	7.388	1879	1881	1883	rVB2	346	109	0.01%	0.001%
59	7.411	1883	1888	1893	rBV2	289	347	0.03%	0.003%
60	7.440	1894	1897	1902	rVV2	416	401	0.03%	0.004%
61	7.469	1902	1906	1908	rVV2	279	168	0.01%	0.002%
62	7.482	1908	1910	1912	rVB	216	88	0.01%	0.001%
63	7.565	1921	1936	1951	rBV	155793	272143	19.87%	2.573%
64	7.739	1987	1990	1993	rBV3	456	406	0.03%	0.004%
65	7.813	2010	2013	2016	rVB2	371	236	0.02%	0.002%
66	7.896	2025	2039	2056	rBV	533788	919286	67.13%	8.693%
67	8.179	2114	2127	2140	rBV	108528	182002	13.29%	1.721%
68	8.475	2215	2219	2222	rBV2	812	679	0.05%	0.006%
69	8.530	2233	2236	2237	rBV	339	173	0.01%	0.002%
70	8.556	2237	2244	2252	rVB4	2779	3902	0.28%	0.037%
71	8.633	2256	2268	2301	rBV2	495817	953347	69.62%	9.015%
72	8.832	2326	2330	2333	rBV2	621	433	0.03%	0.004%
73	9.076	2404	2406	2409	rBV2	299	149	0.01%	0.001%
74	9.157	2425	2431	2434	rBV2	473	467	0.03%	0.004%
75	9.321	2481	2482	2486	rVB	410	163	0.01%	0.002%
76	9.347	2486	2490	2492	rBV	321	278	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092122\
 Data File : VU050881.D
 Acq On : 21 Sep 2022 17:36
 Operator : JC/MD
 Sample : VIBLK135
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK135

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

77	9.417	2499	2512	2537	rBV	543103	897682	65.55%	8.489%
78	9.626	2574	2577	2580	rBV2	359	288	0.02%	0.003%
79	9.694	2592	2598	2607	rVB5	1060	1430	0.10%	0.014%
80	9.771	2619	2622	2625	rVB2	361	252	0.02%	0.002%
81	9.790	2625	2628	2630	rBV2	438	274	0.02%	0.003%
82	9.961	2678	2681	2684	rBV	256	166	0.01%	0.002%
83	9.977	2684	2686	2689	rVB2	421	190	0.01%	0.002%
84	9.996	2689	2692	2693	rBV	156	98	0.01%	0.001%
85	10.240	2764	2768	2771	rBV3	426	268	0.02%	0.003%
86	10.597	2877	2879	2882	rVB2	266	143	0.01%	0.001%
87	10.623	2884	2887	2892	rVV3	300	334	0.02%	0.003%
88	10.755	2915	2928	2948	rBV	474653	765786	55.92%	7.242%
89	10.961	2989	2992	2994	rBV	339	224	0.02%	0.002%
90	10.996	3000	3003	3004	rBV	250	153	0.01%	0.001%
91	11.083	3027	3030	3035	rBV2	516	596	0.04%	0.006%
92	11.141	3046	3048	3050	rBV	391	201	0.01%	0.002%
93	11.366	3115	3118	3121	rBV2	261	164	0.01%	0.002%
94	11.694	3217	3220	3223	rBV3	627	443	0.03%	0.004%
95	11.813	3244	3257	3272	rBV	378166	615064	44.91%	5.816%
96	12.054	3326	3332	3337	rBV2	696	836	0.06%	0.008%
97	12.192	3362	3375	3394	rBV	424161	690542	50.42%	6.530%
98	12.481	3457	3465	3474	rVB3	5591	8824	0.64%	0.083%
99	13.131	3664	3667	3669	rBV	811	574	0.04%	0.005%




Sum of corrected areas: 10574914

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092122\
Data File : VU050881.D
Acq On : 21 Sep 2022 17:36
Operator : JC/MD
Sample : VIBLK135
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK135

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

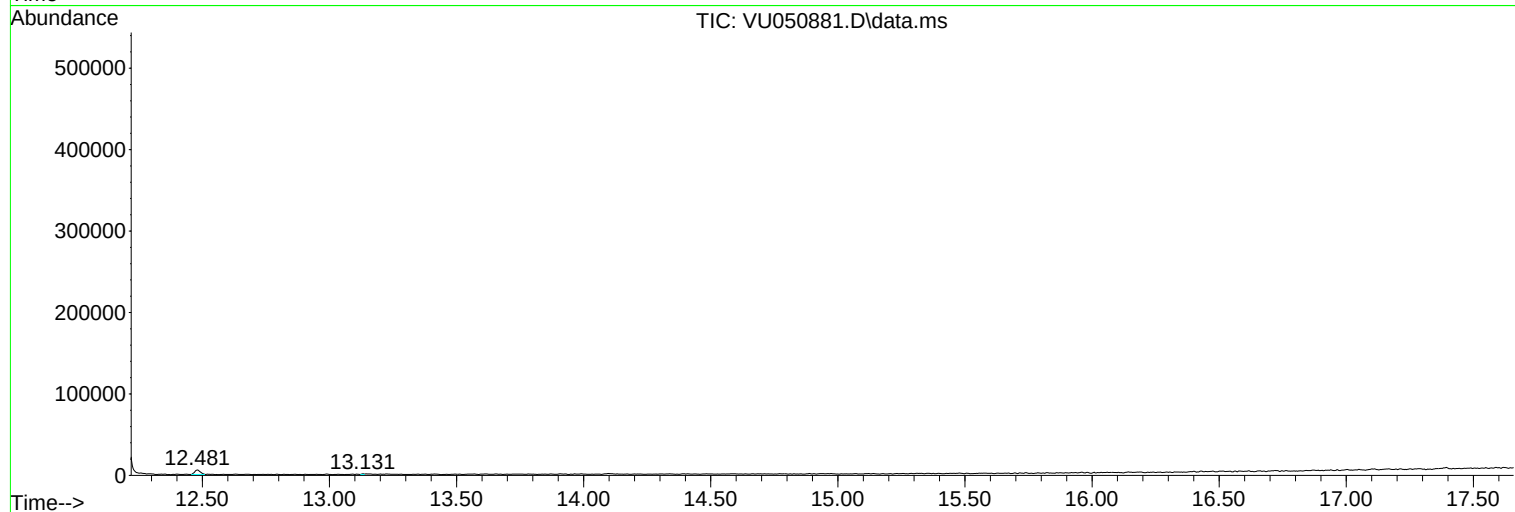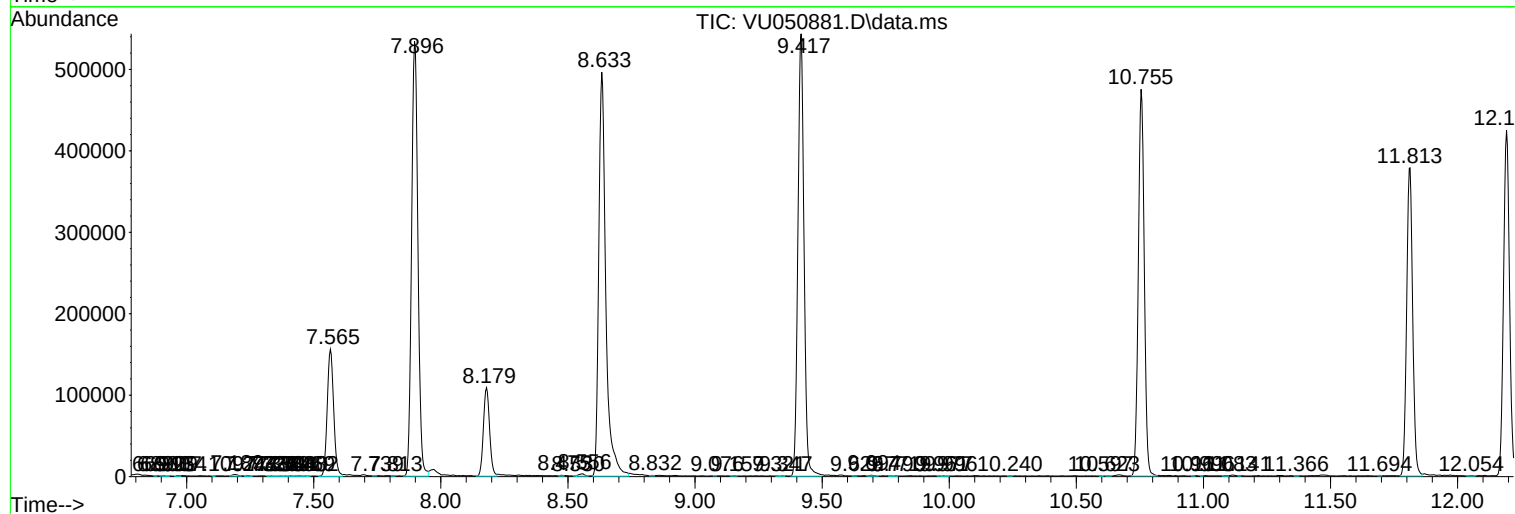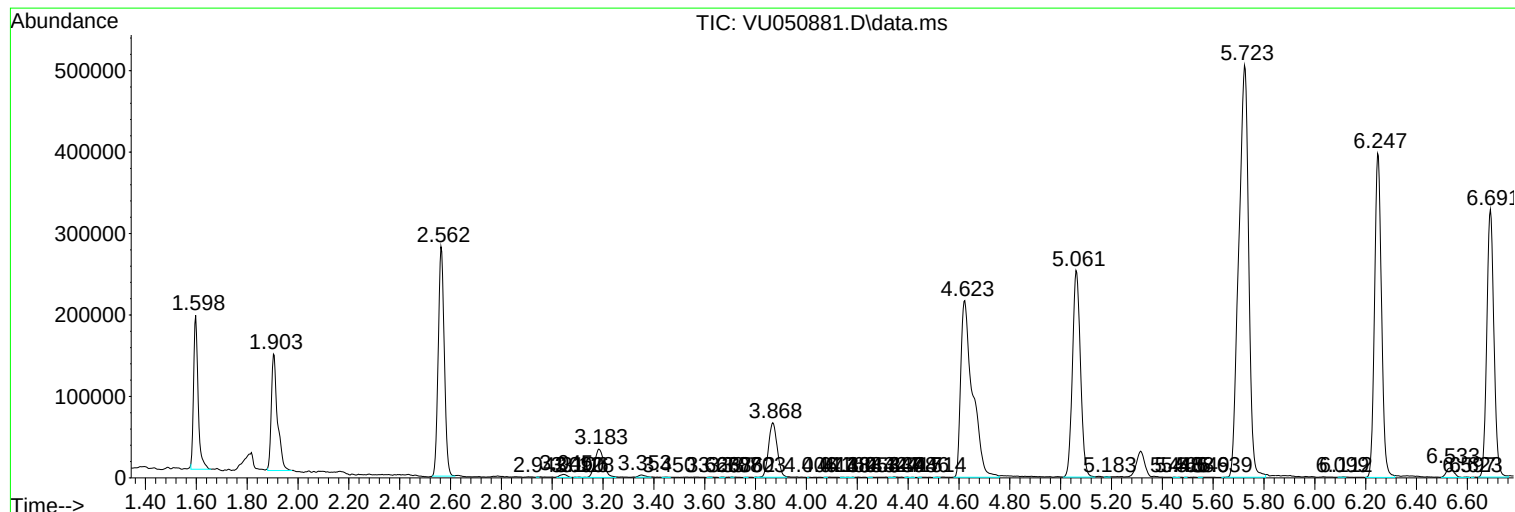

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092122\
Data File : VU050881.D
Acq On : 21 Sep 2022 17:36
Operator : JC/MD
Sample : VIBLK135
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK135

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092122\
Data File : VU050881.D
Acq On : 21 Sep 2022 17:36
Operator : JC/MD
Sample : VIBLK135
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK135

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc