

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092122\
 Data File : VU050884.D
 Acq On : 21 Sep 2022 18:47
 Operator : JC/MD
 Sample : VIBLK138
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK138

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VU050884.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	97	rVB	165234	204259	15.51%	2.035%
2	1.903	168	175	189	rVB	137523	188001	14.28%	1.873%
3	2.562	368	380	396	rBV	270502	458551	34.83%	4.569%
4	2.742	432	436	438	rBV4	485	345	0.03%	0.003%
5	2.790	442	451	461	rVB	9054	15244	1.16%	0.152%
6	2.842	461	467	469	rBV4	396	360	0.03%	0.004%
7	2.951	497	501	502	rBV2	582	435	0.03%	0.004%
8	3.047	522	531	541	rVB5	3167	5841	0.44%	0.058%
9	3.147	558	562	565	rBV	404	340	0.03%	0.003%
10	3.170	565	569	570	rBV2	739	536	0.04%	0.005%
11	3.353	617	626	638	rBV5	5487	10290	0.78%	0.103%
12	3.462	655	660	664	rBV2	381	436	0.03%	0.004%
13	3.584	691	698	701	rBV3	1226	1539	0.12%	0.015%
14	3.790	758	762	768	rVB2	499	583	0.04%	0.006%
15	3.854	777	782	783	rVV2	717	623	0.05%	0.006%
16	3.867	783	786	794	rVV2	1585	1943	0.15%	0.019%
17	3.996	822	826	832	rVB2	381	380	0.03%	0.004%
18	4.028	832	836	839	rBV2	473	389	0.03%	0.004%
19	4.186	881	885	892	rVV3	318	366	0.03%	0.004%
20	4.221	892	896	901	rVB3	421	437	0.03%	0.004%
21	4.263	904	909	913	rBV2	419	418	0.03%	0.004%
22	4.526	984	991	995	rBV2	506	751	0.06%	0.007%
23	4.623	1007	1021	1055	rBV	191084	507628	38.56%	5.058%
24	4.887	1101	1103	1107	rVB3	631	349	0.03%	0.003%
25	5.063	1141	1158	1184	rBV	238703	530689	40.31%	5.288%
26	5.314	1222	1236	1246	rVB8	4697	11363	0.86%	0.113%
27	5.385	1250	1258	1269	rVB8	3381	6400	0.49%	0.064%
28	5.526	1290	1302	1315	rBV6	1447	3185	0.24%	0.032%
29	5.723	1339	1363	1400	rBV2	481955	1316630	100.00%	13.120%
30	5.886	1411	1414	1422	rVB7	1321	1239	0.09%	0.012%
31	6.031	1455	1459	1463	rVB4	626	567	0.04%	0.006%
32	6.250	1513	1527	1546	rBV	377399	714296	54.25%	7.118%
33	6.542	1604	1618	1634	rVB2	93743	179972	13.67%	1.793%
34	6.690	1650	1664	1680	rBV	311594	606541	46.07%	6.044%
35	6.928	1732	1738	1741	rBV3	311	292	0.02%	0.003%
36	7.009	1760	1763	1768	rVB	339	276	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092122\
 Data File : VU050884.D
 Acq On : 21 Sep 2022 18:47
 Operator : JC/MD
 Sample : VIBLK138
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK138

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

37	7.057	1772	1778	1779	rBV3	494	408	0.03%	0.004%
38	7.108	1787	1794	1799	rBV3	1154	1256	0.10%	0.013%
39	7.192	1811	1820	1827	rBV8	2367	4235	0.32%	0.042%
40	7.237	1831	1834	1837	rVB3	474	347	0.03%	0.003%
41	7.317	1857	1859	1866	rVB2	641	552	0.04%	0.006%
42	7.353	1866	1870	1871	rBV	494	294	0.02%	0.003%
43	7.414	1883	1889	1893	rBV3	366	375	0.03%	0.004%
44	7.565	1921	1936	1951	rBV	148038	261851	19.89%	2.609%
45	7.681	1970	1972	1974	rBV3	629	337	0.03%	0.003%
46	7.796	1997	2008	2019	rVV4	4482	7950	0.60%	0.079%
47	7.899	2025	2040	2055	rBV	508677	881739	66.97%	8.786%
48	7.970	2056	2062	2075	rVB2	12807	23304	1.77%	0.232%
49	8.179	2114	2127	2146	rBV	100297	178892	13.59%	1.783%
50	8.314	2166	2169	2172	rBV3	460	361	0.03%	0.004%
51	8.404	2190	2197	2204	rVB6	2523	3854	0.29%	0.038%
52	8.475	2214	2219	2227	rVB4	815	1290	0.10%	0.013%
53	8.510	2227	2230	2232	rBV3	410	308	0.02%	0.003%
54	8.555	2235	2244	2253	rVB6	6494	10647	0.81%	0.106%
55	8.632	2256	2268	2300	rBV2	486142	953722	72.44%	9.503%
56	8.870	2339	2342	2344	rVB4	773	427	0.03%	0.004%
57	8.922	2351	2358	2365	rVV7	1415	2213	0.17%	0.022%
58	9.095	2409	2412	2414	rBV	525	347	0.03%	0.003%
59	9.131	2419	2423	2426	rVV	431	301	0.02%	0.003%
60	9.166	2428	2434	2436	rBV3	371	381	0.03%	0.004%
61	9.417	2499	2512	2545	rBV	492488	820632	62.33%	8.177%
62	9.571	2553	2560	2572	rVB2	7212	10258	0.78%	0.102%
63	9.693	2588	2598	2607	rBV2	6050	9703	0.74%	0.097%
64	9.777	2618	2624	2629	rBV3	364	412	0.03%	0.004%
65	10.108	2717	2727	2741	rBV7	7081	15103	1.15%	0.150%
66	10.298	2777	2786	2793	rVB5	862	1210	0.09%	0.012%
67	10.484	2836	2844	2858	rVB3	5458	8150	0.62%	0.081%
68	10.635	2888	2891	2894	rBV2	573	498	0.04%	0.005%
69	10.652	2894	2896	2898	rBV4	595	368	0.03%	0.004%
70	10.754	2915	2928	2944	rBV	450981	729031	55.37%	7.264%
71	10.963	2989	2993	2995	rVV	451	299	0.02%	0.003%
72	11.092	3024	3033	3048	rBV7	5380	9195	0.70%	0.092%
73	11.198	3064	3066	3071	rVB3	386	306	0.02%	0.003%
74	11.314	3099	3102	3105	rVB2	667	441	0.03%	0.004%
75	11.353	3110	3114	3117	rBV2	537	446	0.03%	0.004%
76	11.468	3141	3150	3164	rBV3	7174	11255	0.85%	0.112%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092122\
 Data File : VU050884.D
 Acq On : 21 Sep 2022 18:47
 Operator : JC/MD
 Sample : VIBLK138
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK138

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis

77	11.539	3169	3172	3177	rVB	356	345	0.03%	0.003%
78	11.565	3178	3180	3186	rBV2	640	582	0.04%	0.006%
79	11.616	3191	3196	3197	rBV2	341	293	0.02%	0.003%
80	11.693	3218	3220	3228	rVB4	550	469	0.04%	0.005%
81	11.748	3228	3237	3245	rBV4	9583	13666	1.04%	0.136%
82	11.812	3245	3257	3278	rBV	331288	545601	41.44%	5.437%
83	12.066	3329	3336	3343	rBV5	2925	4718	0.36%	0.047%
84	12.140	3356	3359	3361	rBV2	466	335	0.03%	0.003%
85	12.192	3362	3375	3401	rVV	383924	625769	47.53%	6.235%
86	12.459	3456	3458	3462	rVB3	597	352	0.03%	0.004%
87	12.597	3497	3501	3504	rBV2	413	316	0.02%	0.003%
88	12.655	3516	3519	3521	rBV	422	279	0.02%	0.003%
89	12.774	3553	3556	3562	rBV4	591	541	0.04%	0.005%
90	13.002	3619	3627	3638	rVB5	3094	5287	0.40%	0.053%
91	13.221	3687	3695	3706	rVB3	11235	16598	1.26%	0.165%
92	13.391	3745	3748	3752	rBV2	522	504	0.04%	0.005%
93	13.545	3793	3796	3800	rBV4	502	544	0.04%	0.005%
94	13.841	3879	3888	3901	rVB3	14343	22822	1.73%	0.227%
95	14.089	3956	3965	3981	rBV	24116	41347	3.14%	0.412%
96	14.330	4029	4040	4056	rBV2	16266	29369	2.23%	0.293%
97	14.394	4056	4060	4064	rVV3	416	391	0.03%	0.004%
98	14.770	4175	4177	4181	rVB2	602	316	0.02%	0.003%
99	14.838	4196	4198	4200	rBV2	571	325	0.02%	0.003%
100	16.069	4578	4581	4583	rBV2	917	698	0.05%	0.007%




Sum of corrected areas: 10035659

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092122\
Data File : VU050884.D
Acq On : 21 Sep 2022 18:47
Operator : JC/MD
Sample : VIBLK138
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK138

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

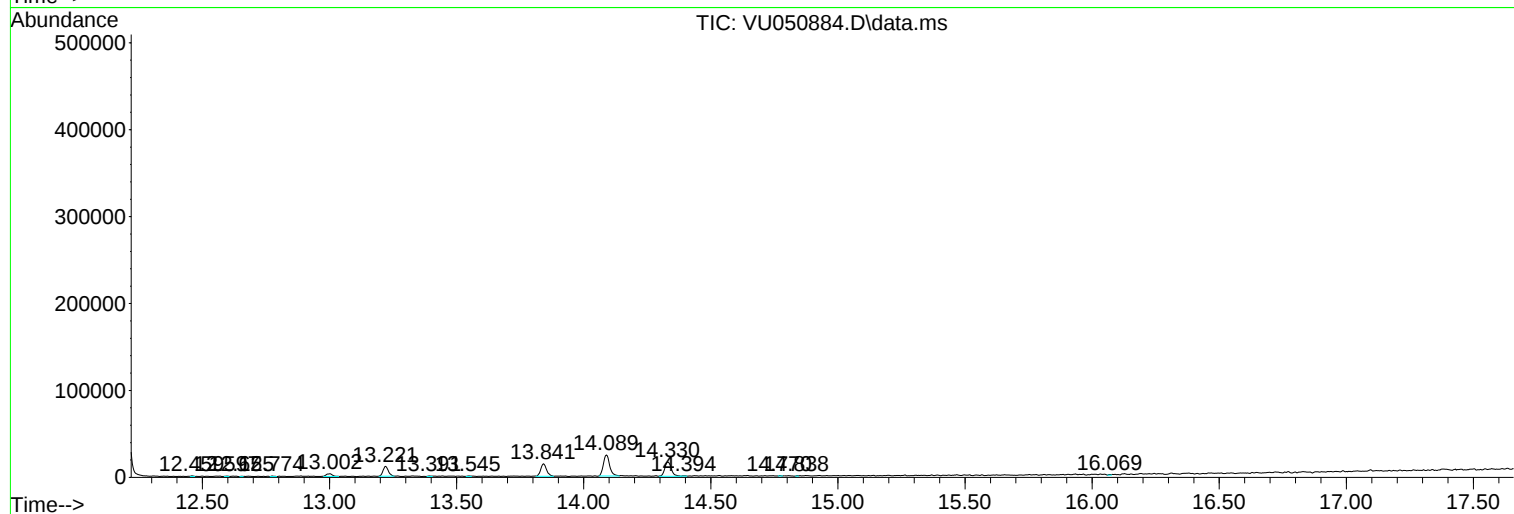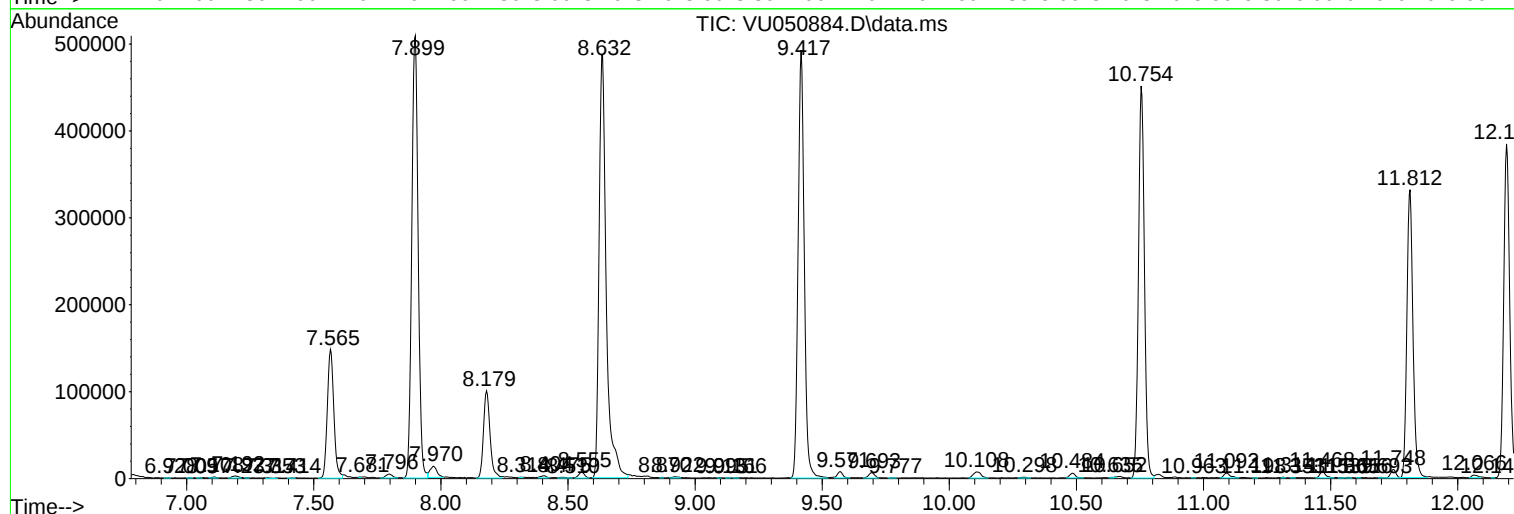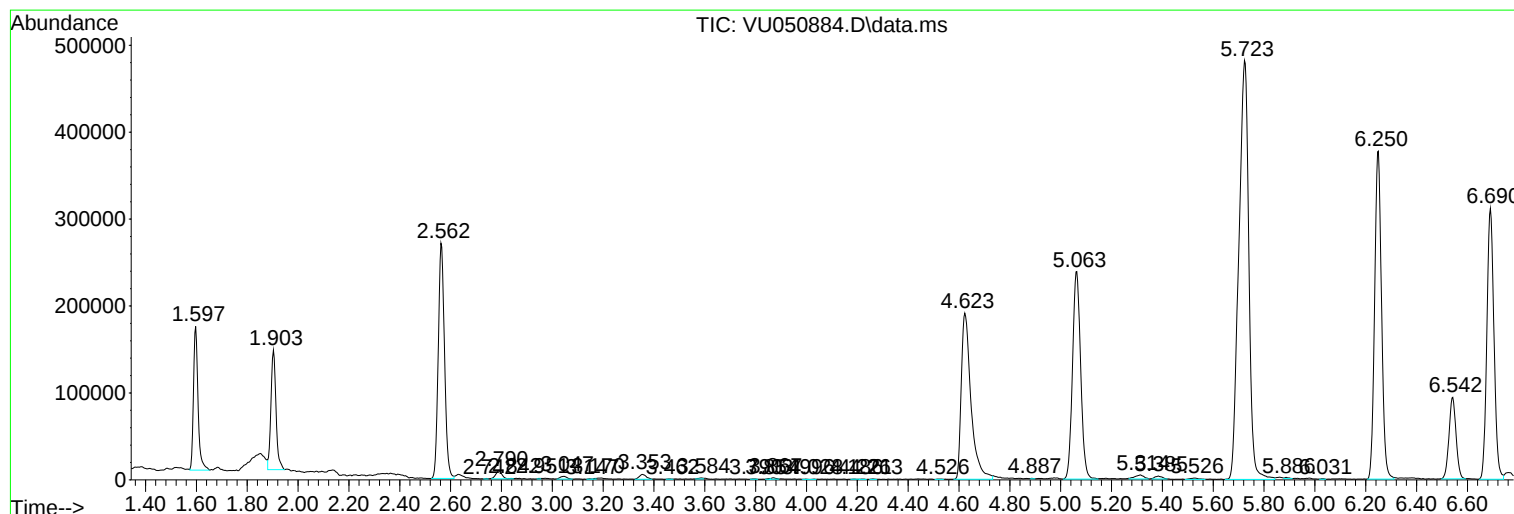

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092122\
Data File : VU050884.D
Acq On : 21 Sep 2022 18:47
Operator : JC/MD
Sample : VIBLK138
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK138

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092122\
Data File : VU050884.D
Acq On : 21 Sep 2022 18:47
Operator : JC/MD
Sample : VIBLK138
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK138

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc