


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092122\
 Data File : VU050871.D
 Acq On : 21 Sep 2022 09:03
 Operator : JC/MD
 Sample : BFB128
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB128

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092022WMA.M
 Title : VOC Analysis
 Last Update : Sat Sep 24 00:22:43 2022

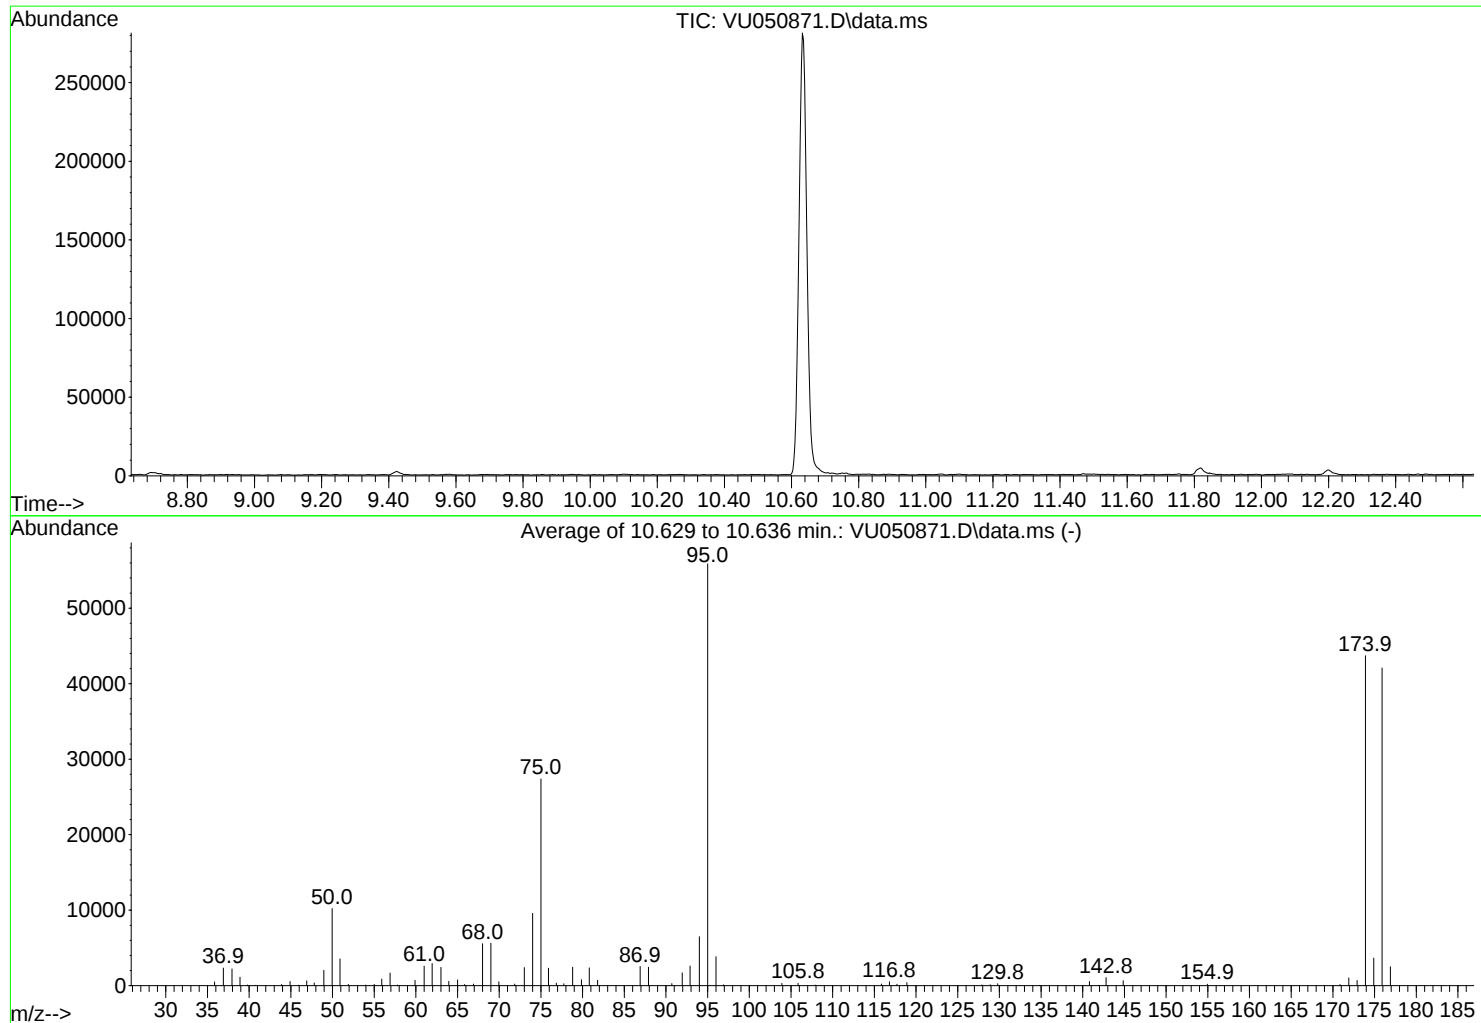

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.3	10225	PASS
75	95	30	80	49.0	27387	PASS
95	95	100	100	100.0	55877	PASS
96	95	5	9	6.9	3843	PASS
173	174	0.00	2	1.6	679	PASS
174	95	50	120	78.2	43696	PASS
175	174	5	9	8.3	3643	PASS
176	174	95	101	96.3	42067	PASS
177	176	5	9	5.9	2496	PASS

Scan 2878 (10.594 min): VU050871.D\data.ms
BFB128

m/z	Abundance
39.90	167.0
43.90	593.0

Instrument :
MSVOA_U
ClientSampleId :
BFB128

m/z	Abundance
35.80	523.0
36.90	2302.0
38.00	2231.0
38.90	1027.0
39.80	258.0
40.70	111.0
43.90	782.0
44.90	542.0
45.90	105.0
46.90	712.0
47.80	332.0
49.00	1995.0
50.00	9651.0
50.90	3492.0
51.90	106.0
55.00	167.0
55.90	780.0
56.90	1557.0
59.90	644.0
61.00	2448.0
61.90	2925.0
63.00	2384.0
64.00	512.0
65.00	766.0
66.00	112.0
66.90	177.0
68.00	5578.0
69.00	5586.0
70.00	502.0
71.90	198.0
73.00	2479.0
74.00	9393.0
75.00	26912.0
75.90	2281.0
76.80	324.0
77.80	305.0
78.80	2219.0
79.90	752.0
80.80	2291.0
81.80	531.0
86.90	2466.0
87.90	2245.0
90.70	294.0
91.90	1706.0
92.90	2670.0
94.00	6373.0
95.00	53408.0
96.00	3712.0
96.80	100.0
103.90	283.0
105.80	226.0
107.90	123.0
115.90	240.0
116.80	483.0
117.70	184.0
118.90	370.0
128.90	148.0
129.80	231.0
140.80	513.0
141.90	116.0
142.80	997.0
144.90	609.0
155.00	132.0
170.90	126.0
171.90	872.0
172.90	579.0
173.90	40608.0
174.90	3461.0
175.90	39264.0
176.90	2497.0

Instrument :
MSVOA_U
ClientSampleId :
BFB128

m/z	Abundance
35.80	496.0
36.90	2410.0
38.00	2319.0
38.90	1158.0
39.80	262.0
43.90	721.0
44.90	561.0
45.90	113.0
46.90	658.0
47.80	395.0
48.90	2085.0
49.90	10575.0
50.90	3686.0
51.90	185.0
54.00	107.0
55.00	169.0
55.90	917.0
56.90	1716.0
57.80	114.0
59.90	751.0
61.00	2644.0
62.00	2990.0
63.00	2522.0
63.90	613.0
65.00	776.0
65.80	154.0
66.90	217.0
68.00	5812.0
69.00	5772.0
69.90	518.0
71.80	221.0
73.00	2430.0
74.00	9827.0
75.00	28104.0
75.90	2356.0
76.80	366.0
77.80	251.0
78.80	2492.0
79.90	790.0
80.80	2440.0
81.80	728.0
86.90	2620.0
87.90	2509.0
90.70	282.0
91.90	1746.0
92.90	2712.0
94.00	6710.0
95.00	57656.0
96.00	4011.0
96.90	119.0
103.90	309.0
105.90	332.0
107.90	110.0
115.90	211.0
116.80	507.0
117.70	211.0
118.90	417.0
127.90	151.0
128.90	154.0
129.80	260.0
134.80	100.0
140.80	532.0
142.80	1117.0
144.90	681.0
154.90	191.0
170.80	152.0
171.90	1056.0
172.90	706.0
173.90	44992.0
174.90	3811.0
175.90	43216.0
176.90	2518.0

Instrument :
MSVOA_U
ClientSampleId :
BFB128

m/z	Abundance
35.90	425.0
36.90	2290.0
37.90	2071.0
38.90	1168.0
39.80	238.0
43.90	752.0
44.90	524.0
46.90	566.0
47.80	382.0
48.90	2044.0
49.90	10450.0
50.90	3461.0
51.90	210.0
53.90	136.0
55.00	171.0
55.90	936.0
56.90	1739.0
57.80	122.0
59.90	713.0
61.00	2672.0
62.00	2832.0
63.00	2356.0
63.90	572.0
65.00	727.0
65.80	172.0
66.90	220.0
68.00	5247.0
69.00	5468.0
69.90	525.0
71.90	215.0
73.00	2289.0
74.00	9513.0
75.00	27144.0
75.90	2278.0
76.90	355.0
77.70	201.0
78.80	2582.0
79.80	832.0
80.80	2317.0
81.80	834.0
86.90	2532.0
87.90	2536.0
90.70	262.0
92.00	1663.0
92.90	2455.0
94.00	6376.0
95.00	56568.0
96.00	3806.0
97.00	133.0
103.90	281.0
105.80	409.0
115.80	189.0
116.80	538.0
117.70	196.0
118.90	443.0
127.90	197.0
128.90	102.0
129.80	272.0
140.80	601.0
142.80	1093.0
144.80	680.0
154.90	231.0
170.90	171.0
171.90	1153.0
172.90	752.0
173.90	45488.0
174.90	3656.0
175.90	43720.0
176.90	2473.0

Instrument :
MSVOA_U
ClientSampleId :
BFB128