

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
 Data File : VU051017.D
 Acq On : 30 Sep 2022 06:37
 Operator : JC/MD
 Sample : N4859-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E10017

Quant Time: Sep 30 07:57:36 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Sep 30 02:29:24 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	278485	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	286679	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152	120845	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	122539	43.418	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	86.840%	
7) Chloroethane-d5	1.906	69	151679	57.855	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	115.720%	
11) 1,1-Dichloroethene-d2	2.565	63	143972	34.534	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	69.060%	
21) 2-Butanone-d5	4.626	46	191128	104.413	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	104.410%	
24) Chloroform-d	5.060	84	220958	48.594	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	97.180%	
26) 1,2-Dichloroethane-d4	5.700	65	142373	50.586	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	101.180%	
32) Benzene-d6	5.726	84	431489	51.398	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	102.800%	
36) 1,2-Dichloropropane-d6	6.690	67	146914	53.931	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	107.860%	
41) Toluene-d8	7.896	98	344604	44.429	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	88.860%	
43) trans-1,3-Dichloroprop...	8.179	79	57103	43.948	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	87.900%	
47) 2-Hexanone-d5	8.632	63	99754	90.689	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	90.690%	
56) 1,1,2,2-Tetrachloroeth...	10.755	84	283526	59.553	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	119.100%	
66) 1,2-Dichlorobenzene-d4	12.192	152	141522	54.820	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	109.640%	
Target Compounds						
13) Acetone	2.639	43	4332	2.964	ug/L	Qvalue 87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
Data File : VU051017.D
Acq On : 30 Sep 2022 06:37
Operator : JC/MD
Sample : N4859-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E10017

Quant Time: Sep 30 07:57:36 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Sep 30 02:29:24 2022
Response via : Initial Calibration

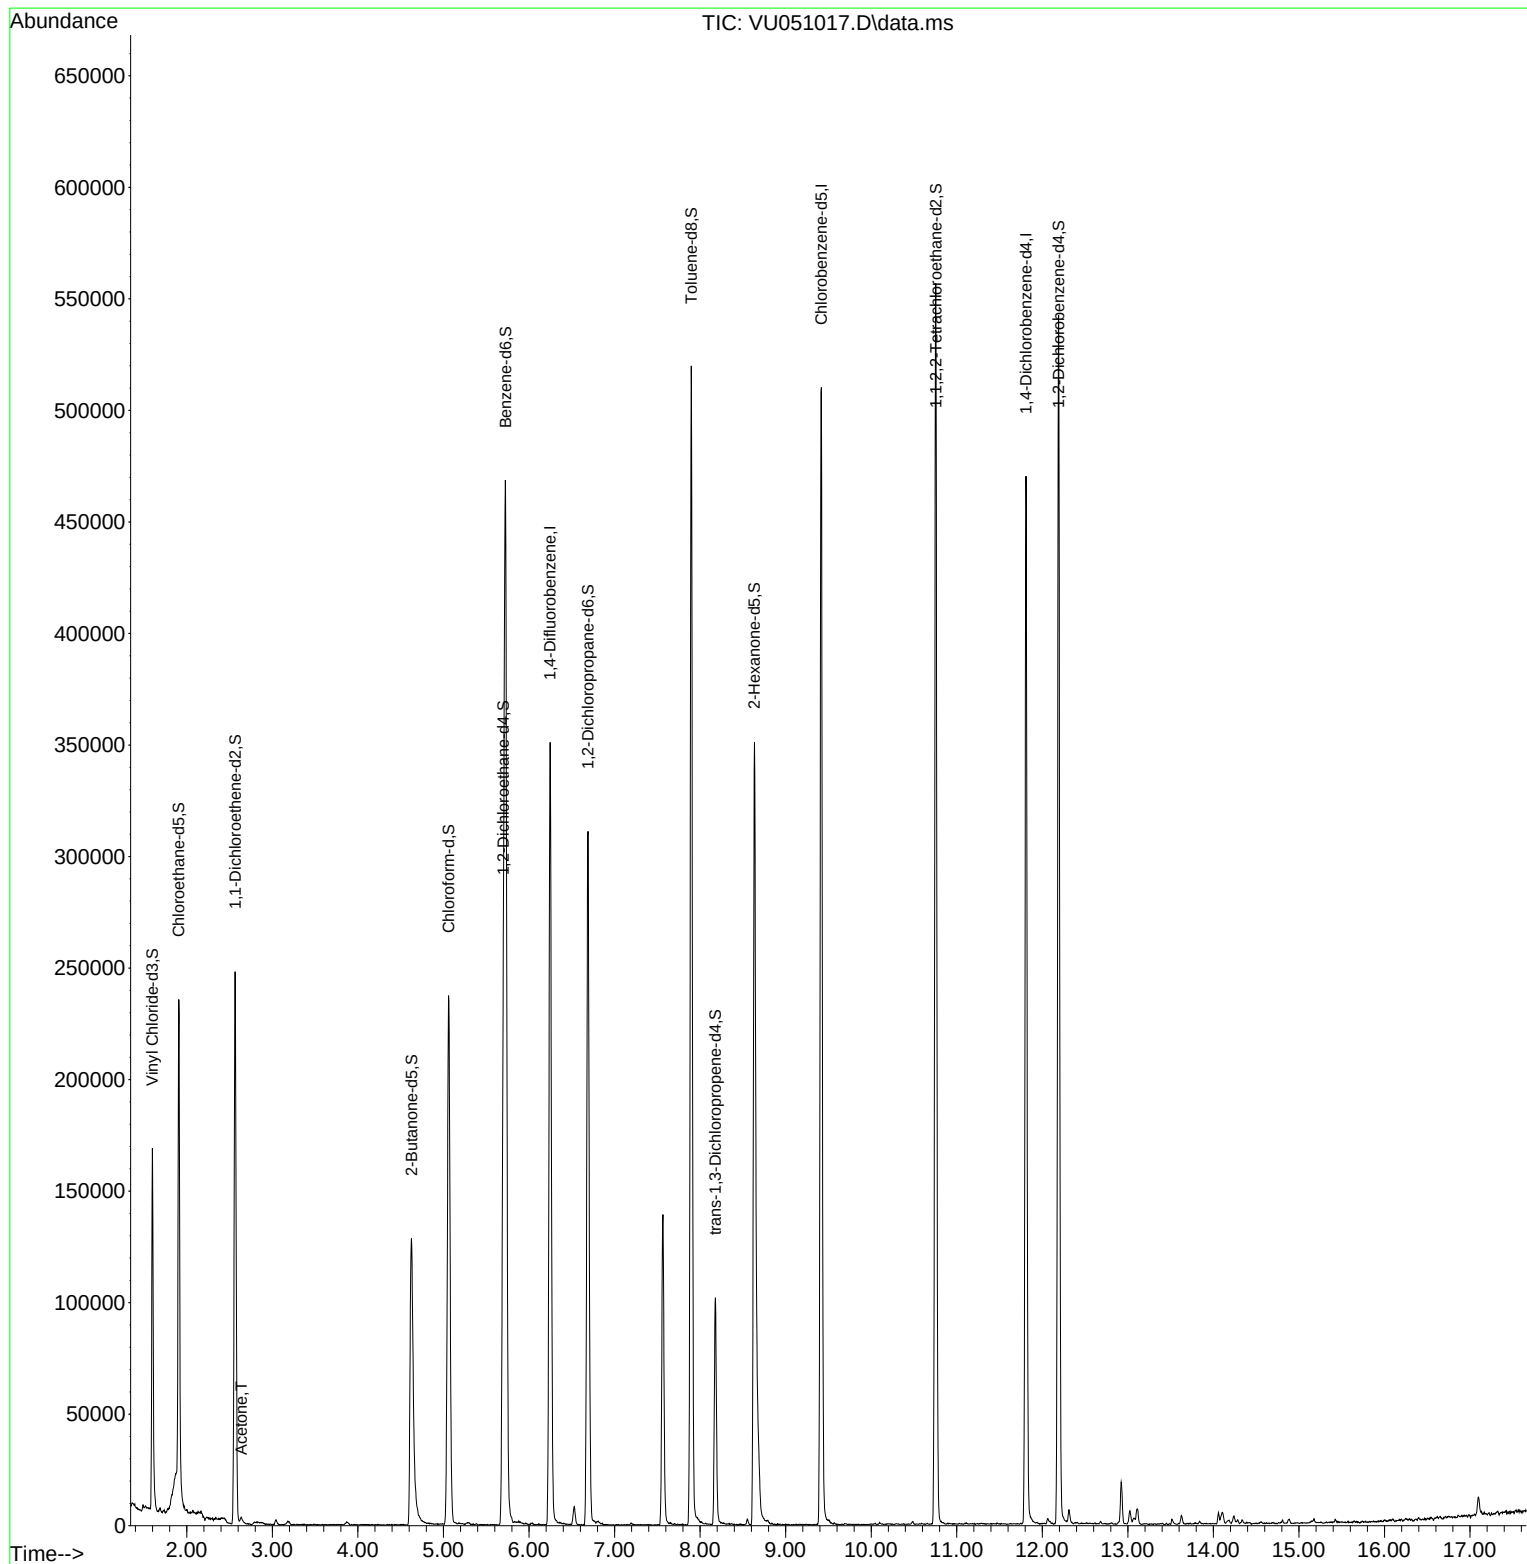

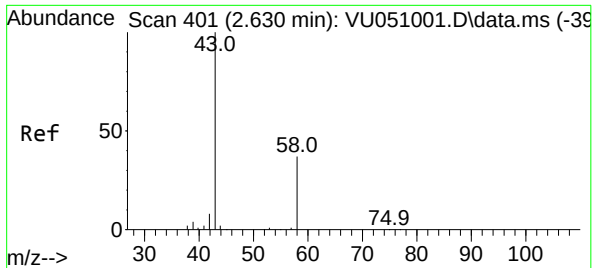

#13
 Acetone
 Concen: 2.964 ug/L
 RT: 2.639 min Scan# 40
 Delta R.T. 0.010 min
 Lab File: VU051017.D
 Acq: 30 Sep 2022 06:37

Instrument :
 MSVOA_U
 ClientSampleId :
 E10017

Tgt Ion: 43 Resp: 4332
 Ion Ratio Lower Upper
 43 100
 58 28.8 0.0 73.6

