

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
 Data File : VU050986.D
 Acq On : 29 Sep 2022 18:06
 Operator : JC/MD
 Sample : N4854-01DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J01DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M

Title : VOC Analysis

Signal : TIC: VU050986.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	100	rVB	204152	243192	16.27%	1.932%
2	1.912	170	178	200	rBV	217980	292909	19.60%	2.327%
3	2.501	357	361	363	rBV4	499	400	0.03%	0.003%
4	2.565	368	381	401	rBV	305807	495744	33.17%	3.939%
5	2.736	431	434	439	rBV3	461	489	0.03%	0.004%
6	2.793	442	452	463	rVB2	2400	3824	0.26%	0.030%
7	2.835	463	465	471	rBV2	404	356	0.02%	0.003%
8	3.044	519	530	546	rVB2	13188	23782	1.59%	0.189%
9	3.182	556	573	591	rVB2	11013	26461	1.77%	0.210%
10	3.279	600	603	607	rBV	397	272	0.02%	0.002%
11	3.356	620	627	629	rBV2	1523	1446	0.10%	0.011%
12	3.498	668	671	676	rVB2	292	235	0.02%	0.002%
13	3.790	759	762	765	rVB2	375	224	0.01%	0.002%
14	3.826	769	773	782	rBV	349	422	0.03%	0.003%
15	3.861	782	784	789	rVB	337	287	0.02%	0.002%
16	4.086	850	854	856	rBV2	439	373	0.02%	0.003%
17	4.099	856	858	861	rVV	429	271	0.02%	0.002%
18	4.121	861	865	867	rVV2	441	322	0.02%	0.003%
19	4.134	867	869	871	rVV	482	267	0.02%	0.002%
20	4.166	874	879	882	rVV2	403	408	0.03%	0.003%
21	4.189	882	886	892	rVV2	344	493	0.03%	0.004%
22	4.221	892	896	899	rVV2	384	395	0.03%	0.003%
23	4.256	904	907	910	rVV2	425	248	0.02%	0.002%
24	4.408	951	954	962	rVB2	364	368	0.02%	0.003%
25	4.443	962	965	967	rBV	359	269	0.02%	0.002%
26	4.465	969	972	977	rVB	409	347	0.02%	0.003%
27	4.514	981	987	989	rBV2	272	312	0.02%	0.002%
28	4.633	1011	1024	1062	rBV	140233	419073	28.04%	3.329%
29	4.896	1103	1106	1110	rBV2	640	412	0.03%	0.003%
30	4.938	1115	1119	1122	rBV2	369	345	0.02%	0.003%
31	5.060	1141	1157	1179	rVV	271726	594567	39.79%	4.724%
32	5.182	1193	1195	1201	rVB4	816	692	0.05%	0.005%
33	5.276	1221	1224	1226	rBV3	702	520	0.03%	0.004%
34	5.295	1228	1230	1238	rVB6	936	1140	0.08%	0.009%
35	5.379	1248	1256	1263	rVB5	900	1549	0.10%	0.012%
36	5.562	1308	1313	1317	rBV	220	229	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
 Data File : VU050986.D
 Acq On : 29 Sep 2022 18:06
 Operator : JC/MD
 Sample : N4854-01DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J01DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	5.607	1324	1327	1330	rVB2	334	222	0.01%	0.002%
38	5.629	1330	1334	1338	rBV2	288	300	0.02%	0.002%
39	5.723	1342	1363	1394	rBV2	553329	1494332	100.00%	11.872%
40	6.247	1512	1526	1545	rBV	436335	818709	54.79%	6.504%
41	6.539	1602	1617	1633	rBV4	82893	166337	11.13%	1.321%
42	6.690	1648	1664	1680	rBV	346742	674075	45.11%	5.355%
43	6.848	1711	1713	1719	rVB5	477	357	0.02%	0.003%
44	6.999	1757	1760	1766	rBV2	245	225	0.02%	0.002%
45	7.186	1813	1818	1820	rBV3	600	507	0.03%	0.004%
46	7.276	1842	1846	1853	rBV3	520	773	0.05%	0.006%
47	7.475	1905	1908	1912	rVB2	433	328	0.02%	0.003%
48	7.565	1923	1936	1957	rBV	182795	323989	21.68%	2.574%
49	7.639	1957	1959	1968	rVB4	1421	1255	0.08%	0.010%
50	7.751	1990	1994	1997	rBV3	281	225	0.02%	0.002%
51	7.771	1997	2000	2002	rBV2	376	232	0.02%	0.002%
52	7.787	2002	2005	2007	rBV	1080	680	0.05%	0.005%
53	7.845	2020	2023	2026	rBV2	401	306	0.02%	0.002%
54	7.896	2026	2039	2060	rBV	725215	1244008	83.25%	9.883%
55	8.179	2114	2127	2143	rBV	129538	226415	15.15%	1.799%
56	8.317	2167	2170	2172	rBV2	450	245	0.02%	0.002%
57	8.481	2216	2221	2223	rVB3	483	386	0.03%	0.003%
58	8.552	2230	2243	2257	rBV	468703	782728	52.38%	6.219%
59	8.636	2258	2269	2302	rVB3	413071	906022	60.63%	7.198%
60	8.883	2343	2346	2348	rBV2	506	280	0.02%	0.002%
61	8.928	2354	2360	2364	rVV5	966	994	0.07%	0.008%
62	8.960	2368	2370	2376	rVB2	357	313	0.02%	0.002%
63	8.996	2376	2381	2383	rBV2	378	319	0.02%	0.003%
64	9.192	2439	2442	2447	rBV2	260	227	0.02%	0.002%
65	9.292	2467	2473	2476	rBV	298	382	0.03%	0.003%
66	9.417	2499	2512	2546	rBV	657489	1104020	73.88%	8.771%
67	9.568	2556	2559	2571	rVB5	1745	2638	0.18%	0.021%
68	9.642	2577	2582	2584	rBV2	353	289	0.02%	0.002%
69	9.684	2589	2595	2596	rVV3	1213	880	0.06%	0.007%
70	9.697	2596	2599	2606	rVV3	1920	2111	0.14%	0.017%
71	9.732	2608	2610	2615	rVB3	271	223	0.01%	0.002%
72	9.783	2623	2626	2631	rBV2	322	344	0.02%	0.003%
73	10.012	2694	2697	2701	rBV	377	271	0.02%	0.002%
74	10.108	2718	2727	2740	rVB7	2518	5608	0.38%	0.045%
75	10.484	2838	2844	2847	rBV4	1118	1302	0.09%	0.010%
76	10.703	2909	2912	2915	rBV	338	219	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
 Data File : VU050986.D
 Acq On : 29 Sep 2022 18:06
 Operator : JC/MD
 Sample : N4854-01DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J01DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	10.755	2915	2928	2945	rBV	518776	843040	56.42%	6.698%
78	10.918	2977	2979	2986	rVB	433	378	0.03%	0.003%
79	10.954	2987	2990	2993	rBV2	336	283	0.02%	0.002%
80	10.989	2999	3001	3004	rBV2	438	303	0.02%	0.002%
81	11.050	3017	3020	3026	rVB2	313	302	0.02%	0.002%
82	11.082	3026	3030	3031	rBV	1410	892	0.06%	0.007%
83	11.472	3147	3151	3158	rVB5	1786	2097	0.14%	0.017%
84	11.545	3168	3174	3177	rBV	371	415	0.03%	0.003%
85	11.745	3228	3236	3244	rVB5	3046	4555	0.30%	0.036%
86	11.809	3244	3256	3275	rBV	537036	864621	57.86%	6.869%
87	11.960	3300	3303	3305	rBV2	366	226	0.02%	0.002%
88	12.192	3361	3375	3397	rBV	582382	952646	63.75%	7.568%
89	12.648	3512	3517	3521	rBV2	822	842	0.06%	0.007%
90	12.889	3589	3592	3594	rBV3	466	304	0.02%	0.002%
91	13.147	3669	3672	3676	rVB2	343	263	0.02%	0.002%
92	13.224	3688	3696	3709	rVB5	3806	6936	0.46%	0.055%
93	13.536	3790	3793	3797	rVB3	788	571	0.04%	0.005%
94	13.561	3799	3801	3806	rVB3	531	453	0.03%	0.004%
95	13.844	3881	3889	3898	rBV4	4982	7478	0.50%	0.059%
96	13.944	3917	3920	3927	rBV3	523	548	0.04%	0.004%
97	14.092	3957	3966	3981	rBV3	7610	14013	0.94%	0.111%
98	14.333	4033	4041	4052	rBV3	5998	8771	0.59%	0.070%
99	14.754	4170	4172	4177	rBV3	415	332	0.02%	0.003%
100	15.516	4405	4409	4414	rVB3	1026	1018	0.07%	0.008%




Sum of corrected areas: 12587006

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
Data File : VU050986.D
Acq On : 29 Sep 2022 18:06
Operator : JC/MD
Sample : N4854-01DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J01DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

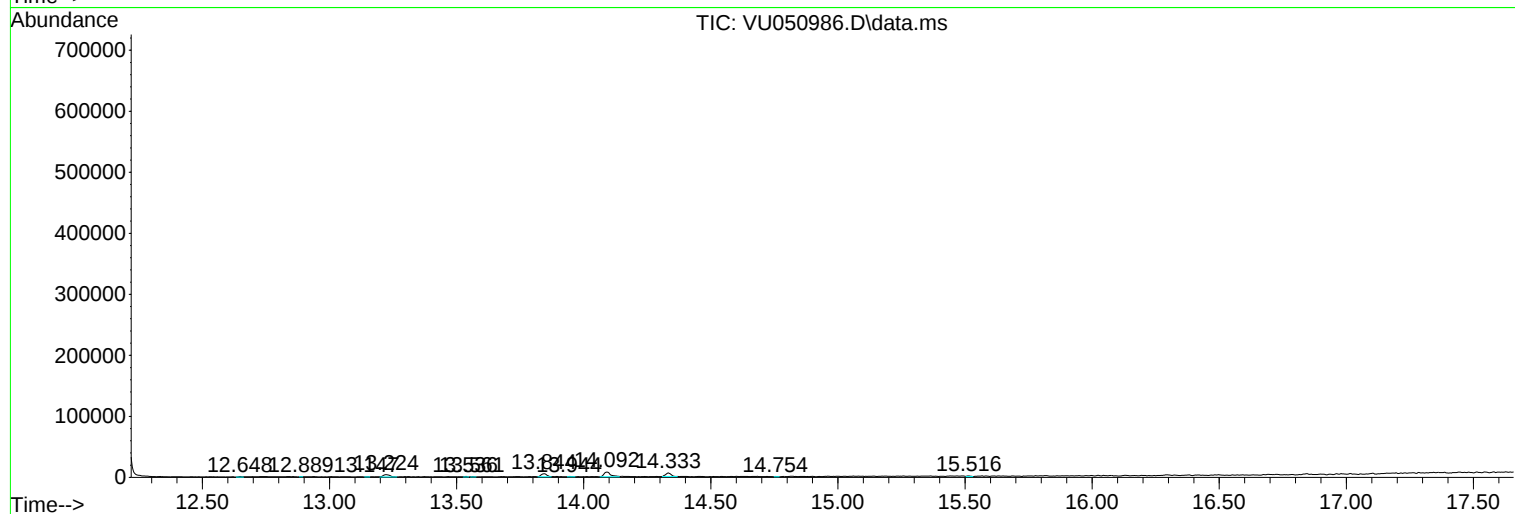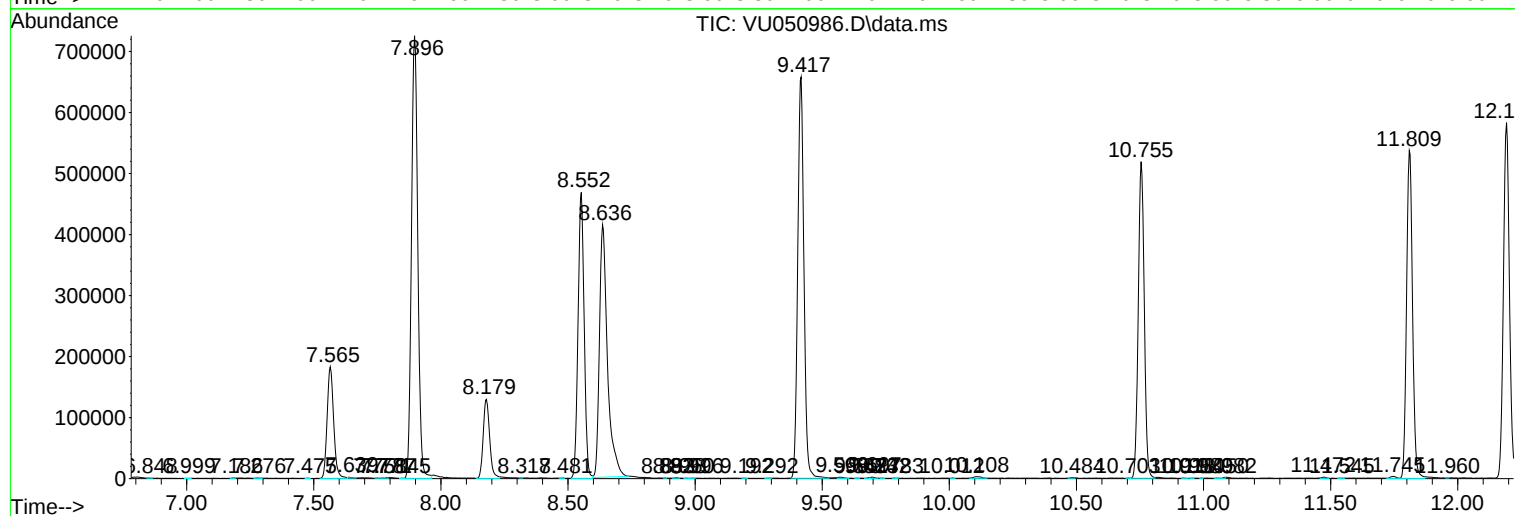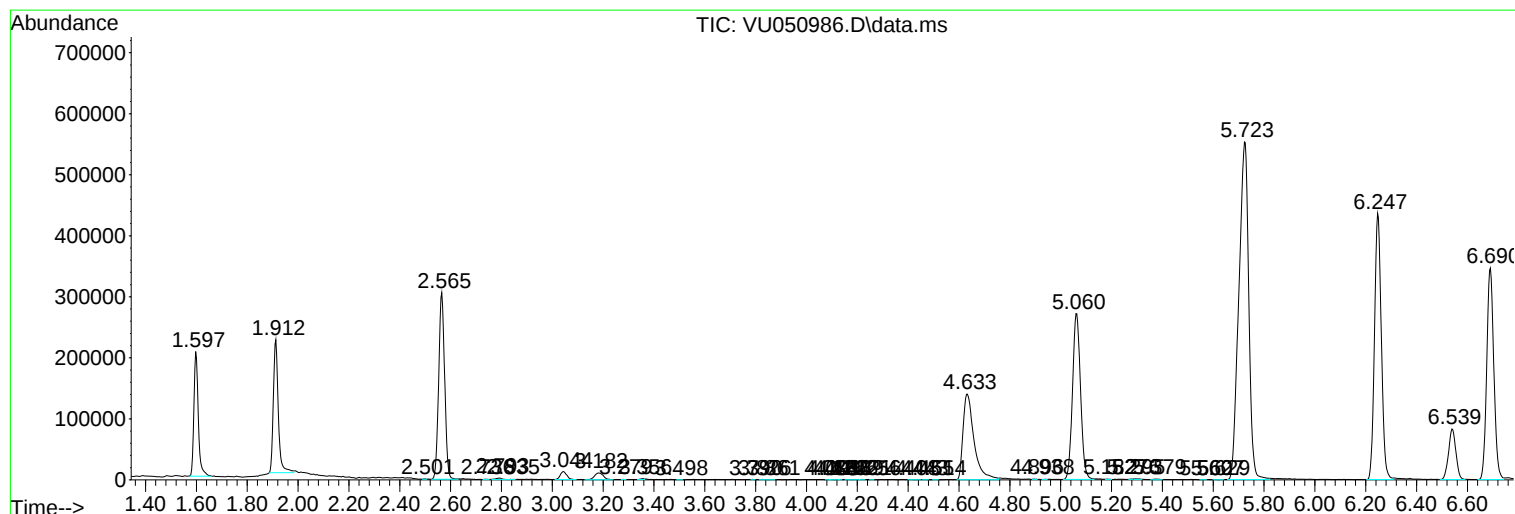

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
Data File : VU050986.D
Acq On : 29 Sep 2022 18:06
Operator : JC/MD
Sample : N4854-01DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J01DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
Data File : VU050986.D
Acq On : 29 Sep 2022 18:06
Operator : JC/MD
Sample : N4854-01DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J01DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------