

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
 Data File : VU050987.D
 Acq On : 29 Sep 2022 18:30
 Operator : JC/MD
 Sample : N4854-02DL 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J04DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M

Title : VOC Analysis

Signal : TIC: VU050987.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.598	73	80	98	rBV	196152	232902	15.91%	1.959%
2	1.906	169	176	192	rVB	200971	268850	18.37%	2.262%
3	2.565	368	381	397	rBV	297270	483765	33.05%	4.070%
4	2.790	442	451	457	rBV2	1731	2873	0.20%	0.024%
5	2.916	488	490	494	rVB2	477	324	0.02%	0.003%
6	3.044	518	530	547	rVB2	14265	28019	1.91%	0.236%
7	3.109	547	550	554	rBV	460	401	0.03%	0.003%
8	3.186	561	574	589	rBV	7603	15788	1.08%	0.133%
9	3.417	639	646	647	rBV2	260	268	0.02%	0.002%
10	3.459	657	659	665	rVB2	374	311	0.02%	0.003%
11	3.575	688	695	697	rBV2	279	290	0.02%	0.002%
12	3.633	709	713	718	rVB	260	236	0.02%	0.002%
13	3.665	719	723	729	rBV2	217	299	0.02%	0.003%
14	3.778	753	758	763	rBV2	398	462	0.03%	0.004%
15	3.810	763	768	774	rBV2	239	306	0.02%	0.003%
16	4.131	864	868	872	rBV2	272	275	0.02%	0.002%
17	4.186	881	885	892	rVB2	420	515	0.04%	0.004%
18	4.237	892	901	907	rVB2	496	790	0.05%	0.007%
19	4.279	910	914	919	rBV2	175	238	0.02%	0.002%
20	4.488	975	979	982	rVB3	382	337	0.02%	0.003%
21	4.623	1008	1021	1062	rBV	142893	392496	26.81%	3.302%
22	4.874	1097	1099	1105	rVB3	551	372	0.03%	0.003%
23	5.060	1140	1157	1183	rBV	265309	585123	39.97%	4.923%
24	5.253	1211	1217	1220	rBV3	760	849	0.06%	0.007%
25	5.305	1231	1233	1238	rVB5	862	553	0.04%	0.005%
26	5.385	1255	1258	1262	rVB3	559	494	0.03%	0.004%
27	5.520	1297	1300	1304	rBV3	448	418	0.03%	0.004%
28	5.578	1315	1318	1326	rVB2	457	464	0.03%	0.004%
29	5.723	1341	1363	1394	rBV2	542622	1463779	100.00%	12.315%
30	5.858	1403	1405	1409	rVB3	653	372	0.03%	0.003%
31	6.038	1458	1461	1464	rBV3	361	265	0.02%	0.002%
32	6.121	1483	1487	1490	rVB4	581	499	0.03%	0.004%
33	6.247	1512	1526	1547	rBV	426776	813622	55.58%	6.845%
34	6.340	1553	1555	1558	rVB2	1042	424	0.03%	0.004%
35	6.372	1558	1565	1569	rBV6	971	1541	0.11%	0.013%
36	6.530	1603	1614	1628	rVB3	15979	33151	2.26%	0.279%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
 Data File : VU050987.D
 Acq On : 29 Sep 2022 18:30
 Operator : JC/MD
 Sample : N4854-02DL 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J04DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	6.691	1649	1664	1685	rBV	359161	702438	47.99%	5.909%
38	6.938	1737	1741	1742	rBV	394	253	0.02%	0.002%
39	7.109	1787	1794	1799	rBV3	683	865	0.06%	0.007%
40	7.192	1816	1820	1823	rBV3	914	854	0.06%	0.007%
41	7.433	1888	1895	1899	rBV2	585	777	0.05%	0.007%
42	7.565	1923	1936	1956	rBV	179154	317001	21.66%	2.667%
43	7.797	2000	2008	2014	rBV6	1991	2550	0.17%	0.021%
44	7.896	2022	2039	2055	rBV	641278	1115212	76.19%	9.382%
45	8.076	2093	2095	2099	rVB3	580	377	0.03%	0.003%
46	8.179	2113	2127	2148	rBV	126858	221319	15.12%	1.862%
47	8.337	2173	2176	2180	rVB3	485	259	0.02%	0.002%
48	8.398	2191	2195	2203	rBV4	1420	1413	0.10%	0.012%
49	8.552	2230	2243	2256	rBV	339839	561268	38.34%	4.722%
50	8.636	2257	2269	2296	rVV2	398976	829549	56.67%	6.979%
51	8.871	2339	2342	2345	rBV2	344	255	0.02%	0.002%
52	8.919	2352	2357	2358	rBV3	656	548	0.04%	0.005%
53	9.137	2422	2425	2429	rVB2	501	323	0.02%	0.003%
54	9.179	2435	2438	2441	rBV2	490	355	0.02%	0.003%
55	9.321	2479	2482	2487	rBV2	249	280	0.02%	0.002%
56	9.359	2492	2494	2498	rVB2	382	262	0.02%	0.002%
57	9.414	2498	2511	2537	rBV	682229	1138639	77.79%	9.579%
58	9.565	2555	2558	2560	rBV2	1592	1088	0.07%	0.009%
59	9.617	2572	2574	2579	rBV2	303	246	0.02%	0.002%
60	9.758	2616	2618	2624	rVB	456	356	0.02%	0.003%
61	9.787	2624	2627	2629	rBV2	411	286	0.02%	0.002%
62	9.871	2651	2653	2656	rBV	322	244	0.02%	0.002%
63	10.022	2698	2700	2703	rBV2	399	257	0.02%	0.002%
64	10.112	2717	2728	2736	rBV7	2711	4757	0.32%	0.040%
65	10.292	2780	2784	2787	rVB2	688	530	0.04%	0.004%
66	10.321	2787	2793	2796	rBV2	344	381	0.03%	0.003%
67	10.372	2803	2809	2812	rBV2	437	581	0.04%	0.005%
68	10.420	2819	2824	2826	rBV	288	241	0.02%	0.002%
69	10.481	2834	2843	2850	rBV5	1667	2609	0.18%	0.022%
70	10.530	2855	2858	2861	rVB	352	223	0.02%	0.002%
71	10.755	2914	2928	2946	rBV	509408	831595	56.81%	6.996%
72	10.819	2946	2948	2957	rVB5	2125	2181	0.15%	0.018%
73	11.086	3028	3031	3032	rBV	745	408	0.03%	0.003%
74	11.285	3091	3093	3097	rBV2	305	231	0.02%	0.002%
75	11.469	3144	3150	3159	rVB3	2047	2430	0.17%	0.020%
76	11.587	3183	3187	3189	rBV	291	249	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
 Data File : VU050987.D
 Acq On : 29 Sep 2022 18:30
 Operator : JC/MD
 Sample : N4854-02DL 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J04DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	11.745	3227	3236	3244	rBV5	2737	4270	0.29%	0.036%
78	11.809	3244	3256	3276	rBV	512298	825350	56.38%	6.944%
79	11.980	3307	3309	3313	rBV	323	245	0.02%	0.002%
80	12.002	3314	3316	3319	rVB	456	244	0.02%	0.002%
81	12.076	3335	3339	3342	rVB3	435	317	0.02%	0.003%
82	12.192	3361	3375	3399	rBV	598664	953053	65.11%	8.018%
83	12.623	3505	3509	3513	rVV3	642	621	0.04%	0.005%
84	12.841	3574	3577	3579	rBV2	517	335	0.02%	0.003%
85	12.996	3623	3625	3635	rVB4	622	690	0.05%	0.006%
86	13.121	3661	3664	3668	rBV3	381	318	0.02%	0.003%
87	13.221	3687	3695	3696	rBV5	2721	2700	0.18%	0.023%
88	13.359	3735	3738	3741	rBV2	448	335	0.02%	0.003%
89	13.417	3754	3756	3761	rVB2	600	503	0.03%	0.004%
90	13.845	3882	3889	3898	rVB4	3256	5217	0.36%	0.044%
91	13.919	3910	3912	3915	rBV2	313	230	0.02%	0.002%
92	14.089	3958	3965	3981	rVB	4725	8352	0.57%	0.070%
93	14.272	4020	4022	4024	rBV2	528	286	0.02%	0.002%
94	14.330	4033	4040	4049	rBV6	3115	5001	0.34%	0.042%
95	14.587	4117	4120	4123	rBV3	482	393	0.03%	0.003%
96	14.857	4200	4204	4207	rBV3	699	662	0.05%	0.006%
97	14.970	4237	4239	4241	rBV	533	224	0.02%	0.002%
98	15.099	4276	4279	4283	rBV3	695	569	0.04%	0.005%
99	15.263	4328	4330	4333	rBV	692	402	0.03%	0.003%
100	15.899	4525	4528	4531	rBV3	1094	923	0.06%	0.008%




Sum of corrected areas: 11886601

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
Data File : VU050987.D
Acq On : 29 Sep 2022 18:30
Operator : JC/MD
Sample : N4854-02DL 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J04DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

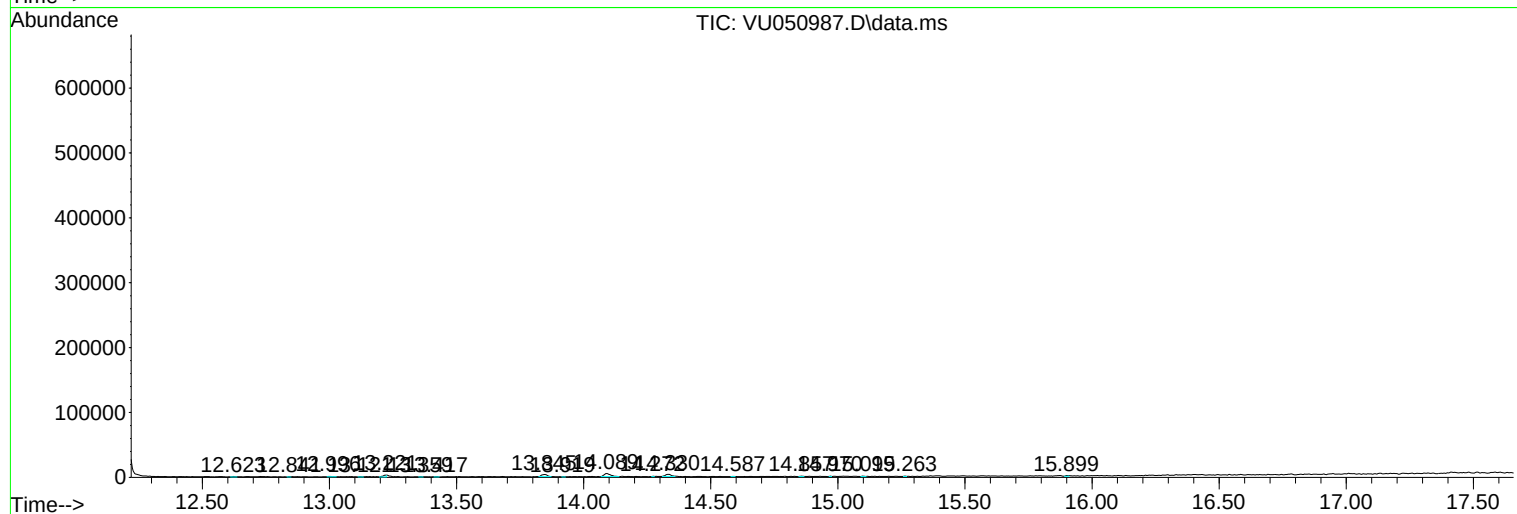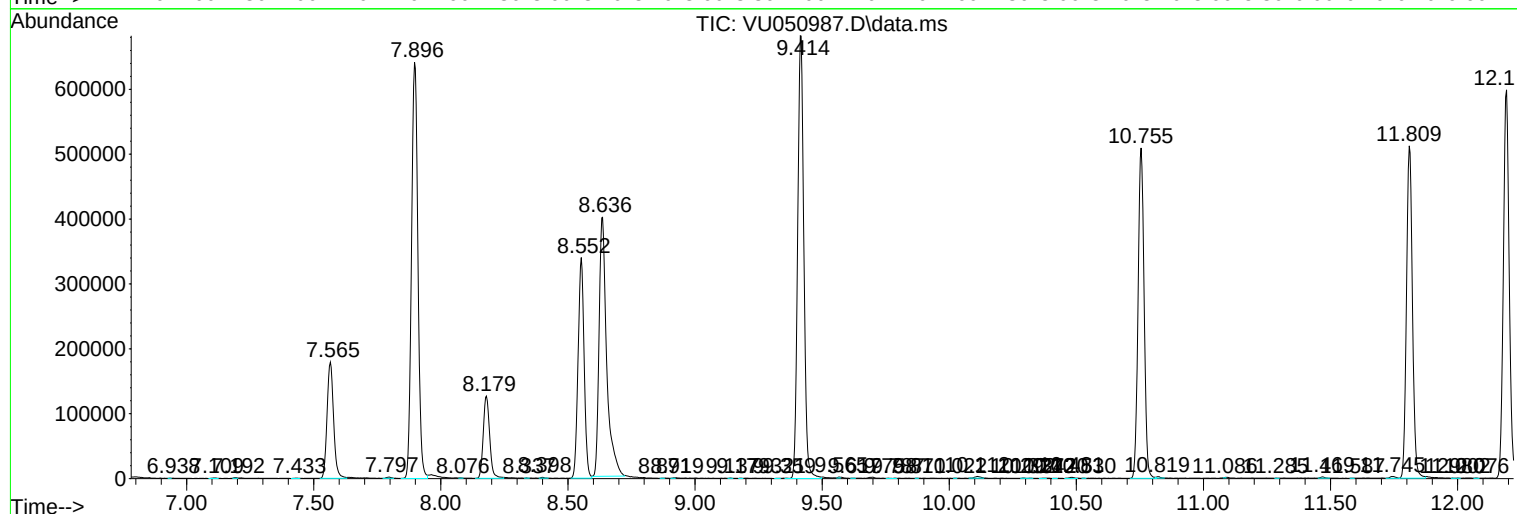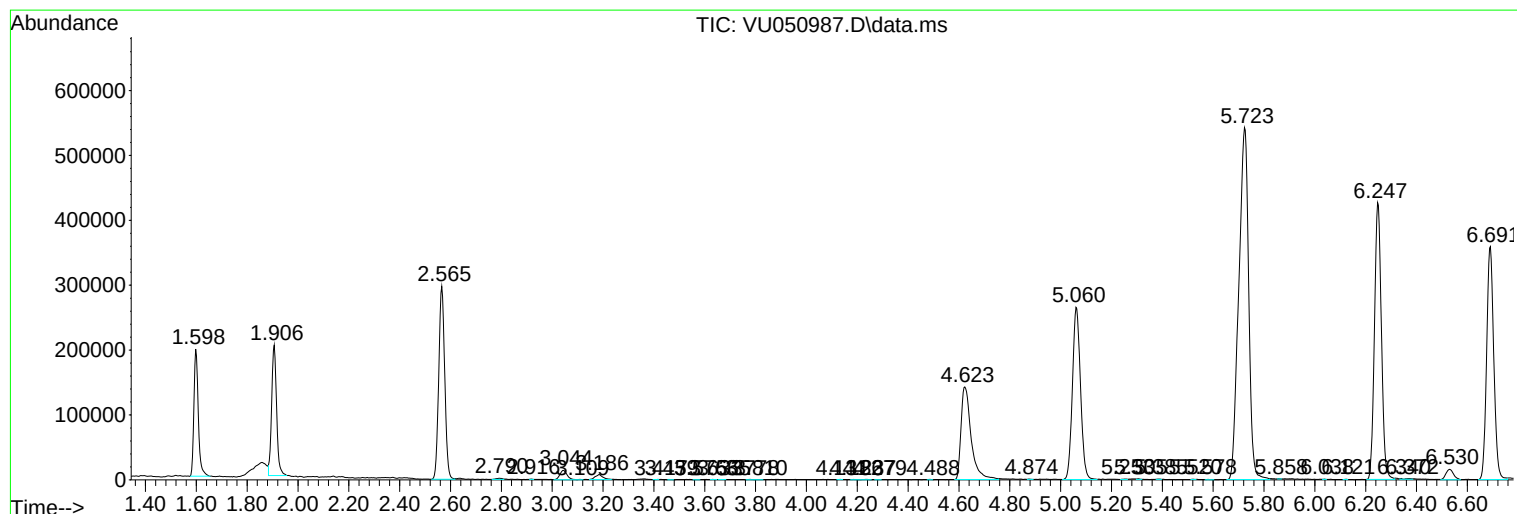

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
Data File : VU050987.D
Acq On : 29 Sep 2022 18:30
Operator : JC/MD
Sample : N4854-02DL 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J04DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
Data File : VU050987.D
Acq On : 29 Sep 2022 18:30
Operator : JC/MD
Sample : N4854-02DL 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J04DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------