

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
 Data File : VU050989.D
 Acq On : 29 Sep 2022 19:16
 Operator : JC/MD
 Sample : N4869-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J02

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M

Title : VOC Analysis

Signal : TIC: VU050989.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.598	73	80	102	rVB	196712	237940	1.09%	0.717%
2	1.900	166	174	192	rVB	168534	231052	1.05%	0.696%
3	2.517	363	366	368	rBV2	490	342	0.00%	0.001%
4	2.565	368	381	397	rVV	295339	474281	2.17%	1.429%
5	2.790	443	451	459	rBV3	1660	2481	0.01%	0.007%
6	2.852	467	470	475	rBV3	449	490	0.00%	0.001%
7	2.890	478	482	485	rVV2	503	329	0.00%	0.001%
8	3.038	522	528	539	rVV6	1299	2358	0.01%	0.007%
9	3.083	539	542	548	rVB4	417	428	0.00%	0.001%
10	3.128	548	556	558	rBV	430	522	0.00%	0.002%
11	3.186	558	574	593	rVB3	2856	7637	0.03%	0.023%
12	3.295	603	608	611	rBV2	288	272	0.00%	0.001%
13	3.360	617	628	629	rBV3	3338	3759	0.02%	0.011%
14	3.507	672	674	679	rVB	344	268	0.00%	0.001%
15	3.549	679	687	695	rBV3	854	1735	0.01%	0.005%
16	3.999	822	827	831	rVB2	324	289	0.00%	0.001%
17	4.051	838	843	847	rVB3	347	283	0.00%	0.001%
18	4.237	898	901	905	rVB2	457	329	0.00%	0.001%
19	4.260	905	908	913	rBV	313	260	0.00%	0.001%
20	4.321	921	927	931	rBV2	269	292	0.00%	0.001%
21	4.421	952	958	961	rVB3	321	313	0.00%	0.001%
22	4.620	1006	1020	1054	rBV	140760	375032	1.71%	1.130%
23	4.829	1083	1085	1089	rVB2	558	345	0.00%	0.001%
24	4.868	1094	1097	1101	rVB2	598	349	0.00%	0.001%
25	5.060	1141	1157	1181	rBV2	264381	586858	2.68%	1.768%
26	5.276	1221	1224	1227	rBV2	714	653	0.00%	0.002%
27	5.376	1250	1255	1257	rBV2	575	413	0.00%	0.001%
28	5.388	1257	1259	1263	rVB2	682	421	0.00%	0.001%
29	5.523	1296	1301	1304	rVB3	333	276	0.00%	0.001%
30	5.633	1328	1335	1338	rBV2	319	324	0.00%	0.001%
31	5.723	1342	1363	1388	rBV2	541698	1457080	6.65%	4.389%
32	5.893	1412	1416	1422	rVB5	1254	897	0.00%	0.003%
33	6.086	1472	1476	1481	rBV2	311	343	0.00%	0.001%
34	6.125	1482	1488	1492	rVB4	553	588	0.00%	0.002%
35	6.247	1512	1526	1549	rBV	394170	739885	3.38%	2.229%
36	6.353	1557	1559	1564	rVB4	884	575	0.00%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
 Data File : VU050989.D
 Acq On : 29 Sep 2022 19:16
 Operator : JC/MD
 Sample : N4869-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J02

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	6.539	1601	1617	1632	rBV5	43319	92265	0.42%	0.278%
38	6.687	1649	1663	1683	rBV	343048	668338	3.05%	2.013%
39	6.903	1726	1730	1733	rVB2	403	323	0.00%	0.001%
40	7.105	1791	1793	1799	rVB2	660	615	0.00%	0.002%
41	7.183	1809	1817	1819	rBV6	1138	1266	0.01%	0.004%
42	7.565	1922	1936	1956	rBV	170328	305122	1.39%	0.919%
43	7.797	2001	2008	2015	rBV5	778	993	0.00%	0.003%
44	7.896	2025	2039	2058	rBV	640050	1088969	4.97%	3.280%
45	8.176	2114	2126	2143	rBV	124318	212758	0.97%	0.641%
46	8.343	2176	2178	2182	rVB	529	324	0.00%	0.001%
47	8.363	2182	2184	2188	rVB2	455	260	0.00%	0.001%
48	8.427	2199	2204	2206	rBV2	397	333	0.00%	0.001%
49	8.552	2227	2243	2258	rBV	13449088	21904918	100.00%	65.978%
50	8.633	2260	2268	2298	rVB2	467202	1012086	4.62%	3.048%
51	8.861	2336	2339	2344	rVV3	1056	931	0.00%	0.003%
52	8.883	2344	2346	2350	rVB4	450	337	0.00%	0.001%
53	9.289	2465	2472	2478	rBV4	1350	1713	0.01%	0.005%
54	9.314	2478	2480	2485	rVB2	339	255	0.00%	0.001%
55	9.414	2498	2511	2534	rBV	664907	1074021	4.90%	3.235%
56	9.565	2556	2558	2566	rVB4	876	1055	0.00%	0.003%
57	9.694	2595	2598	2608	rVB5	1047	1496	0.01%	0.005%
58	9.848	2644	2646	2649	rVB2	486	296	0.00%	0.001%
59	9.964	2678	2682	2686	rBV3	254	267	0.00%	0.001%
60	10.035	2699	2704	2706	rBV3	337	294	0.00%	0.001%
61	10.047	2706	2708	2714	rVB2	366	292	0.00%	0.001%
62	10.157	2739	2742	2744	rBV	398	294	0.00%	0.001%
63	10.417	2817	2823	2827	rBV2	304	381	0.00%	0.001%
64	10.459	2832	2836	2839	rBV3	337	341	0.00%	0.001%
65	10.488	2843	2845	2850	rVB2	619	525	0.00%	0.002%
66	10.629	2886	2889	2893	rBV2	395	293	0.00%	0.001%
67	10.755	2914	2928	2952	rBV	526007	856863	3.91%	2.581%
68	11.034	3008	3015	3018	rBV3	485	529	0.00%	0.002%
69	11.096	3028	3034	3039	rVV4	609	634	0.00%	0.002%
70	11.356	3113	3115	3120	rVB2	505	367	0.00%	0.001%
71	11.388	3121	3125	3130	rBV3	455	638	0.00%	0.002%
72	11.694	3216	3220	3222	rBV2	398	289	0.00%	0.001%
73	11.742	3229	3235	3244	rBV5	1653	2627	0.01%	0.008%
74	11.809	3244	3256	3275	rBV	517676	826615	3.77%	2.490%
75	12.067	3332	3336	3338	rBV	614	442	0.00%	0.001%
76	12.115	3348	3351	3358	rVB2	595	555	0.00%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
 Data File : VU050989.D
 Acq On : 29 Sep 2022 19:16
 Operator : JC/MD
 Sample : N4869-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J02

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	12.192	3361	3375	3401	rBV	608119	987871	4.51%	2.975%
78	12.382	3431	3434	3438	rBV	381	323	0.00%	0.001%
79	12.433	3445	3450	3453	rVB3	298	295	0.00%	0.001%
80	12.456	3453	3457	3460	rBV2	396	386	0.00%	0.001%
81	12.636	3510	3513	3516	rBV3	528	400	0.00%	0.001%
82	13.173	3674	3680	3683	rBV3	331	409	0.00%	0.001%
83	13.195	3683	3687	3689	rBV	517	410	0.00%	0.001%
84	13.349	3731	3735	3739	rVB2	628	398	0.00%	0.001%
85	13.449	3763	3766	3771	rVB2	691	463	0.00%	0.001%
86	13.523	3785	3789	3793	rBV2	618	522	0.00%	0.002%
87	13.722	3847	3851	3854	rVB3	402	303	0.00%	0.001%
88	13.848	3883	3890	3900	rVB6	2750	4466	0.02%	0.013%
89	14.015	3939	3942	3947	rVB2	554	489	0.00%	0.001%
90	14.095	3957	3967	3979	rBV4	2635	5455	0.02%	0.016%
91	14.234	4007	4010	4012	rBV3	509	310	0.00%	0.001%
92	14.330	4036	4040	4041	rBV4	1729	1189	0.01%	0.004%
93	14.568	4111	4114	4115	rBV2	525	340	0.00%	0.001%
94	14.899	4214	4217	4220	rBV2	606	471	0.00%	0.001%
95	15.292	4337	4339	4344	rBV2	486	494	0.00%	0.001%
96	15.340	4352	4354	4361	rVB2	974	910	0.00%	0.003%
97	15.391	4362	4370	4375	rBV7	1208	1721	0.01%	0.005%
98	15.796	4493	4496	4500	rBV3	761	621	0.00%	0.002%
99	15.880	4520	4522	4526	rBV3	849	724	0.00%	0.002%
100	15.928	4535	4537	4542	rBV3	752	664	0.00%	0.002%




Sum of corrected areas: 33200253

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
Data File : VU050989.D
Acq On : 29 Sep 2022 19:16
Operator : JC/MD
Sample : N4869-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

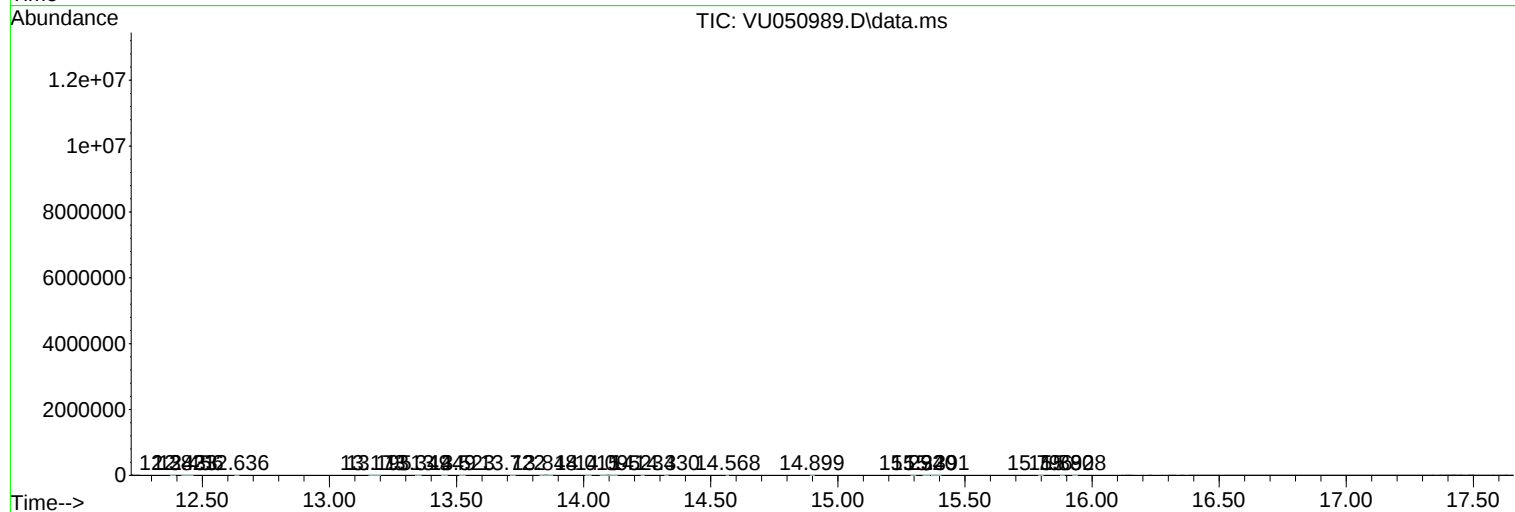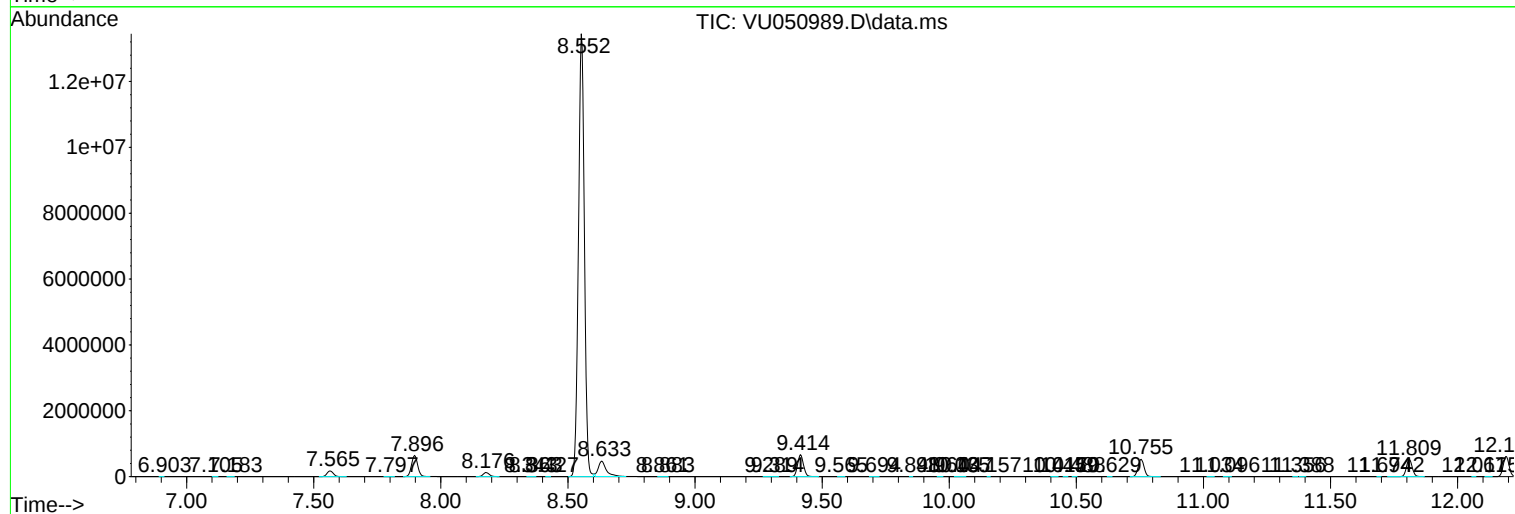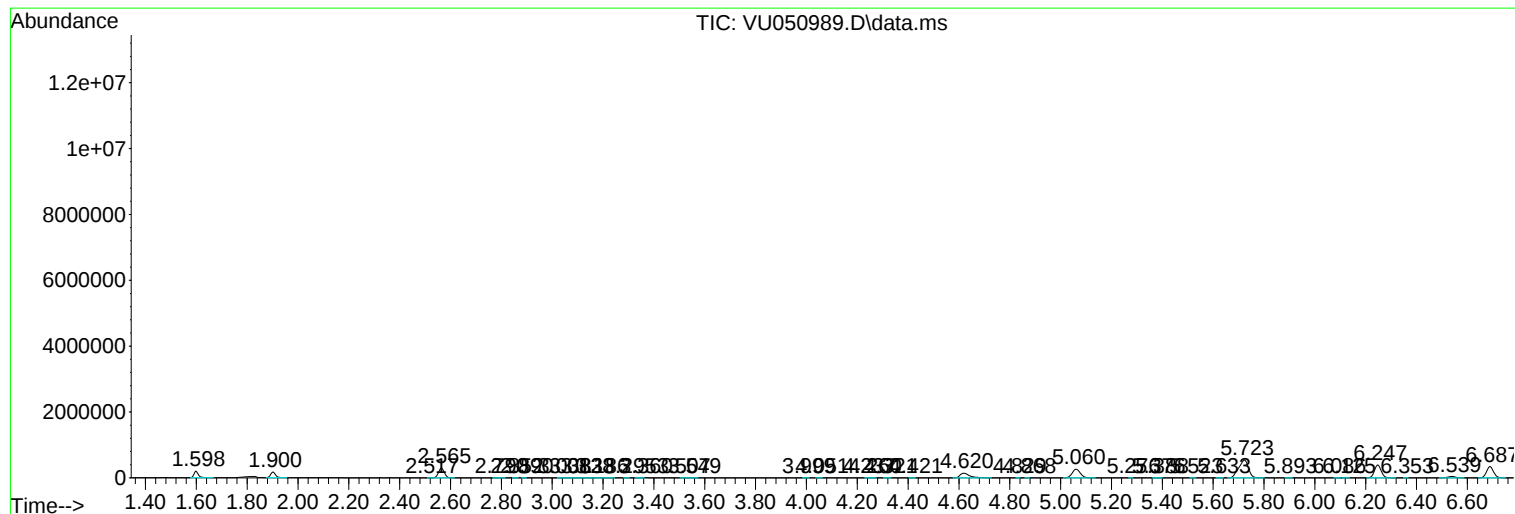

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
Data File : VU050989.D
Acq On : 29 Sep 2022 19:16
Operator : JC/MD
Sample : N4869-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
Data File : VU050989.D
Acq On : 29 Sep 2022 19:16
Operator : JC/MD
Sample : N4869-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------