

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
 Data File : VU050990.D
 Acq On : 29 Sep 2022 19:40
 Operator : JC/MD
 Sample : N4869-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J05

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

Signal : TIC: VU050990.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	101	rVB	175349	208408	0.80%	0.573%
2	1.803	128	144	145	rBV3	31008	62494	0.24%	0.172%
3	1.903	167	175	193	rVB	154236	205778	0.79%	0.565%
4	2.362	316	318	322	rVB4	991	578	0.00%	0.002%
5	2.514	363	365	368	rBV2	360	233	0.00%	0.001%
6	2.565	368	381	396	rBV	252156	407251	1.57%	1.119%
7	2.861	470	473	475	rBV2	548	345	0.00%	0.001%
8	2.896	481	484	490	rVB4	390	345	0.00%	0.001%
9	2.948	497	500	505	rVB2	474	445	0.00%	0.001%
10	3.041	521	529	538	rVB4	1729	3269	0.01%	0.009%
11	3.137	555	559	561	rVV2	459	324	0.00%	0.001%
12	3.179	561	572	589	rVB2	6874	15994	0.06%	0.044%
13	3.266	595	599	603	rBV2	332	378	0.00%	0.001%
14	3.356	618	627	630	rBV5	2469	3115	0.01%	0.009%
15	3.430	646	650	656	rBV2	510	653	0.00%	0.002%
16	3.494	664	670	673	rBV2	416	385	0.00%	0.001%
17	3.632	708	713	717	rBV2	399	372	0.00%	0.001%
18	3.761	750	753	758	rVB	305	244	0.00%	0.001%
19	3.838	773	777	785	rBV2	517	621	0.00%	0.002%
20	4.134	867	869	876	rVB	316	310	0.00%	0.001%
21	4.176	876	882	885	rBV2	381	346	0.00%	0.001%
22	4.526	989	991	998	rVB2	273	240	0.00%	0.001%
23	4.616	1007	1019	1048	rBV	136966	393482	1.51%	1.081%
24	4.784	1068	1071	1074	rBV	363	248	0.00%	0.001%
25	5.060	1139	1157	1182	rBV	242146	534740	2.06%	1.469%
26	5.205	1199	1202	1208	rVB4	543	422	0.00%	0.001%
27	5.269	1220	1222	1225	rBV2	510	440	0.00%	0.001%
28	5.362	1248	1251	1255	rBV	683	574	0.00%	0.002%
29	5.722	1341	1363	1387	rBV2	491354	1321045	5.08%	3.630%
30	5.851	1400	1403	1406	rBV3	776	667	0.00%	0.002%
31	5.976	1440	1442	1448	rVB2	752	566	0.00%	0.002%
32	6.009	1448	1452	1455	rBV2	526	375	0.00%	0.001%
33	6.047	1461	1464	1467	rVB3	515	404	0.00%	0.001%
34	6.115	1479	1485	1486	rBV2	443	380	0.00%	0.001%
35	6.247	1511	1526	1546	rBV	359356	683258	2.63%	1.878%
36	6.468	1591	1595	1597	rBV2	294	241	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
 Data File : VU050990.D
 Acq On : 29 Sep 2022 19:40
 Operator : JC/MD
 Sample : N4869-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J05

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	6.539	1602	1617	1630	rVV3	33165	72907	0.28%	0.200%
38	6.690	1648	1664	1684	rBV	309431	611312	2.35%	1.680%
39	6.886	1719	1725	1727	rVB3	439	438	0.00%	0.001%
40	6.935	1738	1740	1745	rVB	361	299	0.00%	0.001%
41	7.108	1789	1794	1803	rVB6	1696	2247	0.01%	0.006%
42	7.185	1810	1818	1822	rBV4	968	1177	0.00%	0.003%
43	7.462	1894	1904	1905	rBV2	168	263	0.00%	0.001%
44	7.565	1923	1936	1953	rBV	157082	276884	1.06%	0.761%
45	7.703	1977	1979	1984	rVB4	507	383	0.00%	0.001%
46	7.729	1984	1987	1991	rVB3	423	310	0.00%	0.001%
47	7.787	1998	2005	2007	rBV3	382	422	0.00%	0.001%
48	7.896	2022	2039	2058	rBV	573833	971830	3.74%	2.670%
49	8.179	2115	2127	2143	rBV2	116690	196208	0.75%	0.539%
50	8.324	2169	2172	2175	rVB3	533	334	0.00%	0.001%
51	8.378	2185	2189	2193	rBV2	419	391	0.00%	0.001%
52	8.446	2208	2210	2211	rBV2	554	256	0.00%	0.001%
53	8.555	2227	2244	2258	rBV	15990603	25999681	100.00%	71.444%
54	8.632	2260	2268	2304	rVB3	411781	924742	3.56%	2.541%
55	8.928	2355	2360	2364	rVB3	635	578	0.00%	0.002%
56	9.015	2383	2387	2389	rBV2	582	383	0.00%	0.001%
57	9.031	2390	2392	2396	rVB2	459	272	0.00%	0.001%
58	9.121	2416	2420	2425	rBV3	482	535	0.00%	0.001%
59	9.150	2425	2429	2432	rVB2	435	308	0.00%	0.001%
60	9.336	2484	2487	2488	rBV2	398	242	0.00%	0.001%
61	9.417	2498	2512	2540	rBV	547250	904861	3.48%	2.486%
62	9.703	2593	2601	2606	rVB5	532	866	0.00%	0.002%
63	9.803	2627	2632	2634	rBV2	241	245	0.00%	0.001%
64	9.944	2674	2676	2680	rVB2	370	241	0.00%	0.001%
65	9.996	2687	2692	2695	rBV2	343	383	0.00%	0.001%
66	10.301	2780	2787	2791	rBV2	569	894	0.00%	0.002%
67	10.369	2805	2808	2811	rBV	293	241	0.00%	0.001%
68	10.549	2862	2864	2870	rVB2	481	381	0.00%	0.001%
69	10.639	2890	2892	2899	rVB3	362	368	0.00%	0.001%
70	10.680	2902	2905	2908	rVB3	362	279	0.00%	0.001%
71	10.703	2908	2912	2915	rBV2	298	323	0.00%	0.001%
72	10.754	2915	2928	2948	rBV	496945	807420	3.11%	2.219%
73	11.086	3028	3031	3036	rBV3	711	603	0.00%	0.002%
74	11.323	3101	3105	3106	rBV2	389	268	0.00%	0.001%
75	11.378	3120	3122	3127	rVB2	541	396	0.00%	0.001%
76	11.407	3127	3131	3135	rBV	620	513	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
 Data File : VU050990.D
 Acq On : 29 Sep 2022 19:40
 Operator : JC/MD
 Sample : N4869-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J05

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	11.462	3143	3148	3150	rBV3	532	467	0.00%	0.001%
78	11.745	3231	3236	3244	rBV4	1425	1780	0.01%	0.005%
79	11.809	3244	3256	3280	rBV	497899	804797	3.10%	2.211%
80	12.192	3362	3375	3399	rBV	575178	940365	3.62%	2.584%
81	12.336	3417	3420	3422	rBV3	500	273	0.00%	0.001%
82	12.365	3424	3429	3433	rVV3	777	692	0.00%	0.002%
83	12.722	3537	3540	3543	rBV	751	549	0.00%	0.002%
84	12.822	3569	3571	3575	rBV3	335	271	0.00%	0.001%
85	12.947	3607	3610	3613	rBV3	351	260	0.00%	0.001%
86	13.024	3632	3634	3639	rVB2	679	493	0.00%	0.001%
87	13.301	3717	3720	3721	rBV2	437	234	0.00%	0.001%
88	13.442	3761	3764	3766	rBV	417	252	0.00%	0.001%
89	13.542	3792	3795	3798	rVB4	419	288	0.00%	0.001%
90	13.815	3877	3880	3881	rBV4	471	254	0.00%	0.001%
91	13.844	3885	3889	3897	rVB4	1461	1713	0.01%	0.005%
92	14.044	3948	3951	3953	rBV2	532	330	0.00%	0.001%
93	14.095	3959	3967	3974	rBV4	2026	3137	0.01%	0.009%
94	14.246	4011	4014	4017	rBV3	553	418	0.00%	0.001%
95	14.333	4036	4041	4049	rVB5	1854	2467	0.01%	0.007%
96	14.651	4138	4140	4143	rBV2	526	318	0.00%	0.001%
97	14.889	4207	4214	4219	rBV4	589	889	0.00%	0.002%
98	14.941	4228	4230	4233	rVB2	642	341	0.00%	0.001%
99	15.060	4261	4267	4270	rBV3	966	1015	0.00%	0.003%
100	15.999	4555	4559	4560	rBV3	793	510	0.00%	0.001%




Sum of corrected areas: 36391767

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
Data File : VU050990.D
Acq On : 29 Sep 2022 19:40
Operator : JC/MD
Sample : N4869-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J05

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

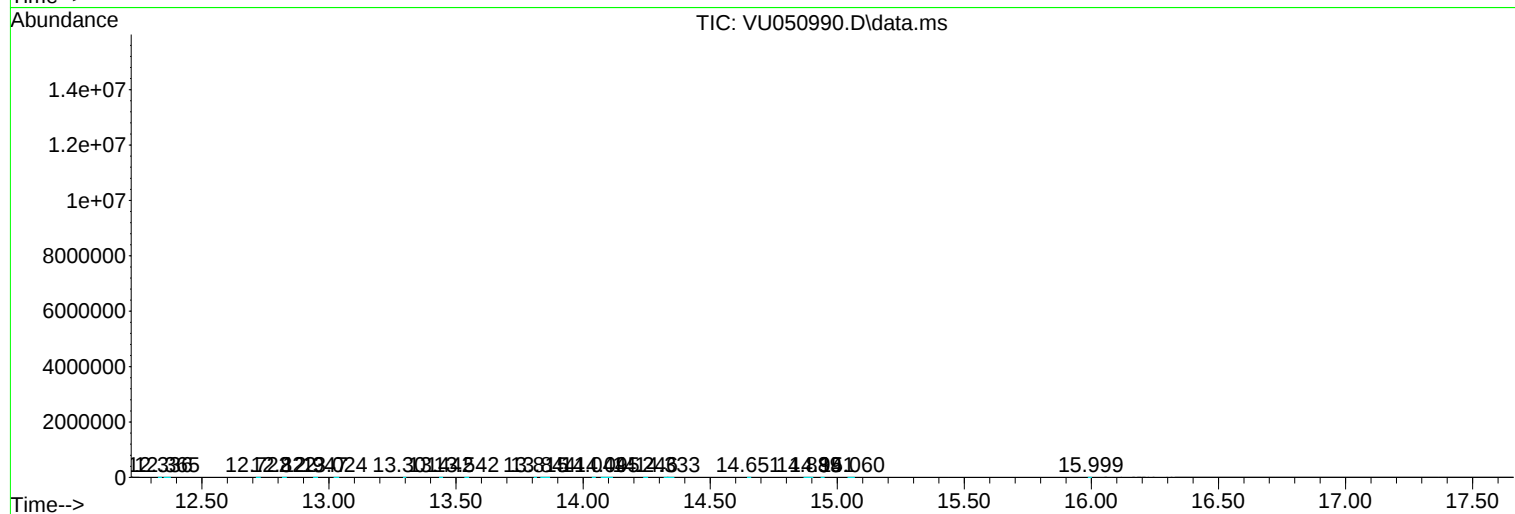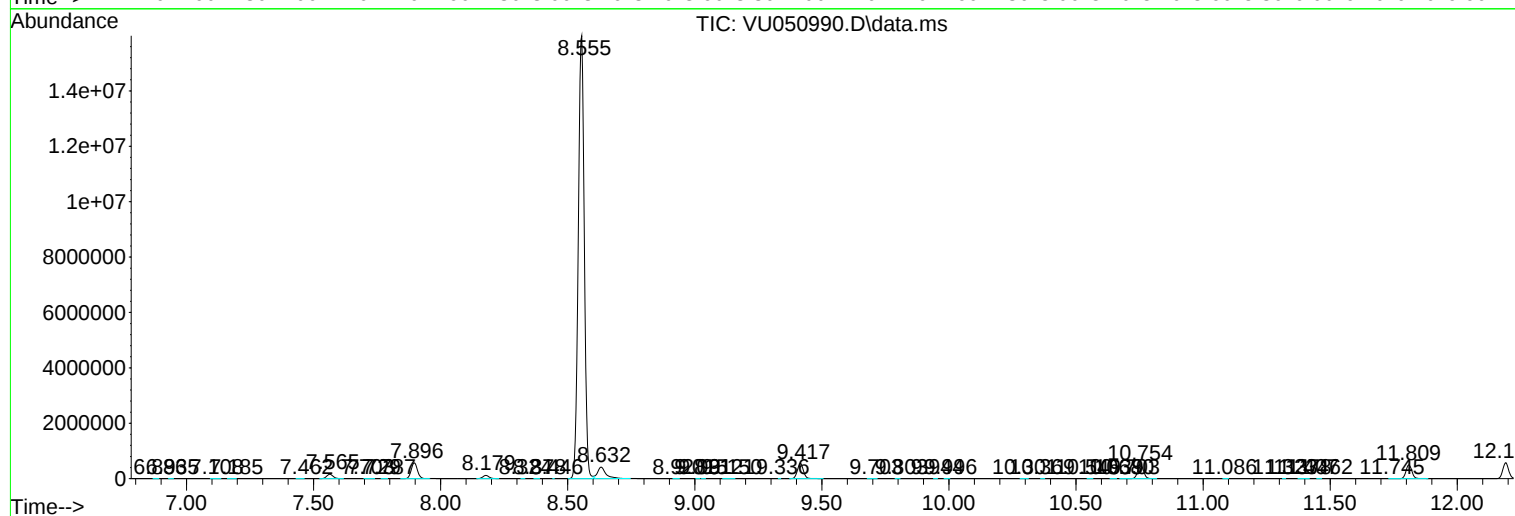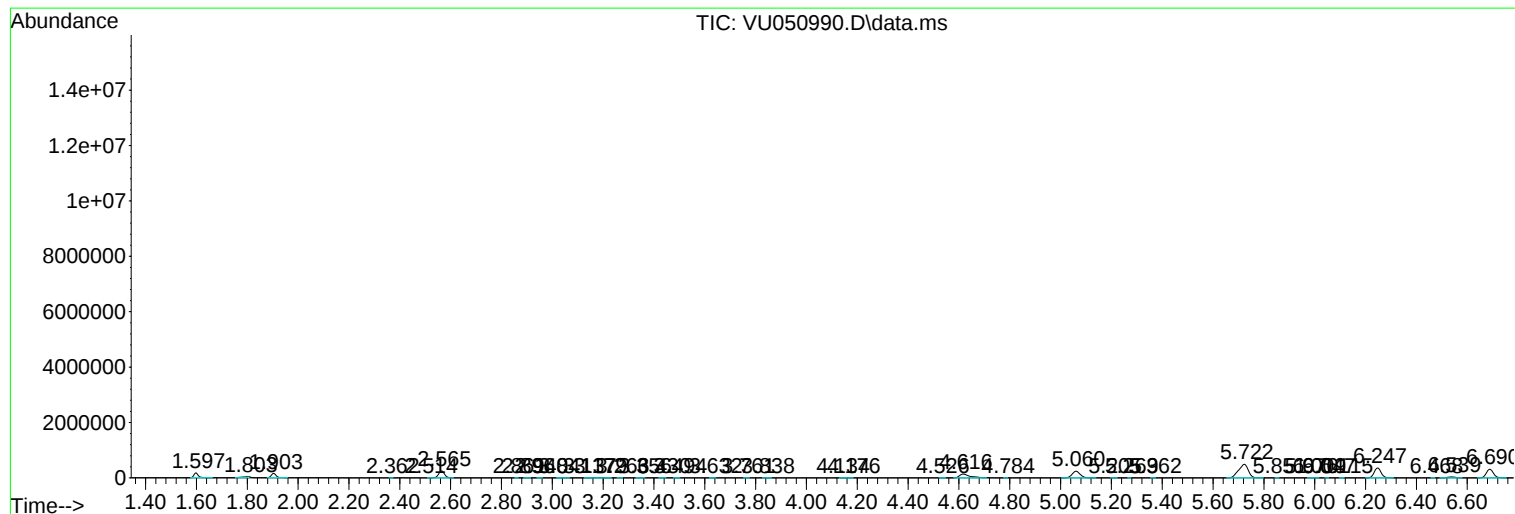

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
Data File : VU050990.D
Acq On : 29 Sep 2022 19:40
Operator : JC/MD
Sample : N4869-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J05

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
Data File : VU050990.D
Acq On : 29 Sep 2022 19:40
Operator : JC/MD
Sample : N4869-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J05

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc