

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
 Data File : VU050992.D
 Acq On : 29 Sep 2022 20:27
 Operator : JC/MD
 Sample : N4869-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J12

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M

Title : VOC Analysis

Signal : TIC: VU050992.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	98	rVB	193582	227441	10.40%	1.836%
2	1.903	167	175	194	rVB	166027	222977	10.20%	1.800%
3	2.565	368	381	405	rBV	278961	456543	20.88%	3.686%
4	3.038	521	528	532	rBV4	1173	1763	0.08%	0.014%
5	3.102	545	548	551	rBV2	263	224	0.01%	0.002%
6	3.118	551	553	558	rVV2	213	168	0.01%	0.001%
7	3.295	605	608	615	rVB3	296	321	0.01%	0.003%
8	3.327	615	618	619	rBV	250	130	0.01%	0.001%
9	3.356	620	627	642	rVB6	2548	5524	0.25%	0.045%
10	3.469	659	662	664	rBV2	400	257	0.01%	0.002%
11	3.578	692	696	699	rBV2	194	223	0.01%	0.002%
12	3.736	741	745	748	rBV	132	125	0.01%	0.001%
13	3.764	749	754	756	rVB	297	259	0.01%	0.002%
14	3.784	756	760	761	rBV	236	158	0.01%	0.001%
15	3.887	790	792	794	rBV	211	110	0.01%	0.001%
16	3.990	821	824	826	rBV	169	106	0.00%	0.001%
17	4.002	826	828	829	rBV	170	63	0.00%	0.001%
18	4.134	863	869	872	rBV2	313	341	0.02%	0.003%
19	4.182	881	884	885	rBV	213	125	0.01%	0.001%
20	4.253	902	906	908	rBV2	174	134	0.01%	0.001%
21	4.282	912	915	918	rVV	187	119	0.01%	0.001%
22	4.334	927	931	934	rVB2	543	453	0.02%	0.004%
23	4.353	934	937	942	rBV2	307	235	0.01%	0.002%
24	4.424	957	959	961	rBV	225	103	0.00%	0.001%
25	4.507	982	985	988	rBV	309	223	0.01%	0.002%
26	4.549	994	998	1001	rBV2	226	216	0.01%	0.002%
27	4.617	1007	1019	1046	rBV	135408	335442	15.34%	2.709%
28	4.967	1124	1128	1132	rBV2	542	540	0.02%	0.004%
29	5.060	1141	1157	1180	rBV	256484	565494	25.87%	4.566%
30	5.498	1290	1293	1295	rBV2	203	151	0.01%	0.001%
31	5.520	1296	1300	1302	rVV3	282	211	0.01%	0.002%
32	5.723	1341	1363	1387	rBV2	519915	1393739	63.75%	11.254%
33	6.096	1476	1479	1481	rBV2	220	150	0.01%	0.001%
34	6.112	1481	1484	1490	rBV3	544	464	0.02%	0.004%
35	6.247	1510	1526	1548	rBV	370883	703254	32.17%	5.678%
36	6.530	1602	1614	1628	rVB6	13581	27245	1.25%	0.220%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
 Data File : VU050992.D
 Acq On : 29 Sep 2022 20:27
 Operator : JC/MD
 Sample : N4869-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J12

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	6.620	1641	1642	1643	rVB6	255	49	0.00%	0.000%
38	6.636	1643	1647	1649	rBV2	315	274	0.01%	0.002%
39	6.687	1649	1663	1682	rBV	332977	639829	29.27%	5.166%
40	7.063	1775	1780	1783	rBV2	225	252	0.01%	0.002%
41	7.086	1783	1787	1791	rVV	260	275	0.01%	0.002%
42	7.105	1791	1793	1795	rVB	197	84	0.00%	0.001%
43	7.153	1804	1808	1809	rBV2	199	143	0.01%	0.001%
44	7.346	1865	1868	1870	rBV2	165	114	0.01%	0.001%
45	7.391	1878	1882	1884	rBV2	180	141	0.01%	0.001%
46	7.423	1889	1892	1895	rBV2	218	163	0.01%	0.001%
47	7.565	1923	1936	1952	rBV	161886	286457	13.10%	2.313%
48	7.896	2022	2039	2058	rBV	593857	1014588	46.41%	8.192%
49	8.176	2112	2126	2144	rBV	116399	198181	9.07%	1.600%
50	8.552	2229	2243	2257	rBV	1306107	2186190	100.00%	17.652%
51	8.632	2258	2268	2303	rVB3	365752	776050	35.50%	6.266%
52	8.928	2358	2360	2365	rVB	545	371	0.02%	0.003%
53	9.034	2391	2393	2397	rVB2	335	226	0.01%	0.002%
54	9.163	2430	2433	2436	rBV2	346	193	0.01%	0.002%
55	9.227	2451	2453	2457	rBV2	392	246	0.01%	0.002%
56	9.304	2475	2477	2480	rBV3	273	206	0.01%	0.002%
57	9.414	2498	2511	2538	rBV	549344	906017	41.44%	7.316%
58	9.690	2590	2597	2599	rBV2	314	377	0.02%	0.003%
59	9.771	2619	2622	2624	rBV	271	200	0.01%	0.002%
60	9.812	2633	2635	2640	rVB2	352	270	0.01%	0.002%
61	9.838	2640	2643	2646	rBV2	330	232	0.01%	0.002%
62	9.870	2650	2653	2654	rVB	182	75	0.00%	0.001%
63	9.912	2662	2666	2670	rBV2	418	393	0.02%	0.003%
64	9.967	2681	2683	2685	rVB	213	84	0.00%	0.001%
65	9.983	2685	2688	2693	rBV3	246	187	0.01%	0.002%
66	10.066	2712	2714	2715	rBV	153	80	0.00%	0.001%
67	10.095	2719	2723	2727	rBV2	494	474	0.02%	0.004%
68	10.124	2728	2732	2734	rVV2	494	323	0.01%	0.003%
69	10.140	2734	2737	2739	rVB	487	266	0.01%	0.002%
70	10.160	2739	2743	2745	rBV	247	205	0.01%	0.002%
71	10.189	2750	2752	2753	rBV	298	123	0.01%	0.001%
72	10.349	2800	2802	2805	rVB2	250	141	0.01%	0.001%
73	10.365	2805	2807	2808	rBV	83	31	0.00%	0.000%
74	10.388	2812	2814	2815	rBV	111	43	0.00%	0.000%
75	10.558	2865	2867	2868	rBV	179	42	0.00%	0.000%
76	10.755	2915	2928	2948	rBV	477290	772452	35.33%	6.237%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
 Data File : VU050992.D
 Acq On : 29 Sep 2022 20:27
 Operator : JC/MD
 Sample : N4869-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J12

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	10.880	2965	2967	2968	rBV	384	174	0.01%	0.001%
78	10.983	2996	2999	3002	rVB	215	151	0.01%	0.001%
79	11.002	3002	3005	3008	rBV	447	342	0.02%	0.003%
80	11.066	3023	3025	3027	rBV	174	51	0.00%	0.000%
81	11.083	3027	3030	3032	rBV	332	264	0.01%	0.002%
82	11.182	3058	3061	3064	rBV	194	136	0.01%	0.001%
83	11.246	3077	3081	3085	rBV	404	436	0.02%	0.004%
84	11.375	3116	3121	3126	rBV3	403	536	0.02%	0.004%
85	11.423	3132	3136	3139	rBV2	276	257	0.01%	0.002%
86	11.462	3146	3148	3150	rBV	333	220	0.01%	0.002%
87	11.504	3158	3161	3164	rVB	311	227	0.01%	0.002%
88	11.526	3164	3168	3172	rBV2	395	363	0.02%	0.003%
89	11.552	3172	3176	3177	rBV2	274	183	0.01%	0.001%
90	11.619	3192	3197	3203	rBV	396	421	0.02%	0.003%
91	11.652	3203	3207	3213	rBV	318	387	0.02%	0.003%
92	11.690	3217	3219	3222	rBV2	268	152	0.01%	0.001%
93	11.748	3230	3237	3241	rVB4	911	1087	0.05%	0.009%
94	11.809	3241	3256	3280	rBV	448488	713823	32.65%	5.764%
95	12.192	3362	3375	3404	rBV	563698	931972	42.63%	7.525%
96	12.378	3427	3433	3439	rBV2	522	809	0.04%	0.007%
97	12.774	3554	3556	3559	rVB2	758	378	0.02%	0.003%
98	13.066	3645	3647	3654	rVB2	457	325	0.01%	0.003%
99	13.227	3693	3697	3704	rBV4	705	901	0.04%	0.007%


Sum of corrected areas: 12384673

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
Data File : VU050992.D
Acq On : 29 Sep 2022 20:27
Operator : JC/MD
Sample : N4869-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J12

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

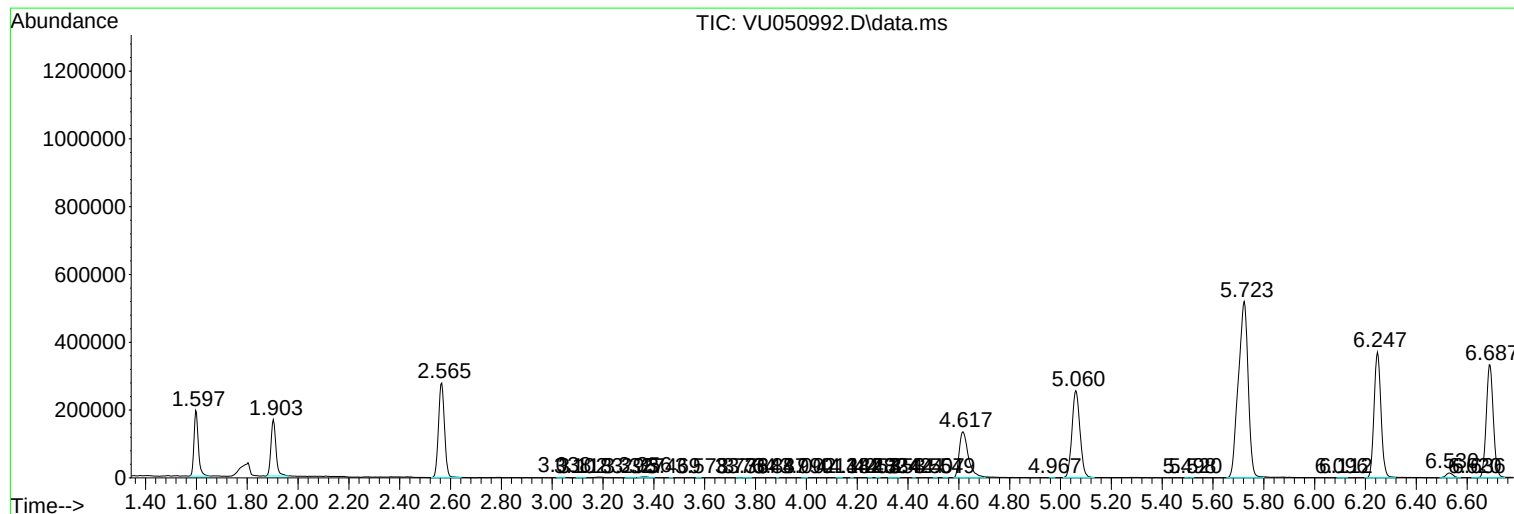

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
Data File : VU050992.D
Acq On : 29 Sep 2022 20:27
Operator : JC/MD
Sample : N4869-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J12

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
Data File : VU050992.D
Acq On : 29 Sep 2022 20:27
Operator : JC/MD
Sample : N4869-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J12

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc