

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
 Data File : VU050994.D
 Acq On : 29 Sep 2022 21:14
 Operator : JC/MD
 Sample : N4869-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J27

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

Signal : TIC: VU050994.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	93	rBV	176522	202313	16.05%	1.939%
2	1.800	124	143	152	rBV3	37500	93978	7.45%	0.901%
3	1.903	167	175	196	rVB	150457	203870	16.17%	1.954%
4	2.350	312	314	318	rBV4	849	607	0.05%	0.006%
5	2.514	360	365	368	rBV2	758	658	0.05%	0.006%
6	2.565	368	381	398	rBV	253122	411889	32.67%	3.948%
7	2.793	443	452	457	rBV3	785	1318	0.10%	0.013%
8	2.848	466	469	474	rBV4	324	291	0.02%	0.003%
9	2.877	474	478	483	rBV2	368	448	0.04%	0.004%
10	3.044	522	530	539	rBV5	1493	2390	0.19%	0.023%
11	3.182	559	573	580	rBV4	1822	3915	0.31%	0.038%
12	3.282	601	604	610	rBV2	251	257	0.02%	0.002%
13	3.366	620	630	637	rVV4	2074	4067	0.32%	0.039%
14	3.501	669	672	677	rVB3	416	395	0.03%	0.004%
15	3.578	693	696	698	rVV	356	222	0.02%	0.002%
16	3.629	706	712	715	rBV2	263	276	0.02%	0.003%
17	3.771	752	756	759	rBV2	324	257	0.02%	0.002%
18	3.880	786	790	797	rBV2	289	427	0.03%	0.004%
19	4.131	866	868	877	rVB2	275	268	0.02%	0.003%
20	4.179	881	883	891	rVB2	322	329	0.03%	0.003%
21	4.250	902	905	910	rVV2	255	220	0.02%	0.002%
22	4.366	936	941	944	rBV2	305	381	0.03%	0.004%
23	4.616	1007	1019	1049	rBV	127013	317107	25.15%	3.040%
24	4.777	1065	1069	1075	rVB3	811	793	0.06%	0.008%
25	5.060	1140	1157	1180	rBV	234146	517467	41.05%	4.960%
26	5.205	1194	1202	1208	rBV4	750	1238	0.10%	0.012%
27	5.276	1220	1224	1226	rBV2	500	413	0.03%	0.004%
28	5.311	1233	1235	1239	rVB2	535	408	0.03%	0.004%
29	5.382	1250	1257	1260	rBV4	642	749	0.06%	0.007%
30	5.510	1293	1297	1302	rBV2	203	240	0.02%	0.002%
31	5.722	1341	1363	1378	rBV2	464331	1260698	100.00%	12.085%
32	5.793	1379	1385	1397	rVB2	19974	38043	3.02%	0.365%
33	5.993	1442	1447	1450	rVB2	376	319	0.03%	0.003%
34	6.115	1479	1485	1490	rBV	732	746	0.06%	0.007%
35	6.247	1512	1526	1545	rBV	373551	703801	55.83%	6.746%
36	6.417	1575	1579	1581	rBV3	483	379	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
 Data File : VU050994.D
 Acq On : 29 Sep 2022 21:14
 Operator : JC/MD
 Sample : N4869-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J27

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	6.475	1593	1597	1599	rVB3	453	290	0.02%	0.003%
38	6.533	1603	1615	1631	rVB5	14230	28700	2.28%	0.275%
39	6.687	1649	1663	1682	rBV	300884	584299	46.35%	5.601%
40	6.848	1711	1713	1716	rVB2	585	298	0.02%	0.003%
41	6.909	1728	1732	1735	rBV2	275	222	0.02%	0.002%
42	6.944	1740	1743	1747	rVB3	345	242	0.02%	0.002%
43	7.015	1759	1765	1771	rVB2	388	585	0.05%	0.006%
44	7.108	1784	1794	1801	rVB4	865	1666	0.13%	0.016%
45	7.185	1814	1818	1821	rBV2	858	727	0.06%	0.007%
46	7.304	1850	1855	1859	rVB2	247	216	0.02%	0.002%
47	7.459	1899	1903	1906	rBV2	282	252	0.02%	0.002%
48	7.565	1923	1936	1956	rVV	145716	257149	20.40%	2.465%
49	7.665	1964	1967	1969	rBV2	393	231	0.02%	0.002%
50	7.745	1988	1992	1998	rVB3	576	562	0.04%	0.005%
51	7.787	2001	2005	2009	rBV3	311	262	0.02%	0.003%
52	7.896	2026	2039	2057	rBV	521232	907543	71.99%	8.699%
53	8.082	2094	2097	2100	rBV3	380	229	0.02%	0.002%
54	8.179	2114	2127	2140	rBV	104596	177502	14.08%	1.701%
55	8.398	2192	2195	2199	rVB3	456	355	0.03%	0.003%
56	8.449	2208	2211	2214	rBV2	272	238	0.02%	0.002%
57	8.472	2214	2218	2230	rVB5	892	1076	0.09%	0.010%
58	8.552	2230	2243	2256	rBV	429410	720182	57.13%	6.903%
59	8.632	2257	2268	2295	rVV2	328772	674408	53.49%	6.465%
60	8.925	2356	2359	2367	rVB2	783	786	0.06%	0.008%
61	8.960	2367	2370	2373	rBV2	554	411	0.03%	0.004%
62	9.118	2416	2419	2421	rBV	340	244	0.02%	0.002%
63	9.288	2466	2472	2475	rBV2	351	371	0.03%	0.004%
64	9.414	2498	2511	2544	rBV	544471	909261	72.12%	8.716%
65	9.565	2555	2558	2566	rVB4	633	758	0.06%	0.007%
66	9.697	2596	2599	2602	rVB2	413	276	0.02%	0.003%
67	9.951	2672	2678	2680	rBV	308	324	0.03%	0.003%
68	10.092	2718	2722	2726	rBV2	459	468	0.04%	0.004%
69	10.481	2841	2843	2848	rBV3	341	236	0.02%	0.002%
70	10.584	2872	2875	2878	rBV	279	236	0.02%	0.002%
71	10.754	2915	2928	2950	rBV	529351	855322	67.85%	8.199%
72	10.889	2964	2970	2971	rBV3	867	686	0.05%	0.007%
73	11.754	3233	3239	3243	rVB3	891	897	0.07%	0.009%
74	11.809	3243	3256	3280	rBV	451567	728268	57.77%	6.981%
75	12.028	3321	3324	3330	rVB2	537	537	0.04%	0.005%
76	12.057	3330	3333	3336	rBV	586	392	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
 Data File : VU050994.D
 Acq On : 29 Sep 2022 21:14
 Operator : JC/MD
 Sample : N4869-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J27

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	12.192	3362	3375	3404	rVV	478651	795975	63.14%	7.630%
78	12.465	3454	3460	3461	rBV3	511	428	0.03%	0.004%
79	12.516	3475	3476	3480	rBV2	271	224	0.02%	0.002%
80	12.539	3480	3483	3486	rVV2	362	304	0.02%	0.003%
81	12.716	3534	3538	3543	rVB2	484	417	0.03%	0.004%
82	12.745	3543	3547	3548	rBV	274	217	0.02%	0.002%
83	12.774	3553	3556	3558	rBV2	353	263	0.02%	0.003%
84	12.841	3574	3577	3579	rBV3	368	271	0.02%	0.003%
85	12.979	3616	3620	3624	rVV3	398	334	0.03%	0.003%
86	13.102	3655	3658	3661	rBV2	366	297	0.02%	0.003%
87	13.153	3672	3674	3679	rVB2	560	373	0.03%	0.004%
88	13.179	3679	3682	3686	rVB	525	344	0.03%	0.003%
89	13.204	3686	3690	3692	rBV3	455	306	0.02%	0.003%
90	13.224	3692	3696	3697	rBV2	569	380	0.03%	0.004%
91	13.314	3721	3724	3729	rVB3	542	446	0.04%	0.004%
92	13.394	3747	3749	3752	rVB2	525	252	0.02%	0.002%
93	13.413	3752	3755	3761	rBV2	368	426	0.03%	0.004%
94	13.706	3843	3846	3850	rBV2	353	340	0.03%	0.003%
95	13.732	3850	3854	3857	rBV3	308	326	0.03%	0.003%
96	13.848	3885	3890	3892	rBV	812	678	0.05%	0.006%
97	14.333	4038	4041	4048	rBV3	578	614	0.05%	0.006%
98	14.674	4144	4147	4150	rBV2	498	339	0.03%	0.003%
99	14.825	4190	4194	4199	rBV2	458	615	0.05%	0.006%
100	15.349	4354	4357	4358	rBV	482	255	0.02%	0.002%




Sum of corrected areas: 10432308

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
Data File : VU050994.D
Acq On : 29 Sep 2022 21:14
Operator : JC/MD
Sample : N4869-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J27

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

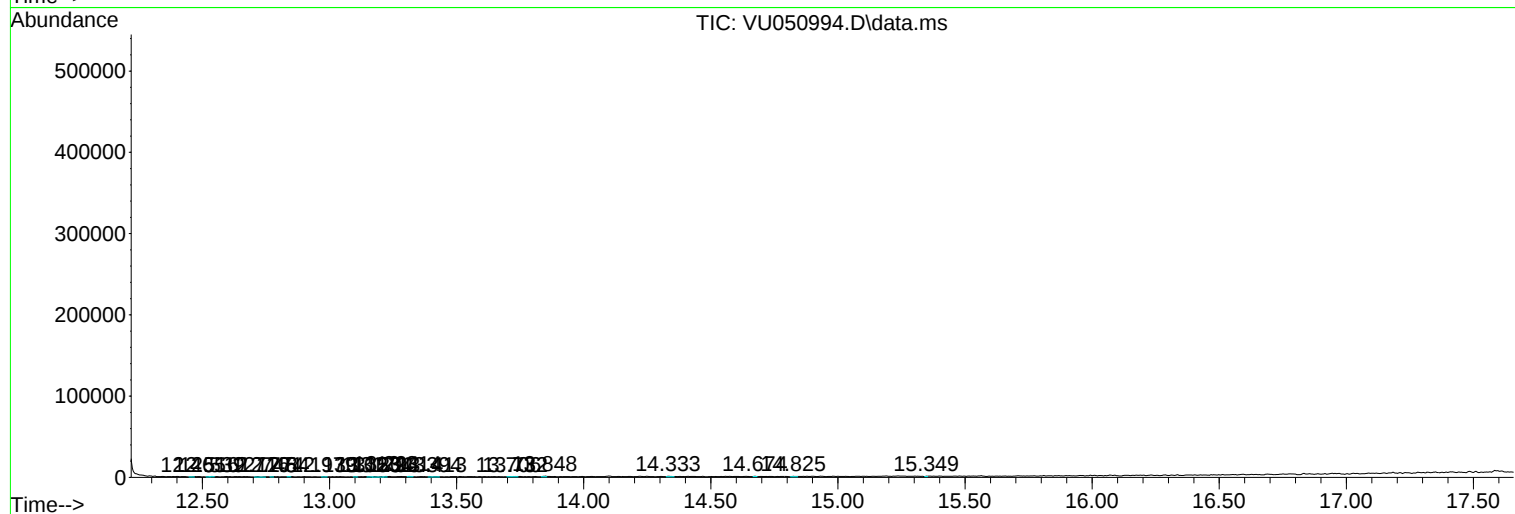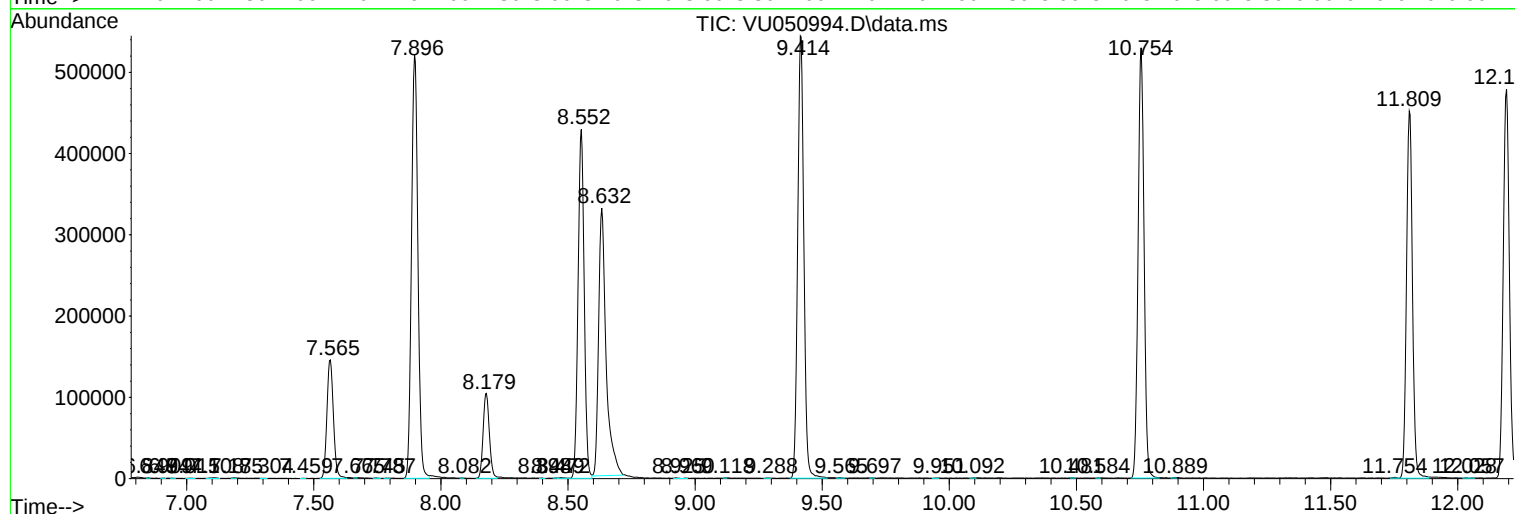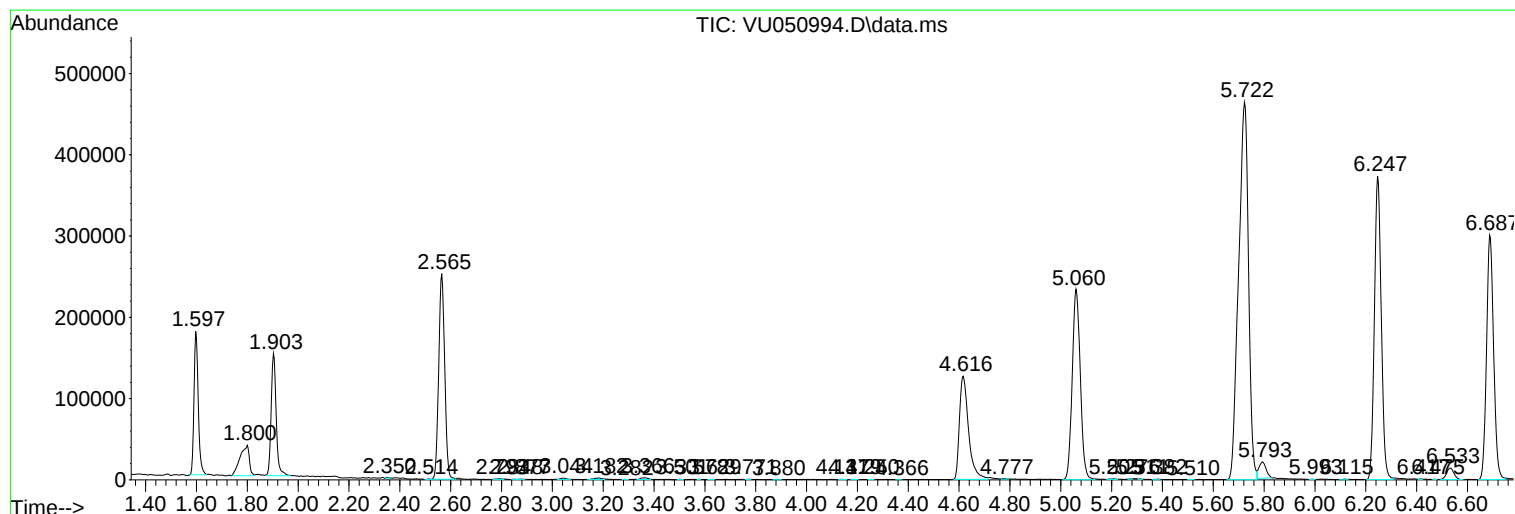

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
Data File : VU050994.D
Acq On : 29 Sep 2022 21:14
Operator : JC/MD
Sample : N4869-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J27

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
Data File : VU050994.D
Acq On : 29 Sep 2022 21:14
Operator : JC/MD
Sample : N4869-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J27

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc