

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
 Data File : VU050996.D
 Acq On : 29 Sep 2022 22:01
 Operator : JC/MD
 Sample : N4869-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J31

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

Signal : TIC: VU050996.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	98	rVB	177661	207058	4.54%	1.430%
2	1.800	127	143	154	rVB4	36223	83950	1.84%	0.580%
3	1.903	167	175	195	rVB	150627	209382	4.59%	1.446%
4	2.565	368	381	400	rBV	259598	423906	9.30%	2.928%
5	2.739	432	435	437	rBV2	444	346	0.01%	0.002%
6	2.781	446	448	452	rBV	550	457	0.01%	0.003%
7	2.832	461	464	469	rBV3	254	230	0.01%	0.002%
8	2.887	477	481	487	rVB3	373	405	0.01%	0.003%
9	2.932	491	495	498	rBV2	403	300	0.01%	0.002%
10	3.044	523	530	532	rBV4	1231	1614	0.04%	0.011%
11	3.179	563	572	588	rVB3	2415	5372	0.12%	0.037%
12	3.279	597	603	606	rBV3	379	427	0.01%	0.003%
13	3.356	616	627	641	rBV6	11310	24053	0.53%	0.166%
14	3.456	654	658	660	rBV	345	293	0.01%	0.002%
15	3.617	705	708	711	rBV3	295	225	0.00%	0.002%
16	3.899								

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
 Data File : VU050996.D
 Acq On : 29 Sep 2022 22:01
 Operator : JC/MD
 Sample : N4869-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J31

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	6.533	1601	1615	1630	rVB5	16912	37259	0.82%	0.257%
38	6.597	1630	1635	1637	rBV3	453	350	0.01%	0.002%
39	6.687	1649	1663	1682	rBV	303403	594082	13.03%	4.103%
40	6.806	1696	1700	1708	rVB6	1042	1214	0.03%	0.008%
41	6.877	1719	1722	1724	rBV	358	275	0.01%	0.002%
42	7.211	1824	1826	1833	rVB3	388	294	0.01%	0.002%
43	7.353	1867	1870	1880	rVV2	240	393	0.01%	0.003%
44	7.565	1922	1936	1956	rBV	147783	258819	5.68%	1.788%
45	7.742	1988	1991	1994	rBV2	250	206	0.00%	0.001%
46	7.829	2016	2018	2021	rBV	384	244	0.01%	0.002%
47	7.896	2026	2039	2056	rBV	550791	932083	20.44%	6.438%
48	8.099	2097	2102	2108	rVB3	799	969	0.02%	0.007%
49	8.179	2113	2127	2148	rBV	105668	181383	3.98%	1.253%
50	8.311	2166	2168	2171	rBV2	575	430	0.01%	0.003%
51	8.401	2193	2196	2198	rVB3	446	269	0.01%	0.002%
52	8.439	2200	2208	2210	rBV3	351	405	0.01%	0.003%
53	8.462	2							

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
 Data File : VU050996.D
 Acq On : 29 Sep 2022 22:01
 Operator : JC/MD
 Sample : N4869-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J31

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis




77	11.513	3157	3164	3167	rBV2	506	584	0.01%	0.004%
78	11.658	3206	3209	3211	rVB2	417	266	0.01%	0.002%
79	11.681	3213	3216	3220	rBV2	519	491	0.01%	0.003%
80	11.809	3243	3256	3275	rBV	477958	760189	16.67%	5.250%
81	11.992	3311	3313	3316	rVB3	565	260	0.01%	0.002%
82	12.192	3362	3375	3395	rBV	557542	899072	19.72%	6.210%
83	12.655	3517	3519	3522	rBV	624	342	0.01%	0.002%
84	12.889	3587	3592	3603	rBV3	524	940	0.02%	0.006%
85	13.070	3645	3648	3650	rBV	491	251	0.01%	0.002%
86	13.815	3874	3880	3883	rBV2	620	748	0.02%	0.005%
87	14.005	3937	3939	3942	rBV2	413	273	0.01%	0.002%
88	14.069	3956	3959	3963	rBV2	459	357	0.01%	0.002%
89	14.269	4016	4021	4025	rBV2	431	450	0.01%	0.003%
90	14.340	4039	4043	4046	rBV2	652	564	0.01%	0.004%
91	14.439	4070	4074	4079	rVB2	498	512	0.01%	0.004%
92	14.928	4221	4226	4232	rVB4	648	719	0.02%	0.005%
93	14.999	4246	4248	4253	rVB3				

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
Data File : VU050996.D
Acq On : 29 Sep 2022 22:01
Operator : JC/MD
Sample : N4869-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J31

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

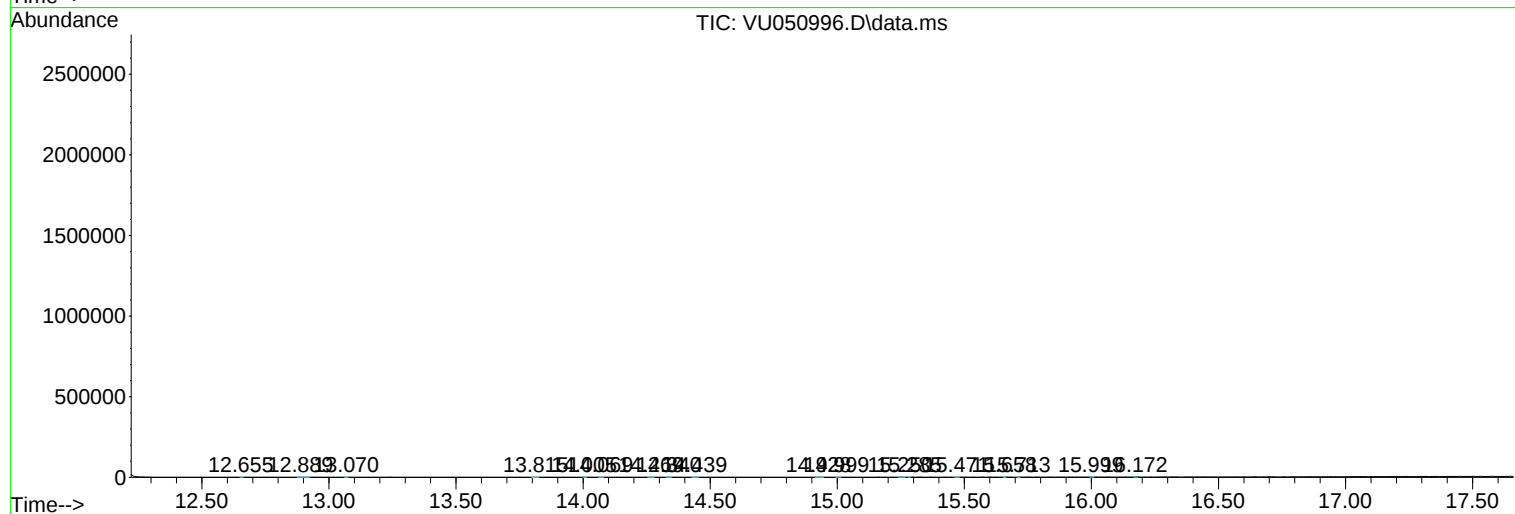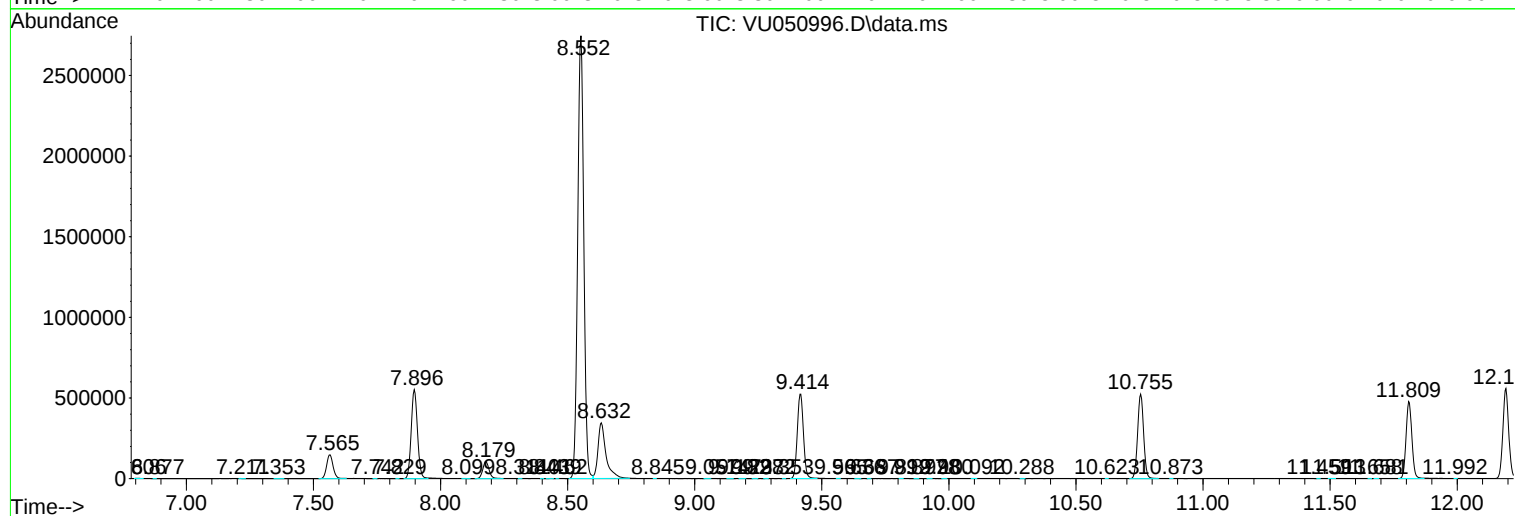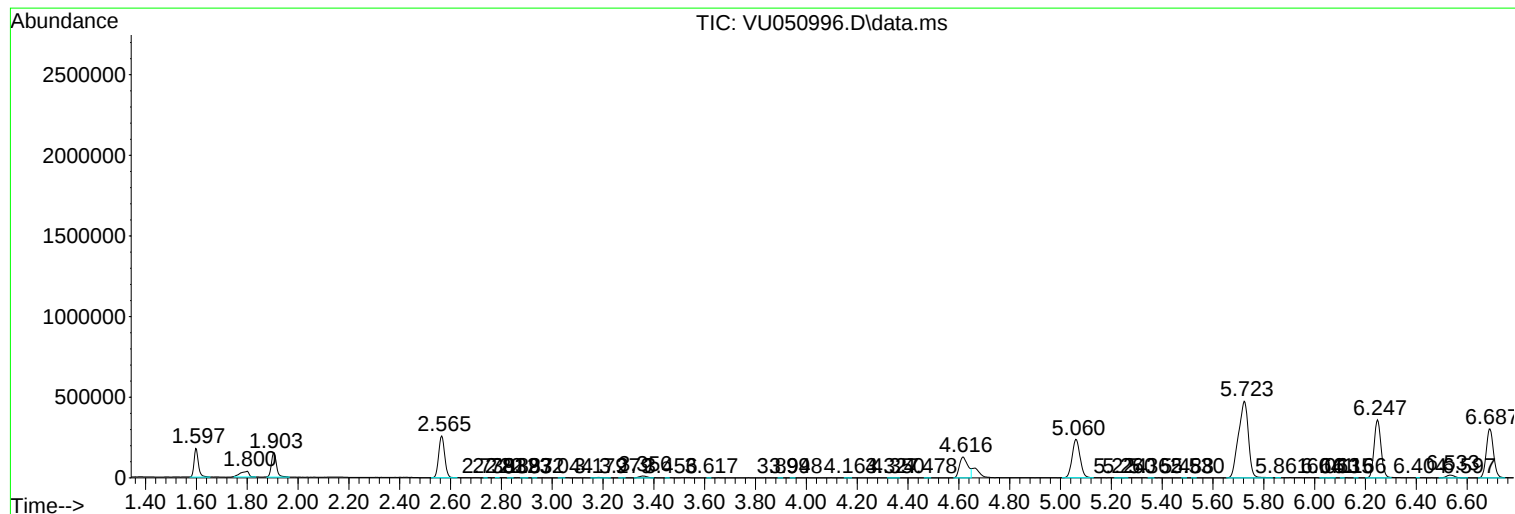

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
Data File : VU050996.D
Acq On : 29 Sep 2022 22:01
Operator : JC/MD
Sample : N4869-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J31

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
Data File : VU050996.D
Acq On : 29 Sep 2022 22:01
Operator : JC/MD
Sample : N4869-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J31

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
