

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
 Data File : VU050999.D
 Acq On : 29 Sep 2022 23:11
 Operator : JC/MD
 Sample : N4869-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J37

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

Signal : TIC: VU050999.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	101	rVB	184521	219980	7.16%	1.694%
2	1.906	169	176	191	rVB	166797	217330	7.07%	1.674%
3	2.565	368	381	397	rBV	277940	445314	14.49%	3.429%
4	2.787	443	450	456	rBV3	720	1295	0.04%	0.010%
5	2.861	469	473	476	rBV2	357	313	0.01%	0.002%
6	3.038	524	528	531	rBV3	1857	1703	0.06%	0.013%
7	3.186	562	574	586	rBV2	4437	8966	0.29%	0.069%
8	3.266	596	599	601	rBV	333	232	0.01%	0.002%
9	3.356	614	627	644	rVB5	16837	37020	1.20%	0.285%
10	3.424	644	648	651	rBV2	353	259	0.01%	0.002%
11	3.581	694	697	701	rVB	352	245	0.01%	0.002%
12	3.929	802	805	808	rBV	174	122	0.00%	0.001%
13	3.948	808	811	812	rBV	203	113	0.00%	0.001%
14	3.990	820	824	825	rBV	259	183	0.01%	0.001%
15	4.118	860	864	867	rBV2	244	205	0.01%	0.002%
16	4.154	873	875	878	rBV2	174	102	0.00%	0.001%
17	4.266	906	910	917	rBV2	286	331	0.01%	0.003%
18	4.298	917	920	922	rBV2	152	114	0.00%	0.001%
19	4.427	958	960	961	rBV	102	48	0.00%	0.000%
20	4.440	961	964	967	rVV2	205	192	0.01%	0.001%
21	4.524	987	990	991	rBV2	85	43	0.00%	0.000%
22	4.620	1008	1020	1047	rBV	132365	351388	11.44%	2.706%
23	5.061	1141	1157	1178	rBV	250137	552944	18.00%	4.258%
24	5.273	1221	1223	1226	rBV3	599	441	0.01%	0.003%
25	5.427	1268	1271	1272	rBV2	219	107	0.00%	0.001%
26	5.572	1314	1316	1318	rBV	191	83	0.00%	0.001%
27	5.604	1325	1326	1329	rBV	190	142	0.00%	0.001%
28	5.723	1341	1363	1387	rBV2	500240	1362333	44.34%	10.492%
29	6.173	1500	1503	1506	rBV	165	134	0.00%	0.001%
30	6.247	1513	1526	1553	rBV	364574	692415	22.54%	5.332%
31	6.540	1602	1617	1633	rVB6	36472	76163	2.48%	0.587%
32	6.601	1634	1636	1637	rBV6	110	30	0.00%	0.000%
33	6.623	1640	1643	1648	rBV2	275	195	0.01%	0.002%
34	6.691	1648	1664	1684	rBV	325191	636875	20.73%	4.905%
35	6.839	1707	1710	1713	rVB2	949	602	0.02%	0.005%
36	6.925	1735	1737	1742	rBV2	275	256	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
 Data File : VU050999.D
 Acq On : 29 Sep 2022 23:11
 Operator : JC/MD
 Sample : N4869-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F5J37

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	6.980	1752	1754	1757	rBV2	212	112	0.00%	0.001%
38	7.003	1757	1761	1765	rBV2	242	248	0.01%	0.002%
39	7.025	1765	1768	1772	rVB	363	257	0.01%	0.002%
40	7.044	1772	1774	1777	rBV2	287	201	0.01%	0.002%
41	7.093	1787	1789	1790	rBV2	106	59	0.00%	0.000%
42	7.186	1813	1818	1819	rBV4	859	623	0.02%	0.005%
43	7.231	1830	1832	1836	rVB	217	69	0.00%	0.001%
44	7.318	1856	1859	1861	rBV	230	148	0.00%	0.001%
45	7.379	1874	1878	1880	rBV	199	139	0.00%	0.001%
46	7.404	1883	1886	1892	rVB	244	196	0.01%	0.002%
47	7.462	1901	1904	1907	rBV2	155	98	0.00%	0.001%
48	7.565	1923	1936	1955	rBV	152766	271325	8.83%	2.090%
49	7.729	1985	1987	1994	rBV2	425	347	0.01%	0.003%
50	7.794	2003	2007	2015	rBV4	564	586	0.02%	0.005%
51	7.896	2025	2039	2056	rBV	569990	981101	31.93%	7.556%
52	8.118	2107	2108	2111	rVB2	371	86	0.00%	0.001%
53	8.179	2115	2127	2143	rBV	112259	190025	6.18%	1.463%
54	8.552	2229	2243	2257	rBV	1844139	3072561	100.00%	23.662%
55	8.633	2259	2268	2309	rVB3	367248	790807	25.74%	6.090%
56	8.855	2335	2337	2343	rBV3	506	385	0.01%	0.003%
57	9.314	2479	2480	2481	rBV3	144	41	0.00%	0.000%
58	9.414	2498	2511	2536	rBV	529444	884465	28.79%	6.811%
59	9.559	2554	2556	2559	rBV4	606	344	0.01%	0.003%
60	9.768	2617	2621	2630	rVB5	1165	1803	0.06%	0.014%
61	9.826	2635	2639	2644	rVB2	312	262	0.01%	0.002%
62	9.851	2644	2647	2650	rBV	392	294	0.01%	0.002%
63	9.867	2650	2652	2654	rVB	366	140	0.00%	0.001%
64	9.938	2671	2674	2677	rBV	347	261	0.01%	0.002%
65	10.263	2772	2775	2778	rBV3	340	203	0.01%	0.002%
66	10.424	2822	2825	2829	rBV	261	229	0.01%	0.002%
67	10.594	2874	2878	2883	rBV	413	506	0.02%	0.004%
68	10.629	2887	2889	2895	rVB	272	214	0.01%	0.002%
69	10.755	2915	2928	2951	rBV	466537	748942	24.38%	5.768%
70	11.147	3042	3050	3055	rVB	361	475	0.02%	0.004%
71	11.170	3055	3057	3060	rBV2	179	139	0.00%	0.001%
72	11.305	3096	3099	3100	rBV	299	163	0.01%	0.001%
73	11.481	3151	3154	3155	rBV2	364	241	0.01%	0.002%
74	11.809	3244	3256	3274	rBV	398397	637122	20.74%	4.907%
75	12.002	3313	3316	3317	rBV	398	205	0.01%	0.002%
76	12.137	3356	3358	3361	rBV2	407	215	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
Data File : VU050999.D
Acq On : 29 Sep 2022 23:11
Operator : JC/MD
Sample : N4869-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J37

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Title : VOC Analysis

77	12.192	3362	3375	3398	rVV	485052	790833	25.74%	6.090%
78	12.629	3509	3511	3514	rBV2	455	362	0.01%	0.003%




Sum of corrected areas: 12985050

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
Data File : VU050999.D
Acq On : 29 Sep 2022 23:11
Operator : JC/MD
Sample : N4869-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J37

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

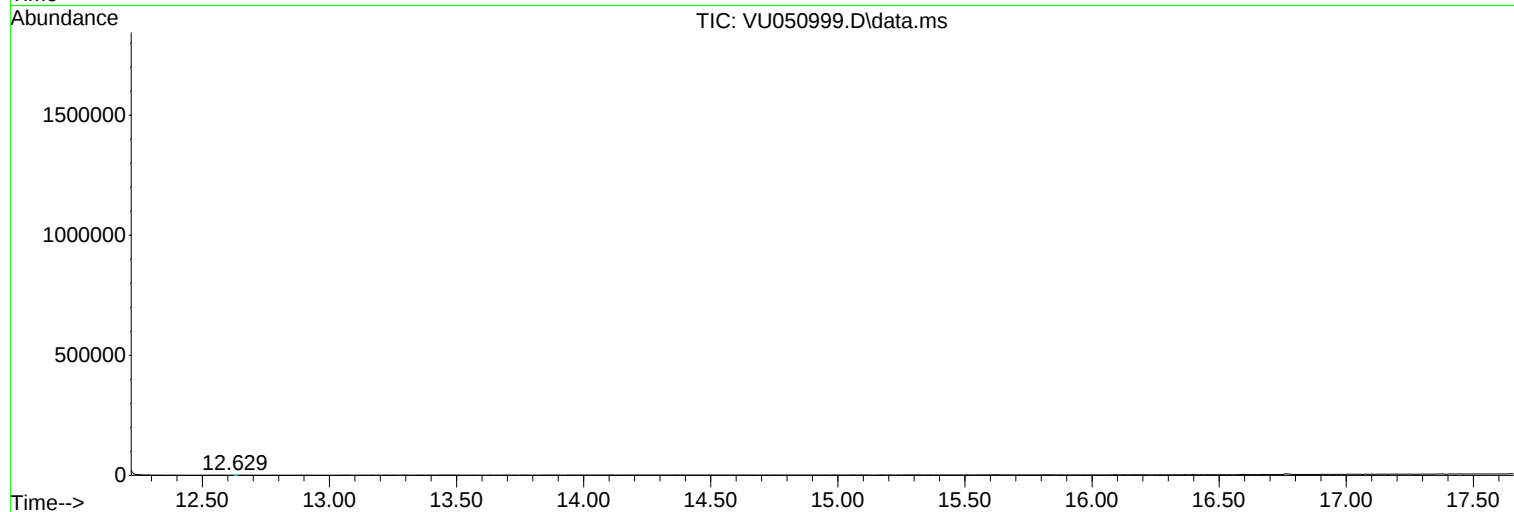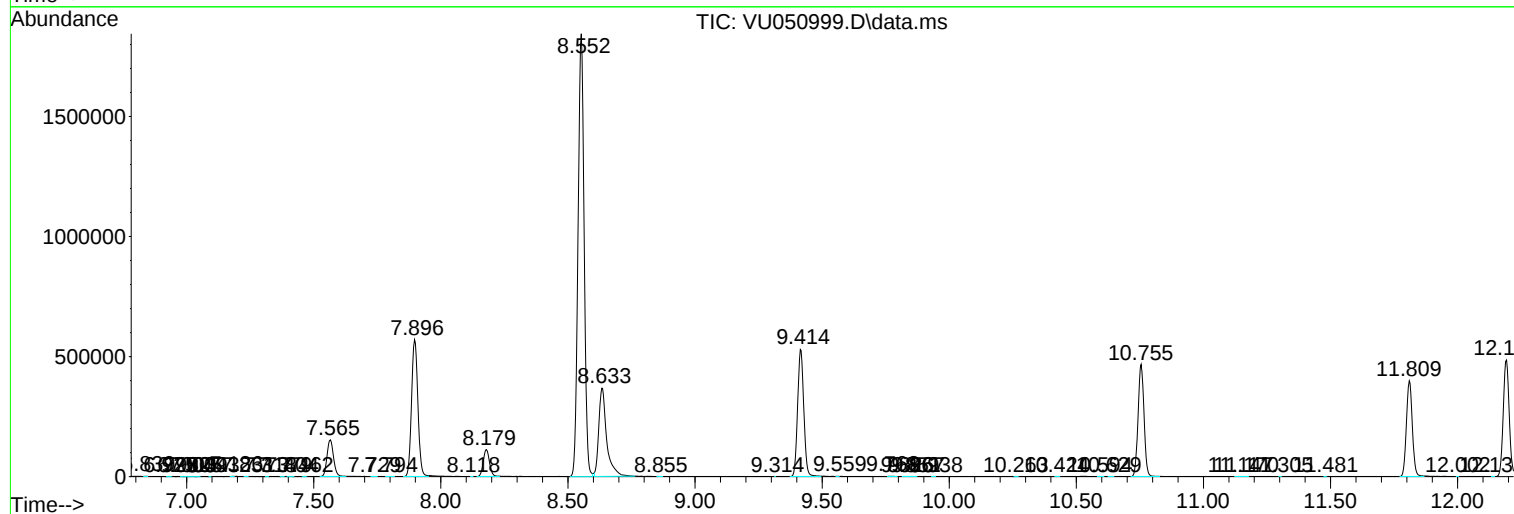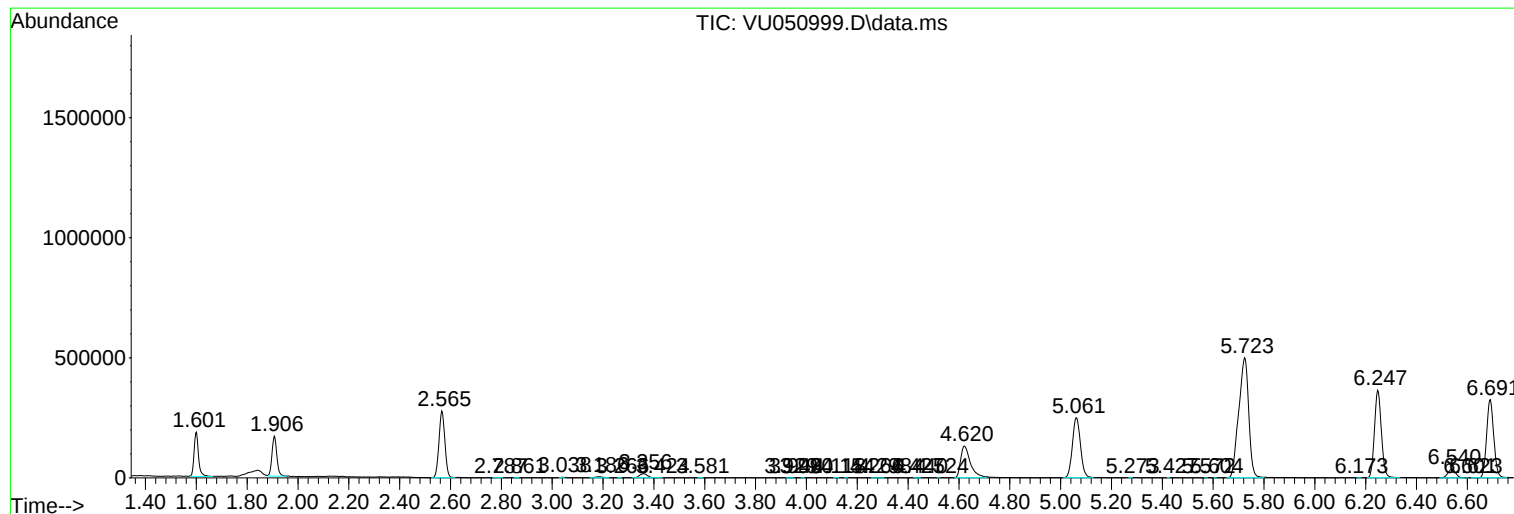

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
Data File : VU050999.D
Acq On : 29 Sep 2022 23:11
Operator : JC/MD
Sample : N4869-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J37

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
Data File : VU050999.D
Acq On : 29 Sep 2022 23:11
Operator : JC/MD
Sample : N4869-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F5J37

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc