

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
 Data File : VU051002.D
 Acq On : 30 Sep 2022 00:45
 Operator : JC/MD
 Sample : VU0929WBL02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK191

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M

Title : VOC Analysis

Signal : TIC: VU051002.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	96	rVB	205705	248330	16.65%	2.274%
2	1.909	169	177	207	rVB	285760	403405	27.04%	3.694%
3	2.511	362	364	368	rVB3	500	214	0.01%	0.002%
4	2.565	368	381	397	rBV	308643	497933	33.38%	4.560%
5	2.732	431	433	436	rBV3	299	227	0.02%	0.002%
6	2.793	443	452	459	rVV2	1454	2358	0.16%	0.022%
7	3.044	521	530	541	rVB3	3980	7160	0.48%	0.066%
8	3.186	559	574	593	rVB	9058	20700	1.39%	0.190%
9	3.292	605	607	610	rVB2	362	209	0.01%	0.002%
10	3.356	623	627	633	rBV5	950	1223	0.08%	0.011%
11	3.584	695	698	702	rBV	260	243	0.02%	0.002%
12	3.629	706	712	714	rBV2	353	286	0.02%	0.003%
13	3.777	754	758	762	rBV2	346	339	0.02%	0.003%
14	3.861	779	784	791	rVB3	526	676	0.05%	0.006%
15	3.922	801	803	808	rVB	322	250	0.02%	0.002%
16	3.996	822	826	827	rBV	331	230	0.02%	0.002%
17	4.073	846	850	852	rBV2	284	258	0.02%	0.002%
18	4.134	865	869	872	rBV	405	364	0.02%	0.003%
19	4.170	875	880	882	rBV2	251	247	0.02%	0.002%
20	4.301	915	921	923	rVB	293	263	0.02%	0.002%
21	4.382	943	946	951	rBV	366	370	0.02%	0.003%
22	4.491	977	980	985	rBV	289	278	0.02%	0.003%
23	4.626	1010	1022	1063	rBV	140927	391208	26.23%	3.582%
24	4.887	1099	1103	1106	rBV3	346	338	0.02%	0.003%
25	4.945	1119	1121	1126	rVB3	377	264	0.02%	0.002%
26	4.980	1128	1132	1138	rVB3	762	676	0.05%	0.006%
27	5.060	1140	1157	1185	rVB	274160	605275	40.58%	5.543%
28	5.211	1202	1204	1213	rVB3	363	298	0.02%	0.003%
29	5.276	1218	1224	1225	rBV3	465	401	0.03%	0.004%
30	5.321	1236	1238	1246	rVB3	873	944	0.06%	0.009%
31	5.375	1251	1255	1256	rBV3	344	258	0.02%	0.002%
32	5.388	1256	1259	1263	rVV3	671	512	0.03%	0.005%
33	5.459	1277	1281	1286	rVV2	275	308	0.02%	0.003%
34	5.533	1299	1304	1308	rVB3	655	718	0.05%	0.007%
35	5.723	1342	1363	1385	rBV2	556018	1491690	100.00%	13.660%
36	6.051	1463	1465	1469	rVB2	411	259	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
 Data File : VU051002.D
 Acq On : 30 Sep 2022 00:45
 Operator : JC/MD
 Sample : VU0929WBL02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK191

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	6.073	1469	1472	1476	rBV3	359	336	0.02%	0.003%
38	6.247	1512	1526	1548	rBV	412333	766118	51.36%	7.016%
39	6.424	1579	1581	1588	rVV4	536	429	0.03%	0.004%
40	6.452	1588	1590	1596	rVB3	642	369	0.02%	0.003%
41	6.526	1603	1613	1632	rVB4	13957	26167	1.75%	0.240%
42	6.600	1632	1636	1641	rBV3	542	478	0.03%	0.004%
43	6.690	1649	1664	1682	rBV	350365	688177	46.13%	6.302%
44	6.951	1743	1745	1750	rBV2	204	207	0.01%	0.002%
45	7.186	1815	1818	1819	rBV	525	239	0.02%	0.002%
46	7.427	1889	1893	1896	rBV2	314	262	0.02%	0.002%
47	7.494	1909	1914	1917	rVV2	205	253	0.02%	0.002%
48	7.565	1922	1936	1953	rBV	165633	295742	19.83%	2.708%
49	7.793	2000	2007	2015	rBV5	1624	2408	0.16%	0.022%
50	7.896	2025	2039	2056	rBV	634009	1086518	72.84%	9.950%
51	8.179	2115	2127	2143	rBV	119595	204431	13.70%	1.872%
52	8.327	2171	2173	2178	rBV3	259	242	0.02%	0.002%
53	8.401	2191	2196	2203	rVB4	1307	1590	0.11%	0.015%
54	8.440	2203	2208	2210	rBV2	365	256	0.02%	0.002%
55	8.552	2232	2243	2255	rVB2	9412	14820	0.99%	0.136%
56	8.636	2256	2269	2308	rBV4	373390	811875	54.43%	7.435%
57	8.925	2354	2359	2360	rBV2	741	733	0.05%	0.007%
58	8.993	2377	2380	2385	rVB2	252	220	0.01%	0.002%
59	9.160	2427	2432	2436	rBV2	264	266	0.02%	0.002%
60	9.333	2480	2486	2488	rBV	247	248	0.02%	0.002%
61	9.417	2498	2512	2538	rBV	579755	972045	65.16%	8.901%
62	9.571	2556	2560	2568	rVB3	2265	2426	0.16%	0.022%
63	9.607	2568	2571	2576	rVB2	288	232	0.02%	0.002%
64	9.632	2576	2579	2582	rBV2	393	326	0.02%	0.003%
65	9.649	2582	2584	2588	rVV3	286	235	0.02%	0.002%
66	9.697	2592	2599	2607	rVB4	1603	2430	0.16%	0.022%
67	9.816	2631	2636	2638	rBV2	297	232	0.02%	0.002%
68	9.835	2638	2642	2647	rVB2	323	286	0.02%	0.003%
69	10.028	2698	2702	2705	rBV	323	256	0.02%	0.002%
70	10.105	2718	2726	2740	rBV8	1939	3801	0.25%	0.035%
71	10.279	2776	2780	2784	rBV2	425	455	0.03%	0.004%
72	10.481	2840	2843	2851	rVB2	1125	1248	0.08%	0.011%
73	10.597	2876	2879	2882	rBV2	295	247	0.02%	0.002%
74	10.755	2915	2928	2947	rBV	496786	798009	53.50%	7.308%
75	11.089	3025	3032	3034	rBV3	698	727	0.05%	0.007%
76	11.176	3057	3059	3064	rVB2	305	221	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
 Data File : VU051002.D
 Acq On : 30 Sep 2022 00:45
 Operator : JC/MD
 Sample : VU0929WBL02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK191

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	11.465	3144	3149	3150	rBV2	913	684	0.05%	0.006%
78	11.558	3173	3178	3181	rBV	237	278	0.02%	0.003%
79	11.748	3230	3237	3244	rBV5	1840	2642	0.18%	0.024%
80	11.809	3244	3256	3278	rBV	434512	685309	45.94%	6.276%
81	11.960	3300	3303	3306	rVB2	425	294	0.02%	0.003%
82	11.992	3310	3313	3318	rVB3	351	302	0.02%	0.003%
83	12.060	3331	3334	3337	rBV2	294	219	0.01%	0.002%
84	12.079	3337	3340	3343	rVB2	384	237	0.02%	0.002%
85	12.192	3361	3375	3399	rBV	508779	832433	55.80%	7.623%
86	12.478	3460	3464	3468	rVB2	287	250	0.02%	0.002%
87	12.500	3468	3471	3474	rVB2	430	260	0.02%	0.002%
88	12.520	3474	3477	3483	rBV4	528	644	0.04%	0.006%
89	12.767	3551	3554	3558	rBV3	387	342	0.02%	0.003%
90	12.854	3576	3581	3584	rBV3	527	424	0.03%	0.004%
91	12.996	3621	3625	3630	rBV4	604	521	0.03%	0.005%
92	13.224	3689	3696	3705	rVB6	2589	3786	0.25%	0.035%
93	13.465	3765	3771	3774	rBV2	607	638	0.04%	0.006%
94	13.664	3830	3833	3840	rVB2	694	659	0.04%	0.006%
95	13.700	3840	3844	3846	rBV2	427	405	0.03%	0.004%
96	13.841	3881	3888	3900	rBV8	3627	5951	0.40%	0.054%
97	13.922	3908	3913	3919	rBV3	637	1020	0.07%	0.009%
98	14.089	3959	3965	3982	rVB2	6757	12010	0.81%	0.110%
99	14.201	3997	4000	4004	rBV3	488	411	0.03%	0.004%
100	14.333	4035	4041	4050	rVB5	4202	6213	0.42%	0.057%




Sum of corrected areas: 10920204

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
Data File : VU051002.D
Acq On : 30 Sep 2022 00:45
Operator : JC/MD
Sample : VU0929WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK191

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

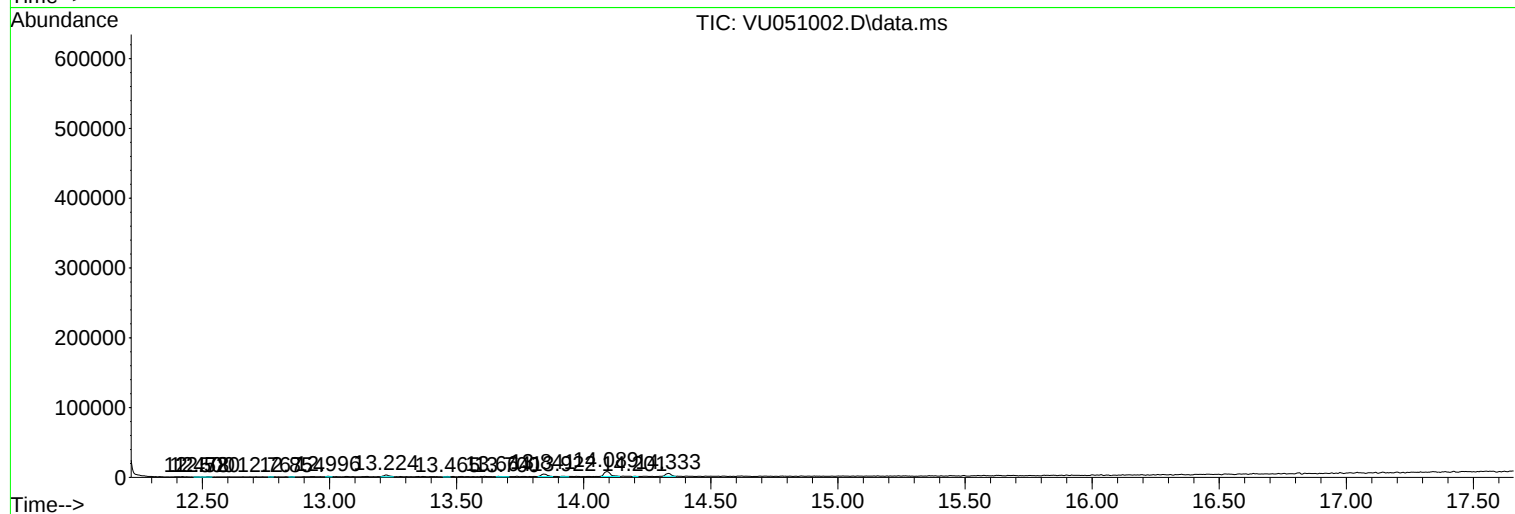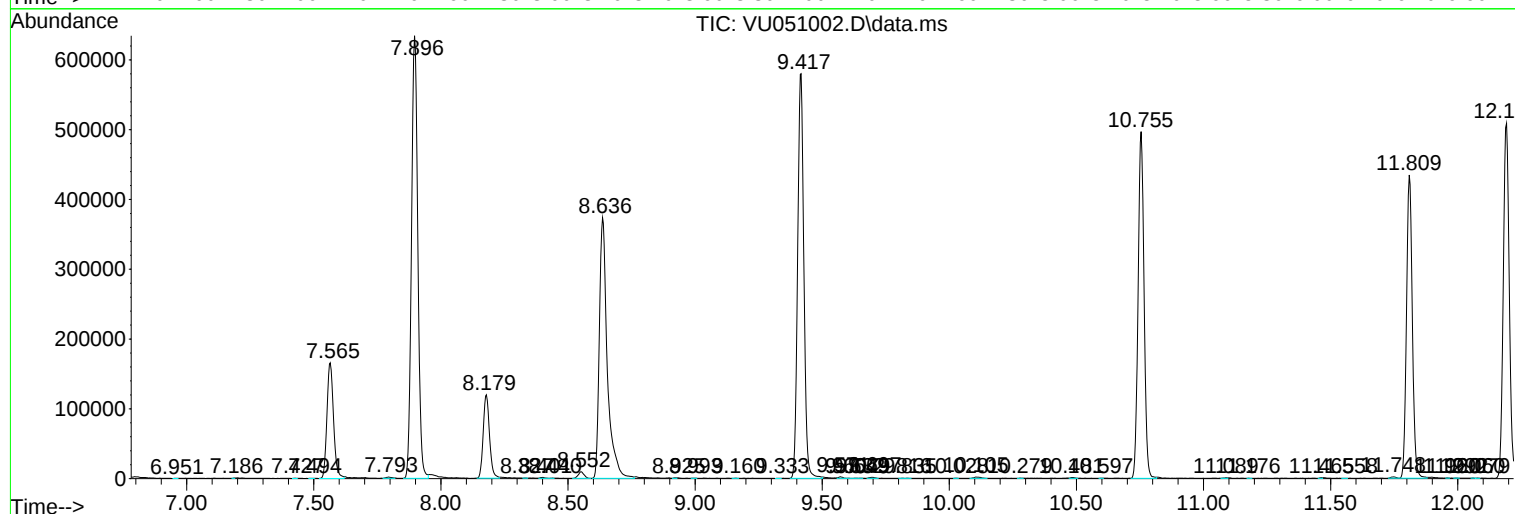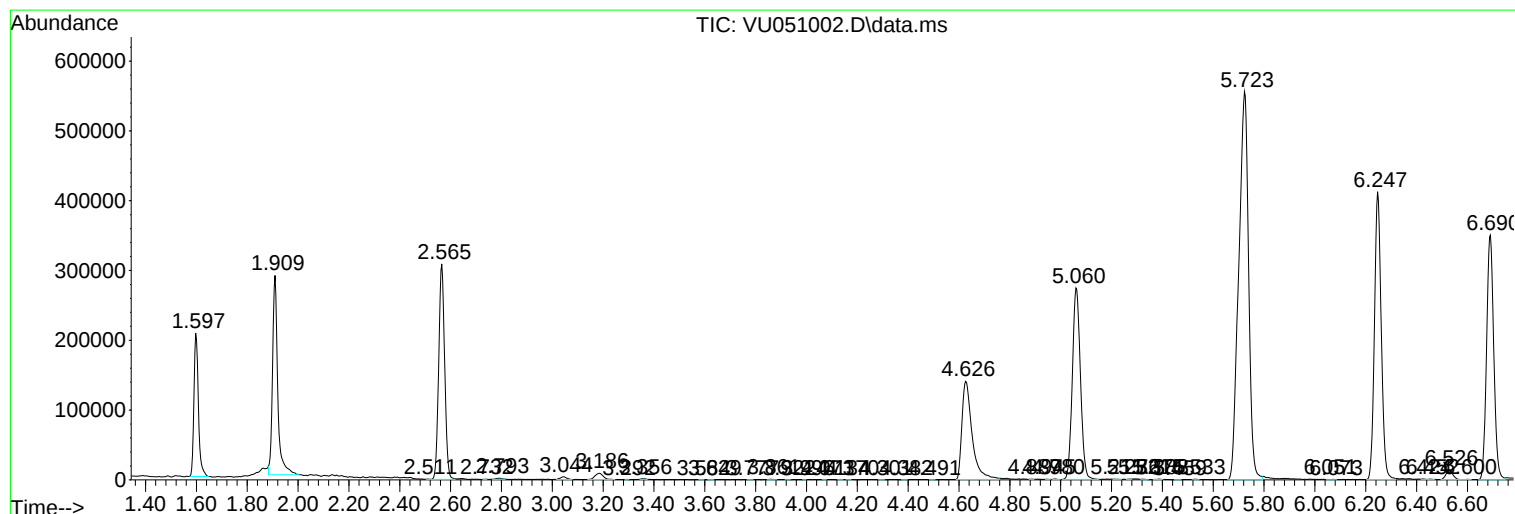

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
Data File : VU051002.D
Acq On : 30 Sep 2022 00:45
Operator : JC/MD
Sample : VU0929WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK191

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
Data File : VU051002.D
Acq On : 30 Sep 2022 00:45
Operator : JC/MD
Sample : VU0929WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK191

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------