

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
 Data File : VU051005.D
 Acq On : 30 Sep 2022 01:55
 Operator : JC/MD
 Sample : N4859-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E10019

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

Signal : TIC: VU051005.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.488	42	46	51	rBV3	5021	4695	0.29%	0.039%
2	1.601	73	81	98	rVB	210007	251155	15.46%	2.097%
3	1.906	169	176	198	rVB	236123	312113	19.21%	2.606%
4	2.565	368	381	395	rBV	331621	535091	32.93%	4.467%
5	2.633	396	402	417	rVB	8410	15571	0.96%	0.130%
6	2.793	440	452	456	rBV5	2224	4052	0.25%	0.034%
7	3.041	522	529	542	rBV5	2169	3660	0.23%	0.031%
8	3.096	542	546	549	rVB	339	264	0.02%	0.002%
9	3.186	565	574	582	rBV5	1846	3646	0.22%	0.030%
10	3.256	593	596	600	rVB2	354	251	0.02%	0.002%
11	3.620	706	709	713	rVB	295	231	0.01%	0.002%
12	3.781	753	759	762	rVB	535	422	0.03%	0.004%
13	3.816	767	770	777	rVB2	281	240	0.01%	0.002%
14	4.086	846	854	856	rBV	314	419	0.03%	0.003%
15	4.234	897	900	906	rVB2	333	309	0.02%	0.003%
16	4.433	960	962	967	rVB2	387	292	0.02%	0.002%
17	4.568	999	1004	1007	rVV3	226	246	0.02%	0.002%
18	4.623	1007	1021	1069	rBV	157032	432077	26.59%	3.607%
19	4.909	1106	1110	1114	rVB4	560	522	0.03%	0.004%
20	4.935	1114	1118	1120	rBV3	400	292	0.02%	0.002%
21	5.063	1141	1158	1190	rBV2	321799	847282	52.14%	7.073%
22	5.285	1223	1227	1228	rBV2	793	531	0.03%	0.004%
23	5.372	1250	1254	1255	rBV	498	328	0.02%	0.003%
24	5.420	1266	1269	1275	rVB	380	340	0.02%	0.003%
25	5.723	1337	1363	1386	rBV2	603018	1624862	100.00%	13.565%
26	6.080	1470	1474	1479	rVB3	339	380	0.02%	0.003%
27	6.186	1503	1507	1512	rBV2	177	232	0.01%	0.002%
28	6.247	1512	1526	1546	rBV	445716	849255	52.27%	7.090%
29	6.407	1574	1576	1579	rBV3	570	310	0.02%	0.003%
30	6.453	1588	1590	1596	rVB3	428	384	0.02%	0.003%
31	6.530	1596	1614	1626	rBV	18012	34934	2.15%	0.292%
32	6.626	1640	1644	1648	rVB3	408	309	0.02%	0.003%
33	6.687	1648	1663	1683	rBV	379605	751288	46.24%	6.272%
34	7.044	1772	1774	1780	rVB2	264	246	0.02%	0.002%
35	7.105	1780	1793	1804	rBV3	9388	17599	1.08%	0.147%
36	7.176	1811	1815	1816	rBV	645	375	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
 Data File : VU051005.D
 Acq On : 30 Sep 2022 01:55
 Operator : JC/MD
 Sample : N4859-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E10019

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	7.186	1816	1818	1822	rVV3	829	687	0.04%	0.006%
38	7.266	1839	1843	1846	rBV2	280	233	0.01%	0.002%
39	7.414	1882	1889	1892	rBV3	306	394	0.02%	0.003%
40	7.491	1904	1913	1918	rBV2	300	457	0.03%	0.004%
41	7.565	1922	1936	1956	rBV	178918	320042	19.70%	2.672%
42	7.793	1997	2007	2024	rBV4	5429	10694	0.66%	0.089%
43	7.896	2024	2039	2058	rBV	676434	1156058	71.15%	9.651%
44	8.092	2096	2100	2104	rVB3	525	436	0.03%	0.004%
45	8.112	2104	2106	2113	rVB2	426	359	0.02%	0.003%
46	8.179	2113	2127	2144	rBV	129292	220395	13.56%	1.840%
47	8.340	2174	2177	2181	rVB3	632	408	0.03%	0.003%
48	8.382	2186	2190	2197	rVB2	380	381	0.02%	0.003%
49	8.420	2198	2202	2203	rBV2	387	299	0.02%	0.002%
50	8.475	2214	2219	2226	rVB2	616	837	0.05%	0.007%
51	8.552	2231	2243	2252	rBV6	5185	8446	0.52%	0.071%
52	8.636	2256	2269	2305	rBV3	418772	916143	56.38%	7.648%
53	8.858	2336	2338	2341	rVB2	646	403	0.02%	0.003%
54	8.883	2342	2346	2349	rBV2	288	263	0.02%	0.002%
55	8.970	2369	2373	2375	rBV2	338	253	0.02%	0.002%
56	8.999	2380	2382	2387	rVV2	366	381	0.02%	0.003%
57	9.263	2460	2464	2468	rVV	353	385	0.02%	0.003%
58	9.346	2486	2490	2494	rVB	445	388	0.02%	0.003%
59	9.417	2494	2512	2542	rBV	647262	1074093	66.10%	8.967%
60	9.571	2551	2560	2570	rVB3	9040	14415	0.89%	0.120%
61	9.652	2582	2585	2589	rBV3	308	258	0.02%	0.002%
62	9.690	2589	2597	2611	rVB3	15818	26616	1.64%	0.222%
63	10.015	2694	2698	2702	rBV	257	253	0.02%	0.002%
64	10.041	2703	2706	2709	rVV2	324	249	0.02%	0.002%
65	10.102	2716	2725	2740	rVV3	9088	15592	0.96%	0.130%
66	10.266	2771	2776	2781	rBV2	291	307	0.02%	0.003%
67	10.404	2815	2819	2820	rBV	392	241	0.01%	0.002%
68	10.484	2841	2844	2848	rBV2	475	355	0.02%	0.003%
69	10.581	2870	2874	2877	rBV	485	308	0.02%	0.003%
70	10.600	2877	2880	2884	rVB	376	274	0.02%	0.002%
71	10.755	2914	2928	2951	rVV	534556	857488	52.77%	7.159%
72	10.896	2969	2972	2976	rVB3	748	618	0.04%	0.005%
73	10.973	2990	2996	3001	rBV2	492	486	0.03%	0.004%
74	11.009	3004	3007	3013	rVB	414	290	0.02%	0.002%
75	11.044	3014	3018	3020	rBV	416	317	0.02%	0.003%
76	11.118	3039	3041	3044	rVB2	442	273	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
 Data File : VU051005.D
 Acq On : 30 Sep 2022 01:55
 Operator : JC/MD
 Sample : N4859-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E10019

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	11.166	3053	3056	3061	rVB	407	314	0.02%	0.003%
78	11.195	3061	3065	3067	rBV	365	314	0.02%	0.003%
79	11.317	3100	3103	3105	rBV	435	256	0.02%	0.002%
80	11.484	3137	3155	3162	rBV7	1337	3326	0.20%	0.028%
81	11.748	3233	3237	3244	rBV4	286	310	0.02%	0.003%
82	11.809	3244	3256	3275	rBV	479152	751793	46.27%	6.276%
83	11.967	3302	3305	3308	rBV2	298	247	0.02%	0.002%
84	12.070	3330	3337	3341	rBV5	1687	1950	0.12%	0.016%
85	12.192	3362	3375	3392	rBV	542095	888666	54.69%	7.419%
86	12.446	3449	3454	3457	rBV2	383	327	0.02%	0.003%
87	12.642	3512	3515	3517	rBV	311	233	0.01%	0.002%
88	12.774	3553	3556	3561	rVB	641	424	0.03%	0.004%
89	12.899	3593	3595	3598	rVB3	566	280	0.02%	0.002%
90	12.957	3610	3613	3618	rVB	508	357	0.02%	0.003%
91	13.028	3629	3635	3636	rBV2	856	825	0.05%	0.007%
92	13.172	3677	3680	3683	rVV2	367	250	0.02%	0.002%
93	13.468	3768	3772	3776	rBV2	461	474	0.03%	0.004%
94	13.980	3929	3931	3937	rBV2	361	305	0.02%	0.003%
95	14.420	4063	4068	4069	rBV	507	375	0.02%	0.003%
96	15.250	4324	4326	4328	rBV	617	312	0.02%	0.003%
97	15.307	4342	4344	4346	rBV	504	246	0.02%	0.002%
98	15.330	4349	4351	4356	rBV3	695	612	0.04%	0.005%
99	15.787	4489	4493	4495	rBV2	733	615	0.04%	0.005%
100	15.899	4525	4528	4533	rVB5	892	768	0.05%	0.006%



Sum of corrected areas: 11978557

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
Data File : VU051005.D
Acq On : 30 Sep 2022 01:55
Operator : JC/MD
Sample : N4859-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E10019

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

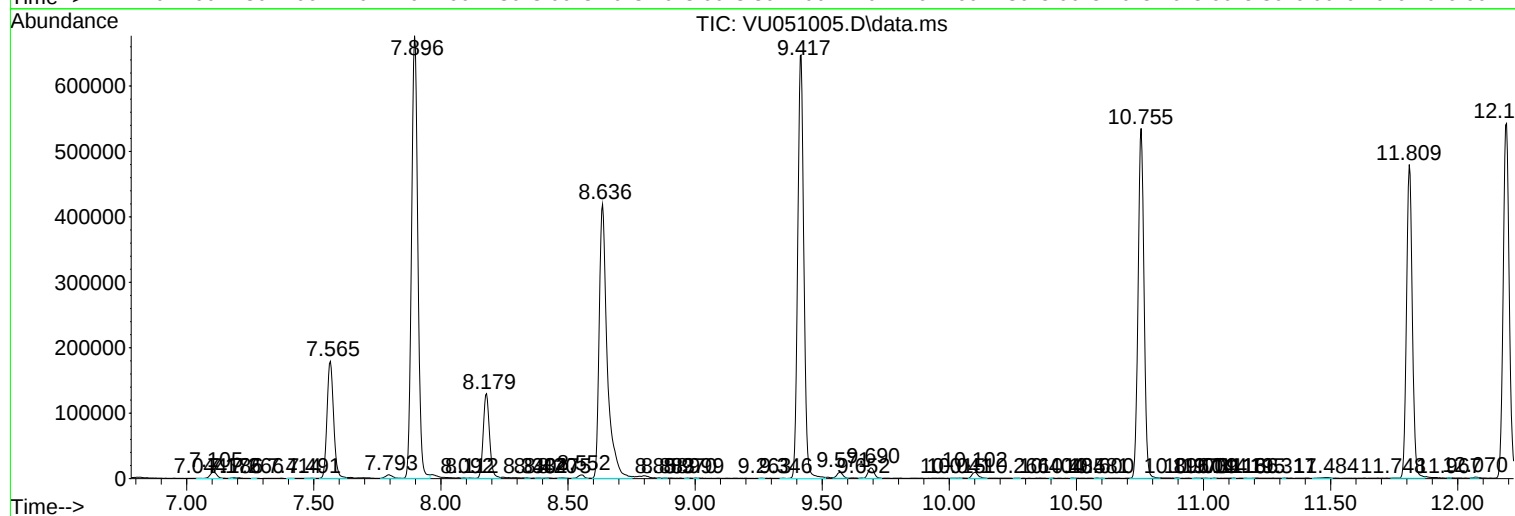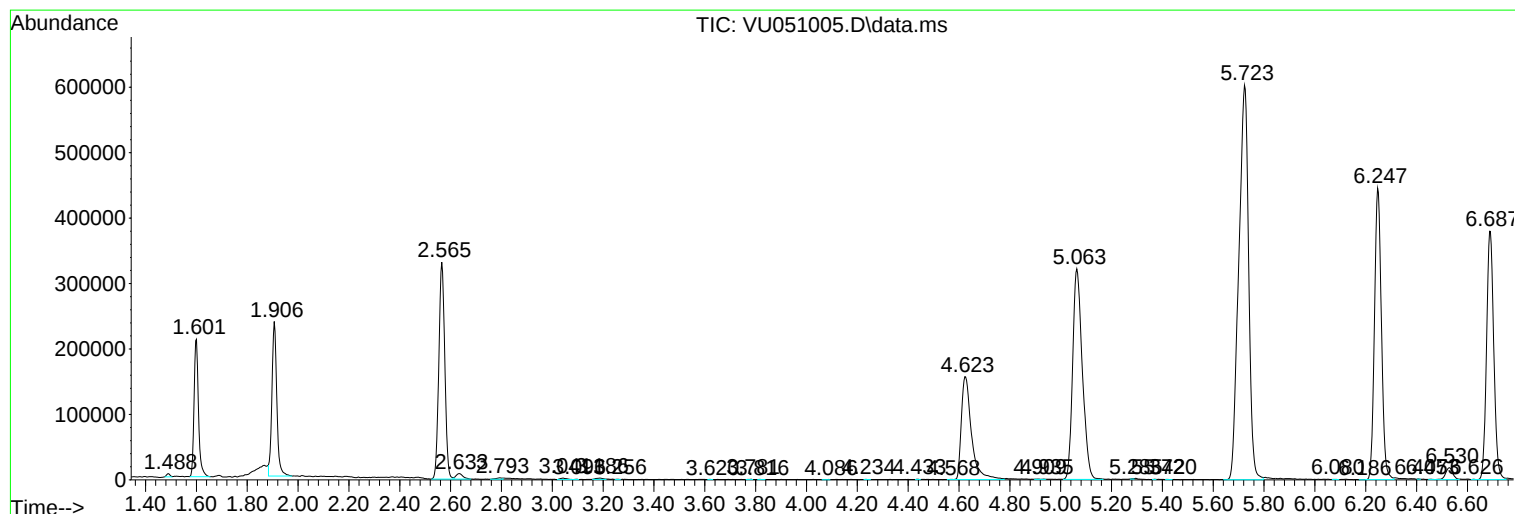

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
Data File : VU051005.D
Acq On : 30 Sep 2022 01:55
Operator : JC/MD
Sample : N4859-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E10019

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
Data File : VU051005.D
Acq On : 30 Sep 2022 01:55
Operator : JC/MD
Sample : N4859-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E10019

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc