

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
 Data File : VU051006.D
 Acq On : 30 Sep 2022 02:19
 Operator : JC/MD
 Sample : N4859-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E10020

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

Signal : TIC: VU051006.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	97	rVB	193672	227535	15.33%	2.052%
2	1.912	170	178	201	rVB	221168	293253	19.76%	2.645%
3	2.565	368	381	396	rBV	279964	452153	30.46%	4.078%
4	2.784	446	449	451	rBV3	420	288	0.02%	0.003%
5	3.051	523	532	540	rVB4	1635	2797	0.19%	0.025%
6	3.173	568	570	571	rBV4	530	258	0.02%	0.002%
7	3.263	593	598	604	rVB2	250	332	0.02%	0.003%
8	3.353	620	626	631	rBV2	284	279	0.02%	0.003%
9	3.440	650	653	657	rBV2	380	357	0.02%	0.003%
10	3.620	705	709	714	rBV2	297	386	0.03%	0.003%
11	3.870	785	787	794	rBV2	196	242	0.02%	0.002%
12	3.973	816	819	824	rVB2	346	276	0.02%	0.002%
13	4.018	824	833	836	rBV2	362	600	0.04%	0.005%
14	4.124	861	866	869	rBV	287	275	0.02%	0.002%
15	4.198	883	889	891	rBV	285	295	0.02%	0.003%
16	4.449	962	967	974	rBV4	377	414	0.03%	0.004%
17	4.629	1009	1023	1067	rBV	128986	369495	24.90%	3.333%
18	5.063	1138	1158	1188	rBV2	284583	759630	51.18%	6.852%
19	5.282	1219	1226	1227	rBV4	725	786	0.05%	0.007%
20	5.321	1236	1238	1242	rVB3	570	356	0.02%	0.003%
21	5.340	1242	1244	1249	rVB2	294	256	0.02%	0.002%
22	5.375	1249	1255	1260	rBV4	551	710	0.05%	0.006%
23	5.401	1260	1263	1266	rVB2	356	266	0.02%	0.002%
24	5.722	1342	1363	1394	rBV2	541288	1484206	100.00%	13.387%
25	5.976	1439	1442	1447	rBV3	420	372	0.03%	0.003%
26	6.034	1457	1460	1465	rVB2	457	333	0.02%	0.003%
27	6.060	1465	1468	1475	rVV2	488	369	0.02%	0.003%
28	6.156	1496	1498	1502	rBV2	462	284	0.02%	0.003%
29	6.247	1512	1526	1549	rBV	416039	785118	52.90%	7.082%
30	6.529	1602	1614	1626	rVV2	16569	30911	2.08%	0.279%
31	6.591	1630	1633	1639	rBV5	486	578	0.04%	0.005%
32	6.690	1646	1664	1684	rBV	396514	772156	52.02%	6.965%
33	6.873	1718	1721	1724	rBV3	449	298	0.02%	0.003%
34	7.102	1782	1792	1806	rVB3	8342	15113	1.02%	0.136%
35	7.192	1816	1820	1824	rBV3	510	575	0.04%	0.005%
36	7.565	1919	1936	1955	rBV	164445	290055	19.54%	2.616%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
 Data File : VU051006.D
 Acq On : 30 Sep 2022 02:19
 Operator : JC/MD
 Sample : N4859-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E10020

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	7.796	2005	2008	2010	rBV2	475	329	0.02%	0.003%
38	7.896	2024	2039	2055	rBV	692582	1176101	79.24%	10.608%
39	8.118	2106	2108	2112	rVB2	420	236	0.02%	0.002%
40	8.179	2115	2127	2146	rBV2	139888	240575	16.21%	2.170%
41	8.452	2210	2212	2216	rBV2	392	354	0.02%	0.003%
42	8.468	2216	2217	2220	rBV3	368	246	0.02%	0.002%
43	8.552	2235	2243	2251	rVB6	5872	8893	0.60%	0.080%
44	8.635	2256	2269	2305	rBV4	442783	994954	67.04%	8.974%
45	8.883	2343	2346	2348	rBV2	426	243	0.02%	0.002%
46	8.951	2364	2367	2371	rVB2	434	348	0.02%	0.003%
47	9.111	2411	2417	2420	rBV2	277	253	0.02%	0.002%
48	9.195	2440	2443	2449	rVB2	295	312	0.02%	0.003%
49	9.227	2449	2453	2455	rBV2	277	259	0.02%	0.002%
50	9.417	2499	2512	2536	rBV	565406	942930	63.53%	8.505%
51	9.565	2557	2558	2563	rVB2	518	369	0.02%	0.003%
52	9.632	2577	2579	2583	rVB2	346	243	0.02%	0.002%
53	9.680	2591	2594	2595	rVV2	743	456	0.03%	0.004%
54	9.693	2595	2598	2606	rVB3	1875	1873	0.13%	0.017%
55	9.864	2646	2651	2655	rBV	398	394	0.03%	0.004%
56	9.912	2664	2666	2671	rBV	241	244	0.02%	0.002%
57	10.012	2690	2697	2700	rBV2	328	328	0.02%	0.003%
58	10.089	2717	2721	2723	rBV	443	321	0.02%	0.003%
59	10.102	2723	2725	2728	rVV2	557	326	0.02%	0.003%
60	10.484	2840	2844	2847	rBV	301	276	0.02%	0.002%
61	10.590	2873	2877	2884	rBV	423	593	0.04%	0.005%
62	10.754	2914	2928	2946	rBV	467572	752395	50.69%	6.787%
63	11.021	3006	3011	3015	rVB2	335	300	0.02%	0.003%
64	11.050	3016	3020	3023	rBV2	341	299	0.02%	0.003%
65	11.105	3034	3037	3041	rBV2	417	404	0.03%	0.004%
66	11.185	3059	3062	3069	rBV	378	388	0.03%	0.003%
67	11.433	3135	3139	3142	rBV	382	373	0.03%	0.003%
68	11.452	3142	3145	3148	rVV	482	382	0.03%	0.003%
69	11.484	3148	3155	3162	rVV4	1388	1864	0.13%	0.017%
70	11.626	3196	3199	3203	rVB2	345	320	0.02%	0.003%
71	11.664	3208	3211	3216	rBV2	251	311	0.02%	0.003%
72	11.745	3233	3236	3242	rVB2	877	740	0.05%	0.007%
73	11.809	3242	3256	3272	rBV	414454	665156	44.82%	6.000%
74	11.918	3288	3290	3294	rVB2	836	428	0.03%	0.004%
75	12.057	3329	3333	3334	rBV2	638	404	0.03%	0.004%
76	12.124	3352	3354	3358	rVB2	516	349	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
 Data File : VU051006.D
 Acq On : 30 Sep 2022 02:19
 Operator : JC/MD
 Sample : N4859-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E10020

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	12.192	3359	3375	3392	rBV	483981	789755	53.21%	7.124%
78	12.401	3438	3440	3441	rBV	520	255	0.02%	0.002%
79	12.465	3456	3460	3464	rBV3	474	499	0.03%	0.005%
80	12.487	3464	3467	3469	rVV2	550	329	0.02%	0.003%
81	12.507	3471	3473	3478	rVV4	573	450	0.03%	0.004%
82	12.532	3479	3481	3485	rVB	643	405	0.03%	0.004%
83	12.558	3485	3489	3496	rBV2	610	755	0.05%	0.007%
84	12.671	3519	3524	3525	rBV2	340	254	0.02%	0.002%
85	12.732	3535	3543	3547	rBV3	498	678	0.05%	0.006%
86	12.905	3593	3597	3599	rBV2	379	266	0.02%	0.002%
87	13.015	3627	3631	3633	rBV	390	306	0.02%	0.003%
88	13.230	3694	3698	3704	rBV4	678	744	0.05%	0.007%
89	13.330	3727	3729	3732	rBV2	431	245	0.02%	0.002%
90	13.455	3764	3768	3771	rBV	548	397	0.03%	0.004%
91	13.870	3894	3897	3899	rBV2	393	293	0.02%	0.003%
92	14.272	4018	4022	4027	rBV3	558	571	0.04%	0.005%
93	14.799	4183	4186	4188	rBV2	453	245	0.02%	0.002%
94	14.876	4207	4210	4213	rBV2	404	295	0.02%	0.003%
95	15.111	4280	4283	4291	rBV2	568	620	0.04%	0.006%
96	15.246	4323	4325	4329	rBV2	395	328	0.02%	0.003%
97	15.423	4378	4380	4384	rVB3	556	357	0.02%	0.003%
98	15.478	4395	4397	4400	rBV4	603	304	0.02%	0.003%
99	15.664	4452	4455	4457	rBV2	859	512	0.03%	0.005%
100	15.703	4464	4467	4470	rBV2	693	549	0.04%	0.005%


Sum of corrected areas: 11086588

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
Data File : VU051006.D
Acq On : 30 Sep 2022 02:19
Operator : JC/MD
Sample : N4859-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E10020

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

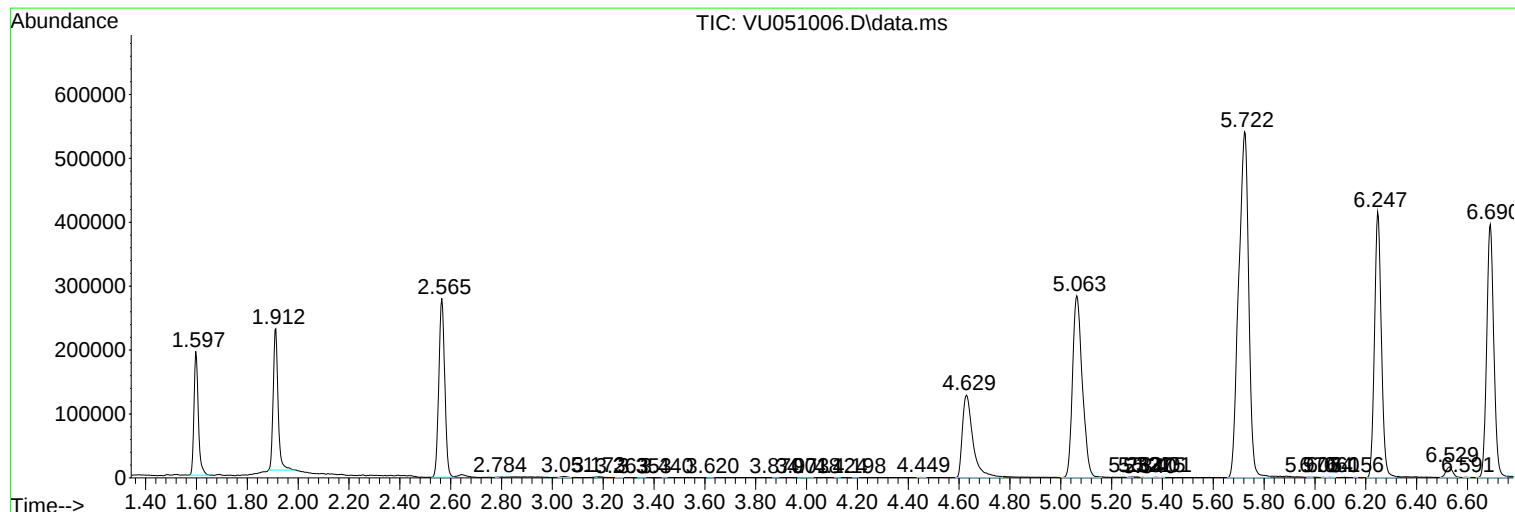

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
Data File : VU051006.D
Acq On : 30 Sep 2022 02:19
Operator : JC/MD
Sample : N4859-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E10020

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
Data File : VU051006.D
Acq On : 30 Sep 2022 02:19
Operator : JC/MD
Sample : N4859-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E10020

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc