

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
 Data File : VU051007.D
 Acq On : 30 Sep 2022 02:42
 Operator : JC/MD
 Sample : N4859-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E10022

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

Signal : TIC: VU051007.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	99	rVB	183037	217705	15.40%	1.934%
2	1.903	167	175	194	rVB	169534	234428	16.58%	2.082%
3	2.565	367	381	394	rBV	283519	453747	32.10%	4.030%
4	2.629	395	401	413	rVB2	5211	9235	0.65%	0.082%
5	2.761	436	442	444	rBV5	1327	1131	0.08%	0.010%
6	2.780	444	448	452	rBV4	1494	1862	0.13%	0.017%
7	2.951	499	501	508	rVB3	365	276	0.02%	0.002%
8	3.044	523	530	537	rVB4	1556	2481	0.18%	0.022%
9	3.137	556	559	563	rVB3	331	246	0.02%	0.002%
10	3.179	563	572	574	rBV	1769	2157	0.15%	0.019%
11	3.288	602	606	609	rBV2	559	468	0.03%	0.004%
12	3.842	775	778	781	rBV	271	224	0.02%	0.002%
13	4.256	903	907	911	rVB2	256	258	0.02%	0.002%
14	4.369	938	942	945	rBV2	260	234	0.02%	0.002%
15	4.443	961	965	969	rVB2	416	358	0.03%	0.003%
16	4.481	969	977	979	rBV2	327	466	0.03%	0.004%
17	4.620	1005	1020	1050	rBV	131996	350013	24.76%	3.109%
18	4.848	1088	1091	1097	rVB3	435	439	0.03%	0.004%
19	4.967	1126	1128	1131	rBV	267	232	0.02%	0.002%
20	5.063	1141	1158	1183	rBV3	275738	730689	51.69%	6.490%
21	5.189	1193	1197	1200	rBV4	326	269	0.02%	0.002%
22	5.337	1241	1243	1247	rBV3	523	361	0.03%	0.003%
23	5.417	1265	1268	1270	rBV2	396	253	0.02%	0.002%
24	5.722	1342	1363	1385	rBV2	528320	1413660	100.00%	12.557%
25	5.867	1406	1408	1411	rBV3	631	366	0.03%	0.003%
26	5.906	1417	1420	1428	rVB5	1414	1588	0.11%	0.014%
27	5.944	1429	1432	1435	rVB3	1010	607	0.04%	0.005%
28	5.967	1435	1439	1440	rBV3	331	204	0.01%	0.002%
29	6.047	1460	1464	1470	rVB3	790	877	0.06%	0.008%
30	6.079	1470	1474	1477	rBV2	261	271	0.02%	0.002%
31	6.247	1508	1526	1550	rBV	411834	780244	55.19%	6.931%
32	6.378	1564	1567	1570	rBV2	533	329	0.02%	0.003%
33	6.530	1602	1614	1627	rBV2	18673	35855	2.54%	0.318%
34	6.690	1647	1664	1685	rBV	359965	702155	49.67%	6.237%
35	6.800	1696	1698	1700	rBV3	856	507	0.04%	0.005%
36	7.018	1763	1766	1770	rVB	346	214	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
 Data File : VU051007.D
 Acq On : 30 Sep 2022 02:42
 Operator : JC/MD
 Sample : N4859-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E10022

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	7.105	1781	1793	1808	rBV3	9824	18087	1.28%	0.161%
38	7.189	1814	1819	1824	rVV4	1251	1353	0.10%	0.012%
39	7.401	1880	1885	1889	rBV	297	344	0.02%	0.003%
40	7.443	1893	1898	1901	rBV2	314	296	0.02%	0.003%
41	7.491	1911	1913	1917	rVB	475	326	0.02%	0.003%
42	7.565	1917	1936	1952	rBV	192528	338950	23.98%	3.011%
43	7.896	2025	2039	2057	rBV	695527	1199247	84.83%	10.652%
44	8.179	2114	2127	2146	rBV	134412	232430	16.44%	2.065%
45	8.382	2187	2190	2195	rVB4	434	455	0.03%	0.004%
46	8.449	2207	2211	2214	rBV4	500	462	0.03%	0.004%
47	8.552	2231	2243	2250	rBV6	5063	7659	0.54%	0.068%
48	8.636	2255	2269	2307	rBV3	419887	914691	64.70%	8.125%
49	8.864	2337	2340	2342	rVB2	459	250	0.02%	0.002%
50	8.896	2347	2350	2353	rVB2	363	247	0.02%	0.002%
51	9.031	2389	2392	2396	rVB2	367	255	0.02%	0.002%
52	9.066	2398	2403	2407	rBV2	243	301	0.02%	0.003%
53	9.414	2498	2511	2532	rBV	601736	1002072	70.88%	8.901%
54	9.648	2581	2584	2585	rBV	461	210	0.01%	0.002%
55	9.693	2591	2598	2608	rVB4	1918	2727	0.19%	0.024%
56	10.021	2692	2700	2703	rBV	404	500	0.04%	0.004%
57	10.092	2719	2722	2724	rBV2	681	491	0.03%	0.004%
58	10.317	2789	2792	2796	rVB	311	210	0.01%	0.002%
59	10.346	2798	2801	2804	rBV	440	321	0.02%	0.003%
60	10.362	2804	2806	2810	rVB2	315	200	0.01%	0.002%
61	10.439	2827	2830	2831	rBV2	352	198	0.01%	0.002%
62	10.754	2915	2928	2955	rBV	567618	916938	64.86%	8.145%
63	10.938	2982	2985	2989	rVB2	411	245	0.02%	0.002%
64	11.086	3028	3031	3034	rBV2	454	326	0.02%	0.003%
65	11.147	3048	3050	3053	rVB	373	214	0.02%	0.002%
66	11.169	3053	3057	3060	rBV3	270	239	0.02%	0.002%
67	11.188	3060	3063	3066	rBV2	280	202	0.01%	0.002%
68	11.407	3127	3131	3133	rBV2	351	258	0.02%	0.002%
69	11.439	3138	3141	3145	rVV2	296	240	0.02%	0.002%
70	11.481	3147	3154	3165	rVB5	1189	2379	0.17%	0.021%
71	11.587	3185	3187	3190	rVB	413	249	0.02%	0.002%
72	11.742	3232	3235	3240	rBV3	493	572	0.04%	0.005%
73	11.809	3244	3256	3276	rBV	472449	752515	53.23%	6.684%
74	12.002	3313	3316	3320	rBV2	502	474	0.03%	0.004%
75	12.069	3330	3337	3342	rBV4	1460	2377	0.17%	0.021%
76	12.192	3361	3375	3394	rBV	553954	904962	64.02%	8.038%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
 Data File : VU051007.D
 Acq On : 30 Sep 2022 02:42
 Operator : JC/MD
 Sample : N4859-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E10022

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	12.446	3451	3454	3458	rBV3	386	316	0.02%	0.003%
78	12.735	3541	3544	3548	rVV3	374	273	0.02%	0.002%
79	12.803	3563	3565	3570	rVB3	353	295	0.02%	0.003%
80	12.864	3582	3584	3587	rBV	337	228	0.02%	0.002%
81	12.979	3617	3620	3624	rBV2	484	363	0.03%	0.003%
82	13.008	3626	3629	3633	rVB3	419	388	0.03%	0.003%
83	13.047	3638	3641	3645	rVV	448	332	0.02%	0.003%
84	13.143	3667	3671	3678	rBV2	479	634	0.04%	0.006%
85	13.221	3693	3695	3701	rVB4	513	351	0.02%	0.003%
86	13.430	3758	3760	3763	rBV2	459	352	0.02%	0.003%
87	13.722	3848	3851	3857	rBV3	314	288	0.02%	0.003%
88	13.912	3907	3910	3912	rBV2	359	264	0.02%	0.002%
89	14.053	3951	3954	3955	rBV	349	229	0.02%	0.002%
90	14.330	4037	4040	4041	rBV2	557	328	0.02%	0.003%
91	14.590	4117	4121	4125	rBV2	542	391	0.03%	0.003%
92	14.613	4126	4128	4130	rBV	378	222	0.02%	0.002%
93	14.844	4197	4200	4204	rVB3	490	365	0.03%	0.003%
94	14.938	4227	4229	4231	rBV	434	261	0.02%	0.002%
95	15.529	4410	4413	4415	rBV2	655	342	0.02%	0.003%
96	15.677	4455	4459	4463	rVB4	570	586	0.04%	0.005%
97	15.725	4472	4474	4476	rBV2	460	218	0.02%	0.002%
98	15.854	4512	4514	4517	rBV3	609	382	0.03%	0.003%
99	15.918	4529	4534	4537	rBV3	914	974	0.07%	0.009%
100	16.339	4663	4665	4669	rBV3	850	676	0.05%	0.006%




Sum of corrected areas: 11257939

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
Data File : VU051007.D
Acq On : 30 Sep 2022 02:42
Operator : JC/MD
Sample : N4859-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E10022

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

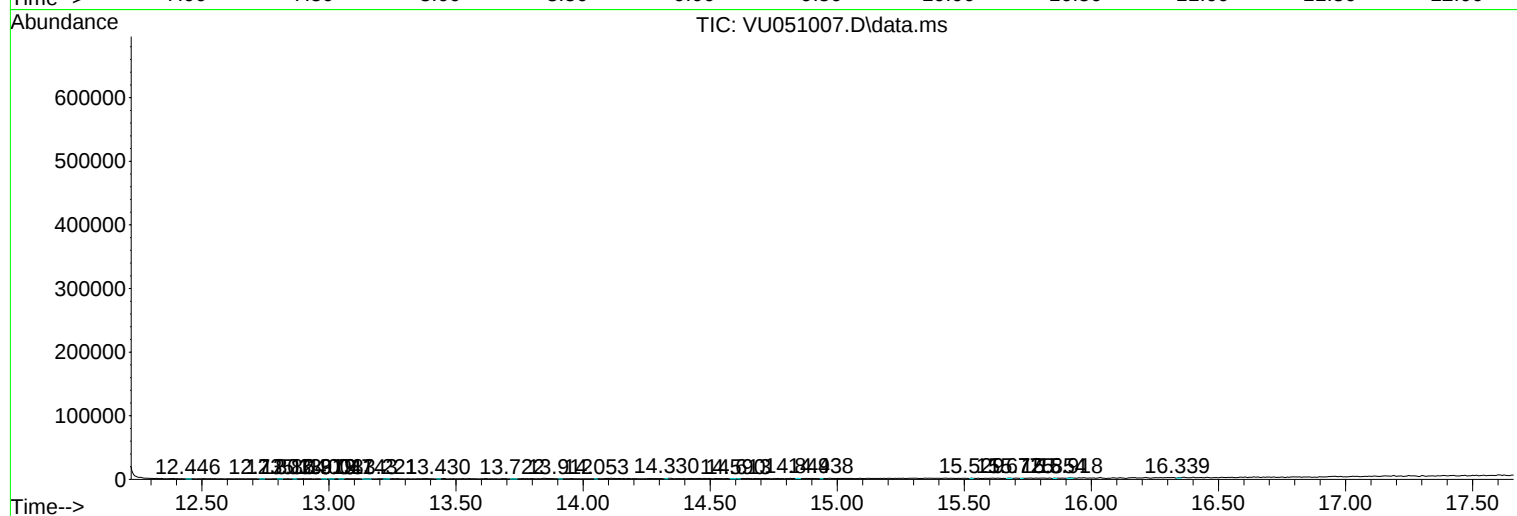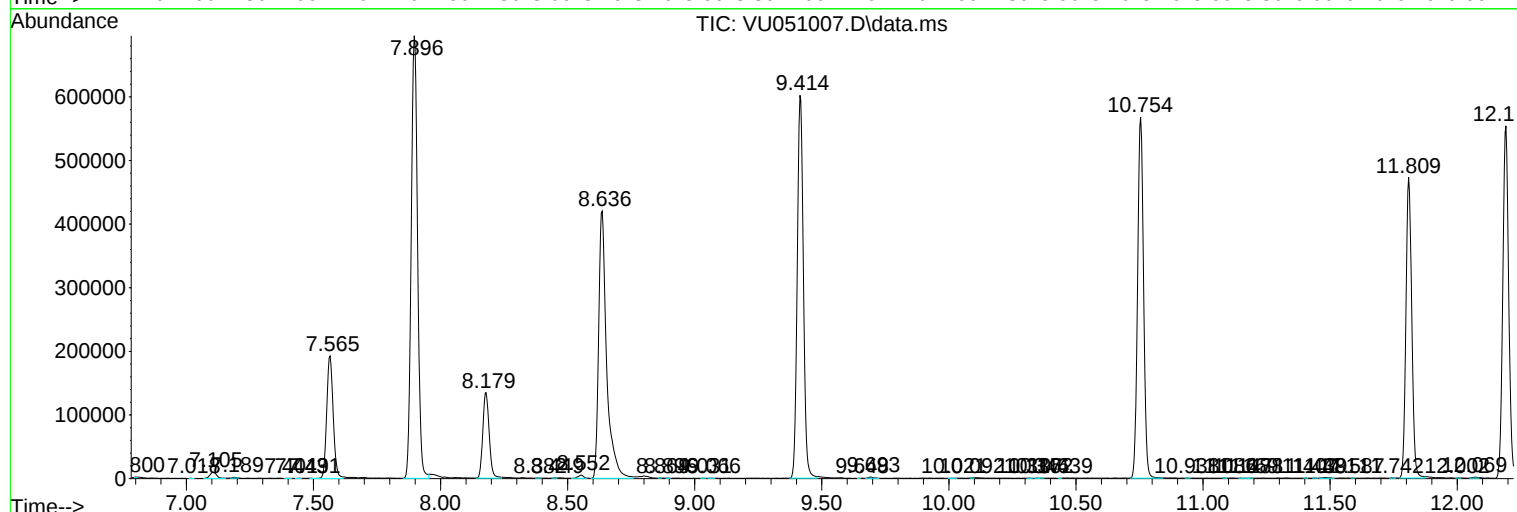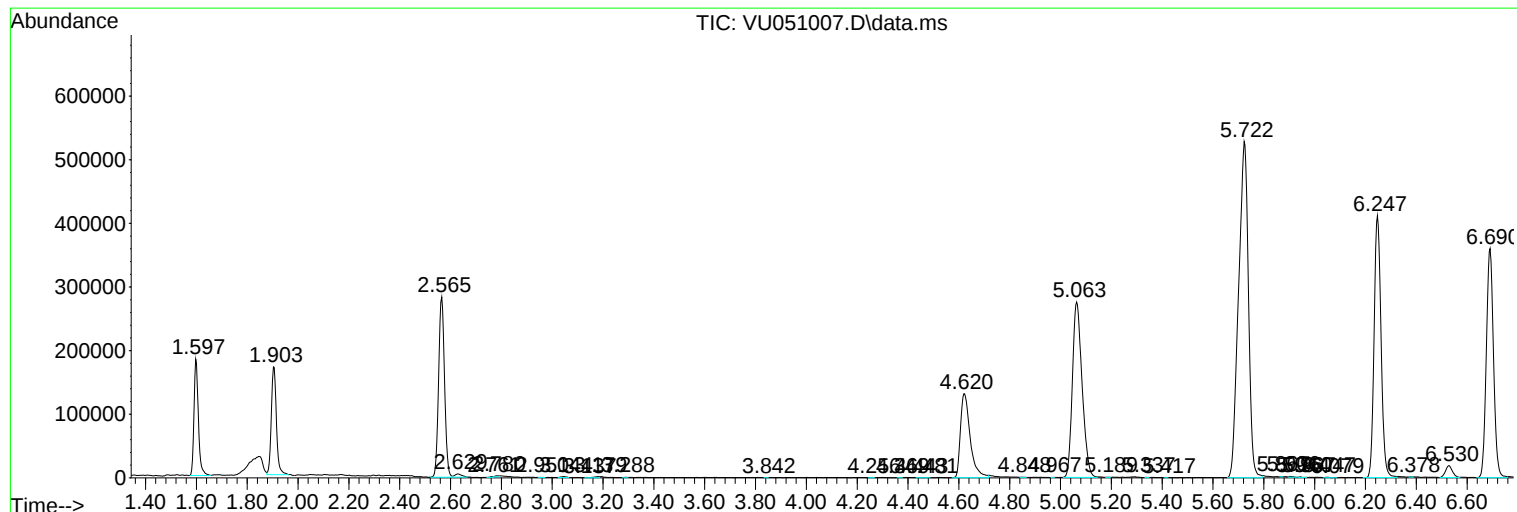

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
Data File : VU051007.D
Acq On : 30 Sep 2022 02:42
Operator : JC/MD
Sample : N4859-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E10022

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
Data File : VU051007.D
Acq On : 30 Sep 2022 02:42
Operator : JC/MD
Sample : N4859-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E10022

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc