

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
 Data File : VU051008.D
 Acq On : 30 Sep 2022 03:06
 Operator : JC/MD
 Sample : N4859-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E10021

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

Signal : TIC: VU051008.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.488	42	46	51	rBV2	4952	4319	0.31%	0.040%
2	1.597	72	80	98	rBV	176832	216605	15.57%	2.012%
3	1.903	168	175	192	rVB	170697	229365	16.49%	2.130%
4	2.488	354	357	360	rBV3	420	297	0.02%	0.003%
5	2.565	369	381	394	rBV	277844	441539	31.74%	4.101%
6	2.629	396	401	417	rVB	6631	11328	0.81%	0.105%
7	2.774	437	446	447	rBV3	1183	1240	0.09%	0.012%
8	2.887	477	481	483	rBV3	759	618	0.04%	0.006%
9	2.919	489	491	496	rVB2	587	434	0.03%	0.004%
10	2.951	496	501	504	rBV3	605	634	0.05%	0.006%
11	3.041	523	529	539	rVB5	1872	3043	0.22%	0.028%
12	3.179	565	572	574	rBV2	881	1058	0.08%	0.010%
13	3.607	701	705	707	rBV	320	278	0.02%	0.003%
14	3.642	710	716	720	rBV2	363	458	0.03%	0.004%
15	3.671	721	725	729	rBV	304	249	0.02%	0.002%
16	3.726	738	742	746	rVB2	423	390	0.03%	0.004%
17	3.758	746	752	758	rBV2	344	637	0.05%	0.006%
18	3.838	774	777	781	rBV2	336	314	0.02%	0.003%
19	4.089	852	855	861	rVB	347	343	0.02%	0.003%
20	4.369	938	942	945	rBV	275	228	0.02%	0.002%
21	4.514	981	987	990	rBV2	304	368	0.03%	0.003%
22	4.578	999	1007	1008	rBV3	387	438	0.03%	0.004%
23	4.623	1008	1021	1050	rBV2	133140	345350	24.83%	3.208%
24	5.063	1141	1158	1184	rBV2	276717	725989	52.19%	6.743%
25	5.192	1194	1198	1199	rBV2	584	384	0.03%	0.004%
26	5.369	1249	1253	1256	rBV3	446	300	0.02%	0.003%
27	5.404	1261	1264	1270	rVB3	344	320	0.02%	0.003%
28	5.481	1284	1288	1291	rBV2	397	346	0.02%	0.003%
29	5.723	1341	1363	1388	rBV2	514331	1390995	100.00%	12.920%
30	5.867	1405	1408	1410	rBV5	552	389	0.03%	0.004%
31	6.041	1460	1462	1465	rVB2	513	310	0.02%	0.003%
32	6.063	1465	1469	1472	rBV3	355	310	0.02%	0.003%
33	6.108	1479	1483	1486	rBV4	392	319	0.02%	0.003%
34	6.147	1491	1495	1499	rBV3	458	385	0.03%	0.004%
35	6.247	1511	1526	1549	rBV	381973	727942	52.33%	6.761%
36	6.530	1603	1614	1631	rVB4	14229	28501	2.05%	0.265%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
 Data File : VU051008.D
 Acq On : 30 Sep 2022 03:06
 Operator : JC/MD
 Sample : N4859-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E10021

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	6.690	1649	1664	1685	rBV	328228	642362	46.18%	5.966%
38	6.784	1690	1693	1694	rBV2	541	247	0.02%	0.002%
39	6.858	1714	1716	1718	rVB3	631	314	0.02%	0.003%
40	6.870	1718	1720	1722	rBV	410	237	0.02%	0.002%
41	6.970	1746	1751	1754	rBV2	348	287	0.02%	0.003%
42	7.105	1783	1793	1807	rVV4	8468	14711	1.06%	0.137%
43	7.182	1812	1817	1818	rBV3	833	648	0.05%	0.006%
44	7.317	1853	1859	1863	rVB2	359	376	0.03%	0.003%
45	7.366	1869	1874	1877	rVB3	251	248	0.02%	0.002%
46	7.469	1905	1906	1911	rVB2	355	239	0.02%	0.002%
47	7.565	1916	1936	1952	rBV	155588	275054	19.77%	2.555%
48	7.710	1979	1981	1985	rVB2	678	422	0.03%	0.004%
49	7.796	1999	2008	2023	rVB6	4026	7645	0.55%	0.071%
50	7.896	2025	2039	2056	rBV	614648	1046652	75.24%	9.722%
51	8.050	2085	2087	2091	rVB2	609	392	0.03%	0.004%
52	8.179	2114	2127	2144	rBV	115565	196846	14.15%	1.828%
53	8.295	2161	2163	2166	rVB2	677	363	0.03%	0.003%
54	8.388	2187	2192	2195	rVB2	471	485	0.03%	0.005%
55	8.407	2195	2198	2203	rBV3	308	316	0.02%	0.003%
56	8.481	2218	2221	2228	rVB3	470	355	0.03%	0.003%
57	8.555	2232	2244	2251	rBV5	3581	5915	0.43%	0.055%
58	8.636	2256	2269	2309	rBV3	416880	907229	65.22%	8.427%
59	8.941	2358	2364	2367	rVB4	580	620	0.04%	0.006%
60	9.202	2442	2445	2448	rVB	438	248	0.02%	0.002%
61	9.253	2458	2461	2467	rVB2	319	288	0.02%	0.003%
62	9.417	2499	2512	2532	rBV	669007	1112022	79.94%	10.329%
63	9.571	2552	2560	2578	rVB	10500	16652	1.20%	0.155%
64	9.690	2588	2597	2608	rVB2	20169	32655	2.35%	0.303%
65	10.099	2715	2724	2738	rBV3	11460	19520	1.40%	0.181%
66	10.224	2759	2763	2765	rBV2	274	233	0.02%	0.002%
67	10.365	2801	2807	2809	rBV2	392	303	0.02%	0.003%
68	10.755	2915	2928	2950	rBV	474442	767507	55.18%	7.129%
69	10.941	2982	2986	2990	rVB2	280	255	0.02%	0.002%
70	10.970	2990	2995	2999	rBV2	520	529	0.04%	0.005%
71	11.182	3057	3061	3067	rBV3	333	282	0.02%	0.003%
72	11.234	3073	3077	3079	rBV2	415	313	0.02%	0.003%
73	11.320	3101	3104	3109	rVB3	697	556	0.04%	0.005%
74	11.423	3134	3136	3144	rVB2	280	296	0.02%	0.003%
75	11.478	3144	3153	3165	rBV6	1200	2668	0.19%	0.025%
76	11.697	3217	3221	3225	rBV2	532	449	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
 Data File : VU051008.D
 Acq On : 30 Sep 2022 03:06
 Operator : JC/MD
 Sample : N4859-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E10021

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	11.748	3235	3237	3243	rVB3	430	381	0.03%	0.004%
78	11.809	3244	3256	3278	rBV	427729	666218	47.90%	6.188%
79	12.073	3332	3338	3341	rBV5	1355	1282	0.09%	0.012%
80	12.192	3362	3375	3397	rBV	553839	896254	64.43%	8.325%
81	12.340	3417	3421	3424	rVB3	669	387	0.03%	0.004%
82	12.362	3424	3428	3431	rBV4	677	497	0.04%	0.005%
83	12.407	3438	3442	3445	rBV3	427	454	0.03%	0.004%
84	12.687	3523	3529	3533	rBV3	491	432	0.03%	0.004%
85	12.796	3554	3563	3566	rBV	604	644	0.05%	0.006%
86	13.111	3659	3661	3665	rBV2	398	289	0.02%	0.003%
87	13.189	3682	3685	3688	rVB2	461	273	0.02%	0.003%
88	13.221	3692	3695	3700	rVB	347	255	0.02%	0.002%
89	13.417	3753	3756	3763	rVB2	363	413	0.03%	0.004%
90	13.674	3833	3836	3841	rVB	336	248	0.02%	0.002%
91	13.793	3867	3873	3875	rBV3	297	347	0.02%	0.003%
92	13.864	3892	3895	3898	rVB3	399	249	0.02%	0.002%
93	14.015	3937	3942	3946	rBV3	433	533	0.04%	0.005%
94	14.179	3990	3993	3995	rBV2	365	277	0.02%	0.003%
95	14.941	4224	4230	4233	rBV3	645	771	0.06%	0.007%
96	15.160	4296	4298	4300	rBV	452	261	0.02%	0.002%
97	15.606	4434	4437	4438	rBV	691	388	0.03%	0.004%
98	15.780	4489	4491	4494	rBV3	530	393	0.03%	0.004%
99	16.182	4613	4616	4622	rBV5	904	783	0.06%	0.007%
100	16.362	4668	4672	4678	rBV4	1293	1547	0.11%	0.014%




Sum of corrected areas: 10766338

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
Data File : VU051008.D
Acq On : 30 Sep 2022 03:06
Operator : JC/MD
Sample : N4859-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E10021

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

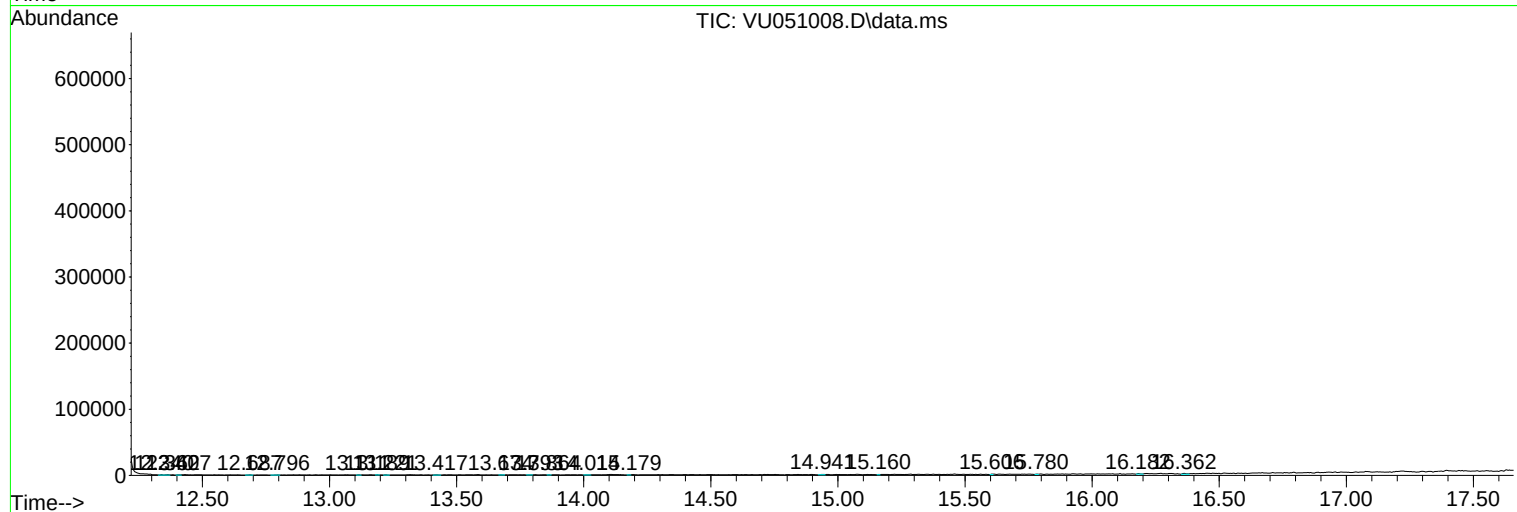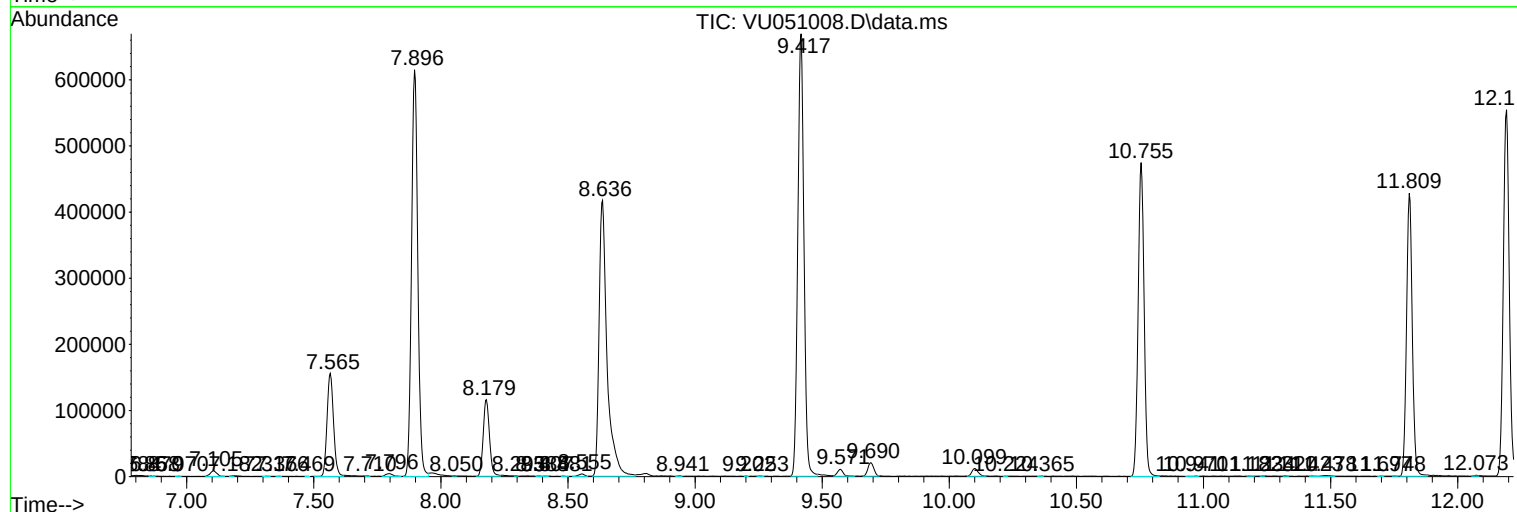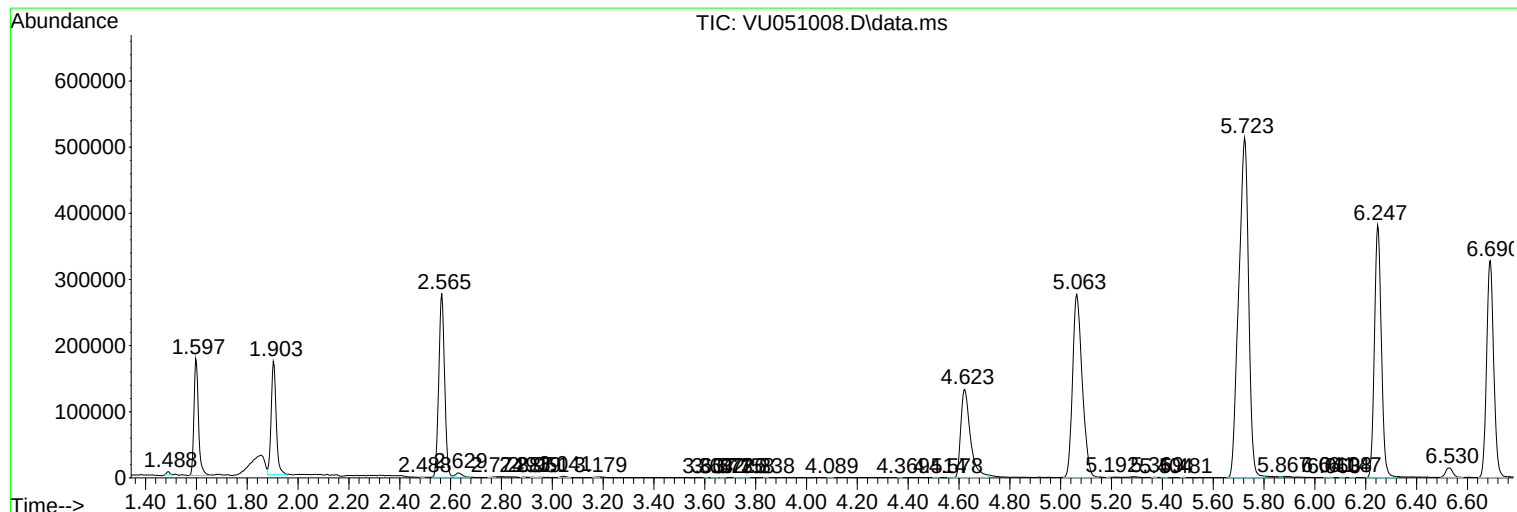

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
Data File : VU051008.D
Acq On : 30 Sep 2022 03:06
Operator : JC/MD
Sample : N4859-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E10021

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
Data File : VU051008.D
Acq On : 30 Sep 2022 03:06
Operator : JC/MD
Sample : N4859-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E10021

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc