

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
 Data File : VU051009.D
 Acq On : 30 Sep 2022 03:29
 Operator : JC/MD
 Sample : N4880-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGS3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M

Title : VOC Analysis

Signal : TIC: VU051009.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.359	3	6	15	rVB3	5742	5526	0.41%	0.051%
2	1.597	71	80	96	rVB	175610	216932	16.15%	2.006%
3	1.684	102	107	114	rVB	13326	14025	1.04%	0.130%
4	1.906	168	176	196	rVB	161283	215290	16.03%	1.991%
5	2.565	369	381	394	rBV	269969	434767	32.38%	4.020%
6	2.729	431	432	437	rBV3	333	238	0.02%	0.002%
7	2.784	445	449	451	rBV2	482	430	0.03%	0.004%
8	2.854	465	471	475	rBV5	718	891	0.07%	0.008%
9	2.874	475	477	479	rVB2	664	208	0.02%	0.002%
10	3.050	525	532	540	rVB5	1383	2270	0.17%	0.021%
11	3.169	565	569	570	rBV	886	648	0.05%	0.006%
12	3.324	615	617	620	rVV	370	207	0.02%	0.002%
13	3.369	625	631	634	rBV2	357	332	0.02%	0.003%
14	3.976	814	820	821	rBV2	232	215	0.02%	0.002%
15	4.128	864	867	871	rBV2	251	239	0.02%	0.002%
16	4.182	879	884	890	rVB2	369	571	0.04%	0.005%
17	4.218	890	895	898	rBV	353	425	0.03%	0.004%
18	4.234	898	900	908	rVB2	385	474	0.04%	0.004%
19	4.394	944	950	953	rBV2	337	444	0.03%	0.004%
20	4.459	966	970	975	rBV3	657	685	0.05%	0.006%
21	4.484	975	978	985	rVV	409	330	0.02%	0.003%
22	4.619	1005	1020	1062	rBV	130454	334433	24.90%	3.092%
23	4.832	1084	1086	1088	rBV	634	213	0.02%	0.002%
24	5.060	1140	1157	1180	rBV	246766	548857	40.87%	5.075%
25	5.185	1192	1196	1199	rBV2	317	264	0.02%	0.002%
26	5.266	1214	1221	1222	rBV4	646	656	0.05%	0.006%
27	5.382	1252	1257	1261	rVV4	597	579	0.04%	0.005%
28	5.446	1270	1277	1280	rBV2	399	486	0.04%	0.004%
29	5.722	1339	1363	1383	rBV2	503192	1342873	100.00%	12.417%
30	5.960	1429	1437	1439	rBV3	698	639	0.05%	0.006%
31	6.060	1465	1468	1470	rBV3	288	193	0.01%	0.002%
32	6.160	1493	1499	1501	rBV	433	278	0.02%	0.003%
33	6.246	1511	1526	1551	rBV	392076	747237	55.64%	6.909%
34	6.436	1579	1585	1588	rBV3	417	478	0.04%	0.004%
35	6.491	1598	1602	1603	rBV2	440	293	0.02%	0.003%
36	6.529	1603	1614	1628	rVB3	10865	21537	1.60%	0.199%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
 Data File : VU051009.D
 Acq On : 30 Sep 2022 03:29
 Operator : JC/MD
 Sample : N4880-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGS3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	6.687	1649	1663	1683	rBV	365122	719376	53.57%	6.652%
38	7.015	1762	1765	1768	rBV2	357	295	0.02%	0.003%
39	7.182	1809	1817	1818	rBV4	1103	1051	0.08%	0.010%
40	7.565	1923	1936	1954	rBV	184180	325225	24.22%	3.007%
41	7.896	2022	2039	2057	rBV	650604	1118253	83.27%	10.340%
42	8.179	2115	2127	2144	rBV	129449	222280	16.55%	2.055%
43	8.471	2213	2218	2224	rVB3	719	752	0.06%	0.007%
44	8.552	2233	2243	2256	rVB2	22581	38338	2.85%	0.354%
45	8.632	2256	2268	2309	rBV2	450707	971052	72.31%	8.979%
46	8.790	2310	2317	2326	rVB8	4546	8417	0.63%	0.078%
47	8.976	2371	2375	2378	rVB3	473	330	0.02%	0.003%
48	8.996	2378	2381	2385	rVB2	486	345	0.03%	0.003%
49	9.018	2385	2388	2390	rBV2	334	227	0.02%	0.002%
50	9.114	2416	2418	2420	rBV	403	231	0.02%	0.002%
51	9.417	2498	2512	2535	rBV	647885	1078166	80.29%	9.969%
52	9.571	2554	2560	2565	rVB4	1010	1236	0.09%	0.011%
53	9.687	2593	2596	2598	rBV2	682	442	0.03%	0.004%
54	9.741	2611	2613	2617	rVB2	415	250	0.02%	0.002%
55	9.822	2634	2638	2640	rBV2	325	251	0.02%	0.002%
56	9.867	2649	2652	2658	rVV2	621	570	0.04%	0.005%
57	9.931	2669	2672	2676	rBV2	426	290	0.02%	0.003%
58	10.105	2721	2726	2727	rBV2	436	340	0.03%	0.003%
59	10.137	2732	2736	2740	rBV2	305	297	0.02%	0.003%
60	10.282	2777	2781	2782	rBV	360	230	0.02%	0.002%
61	10.346	2798	2801	2803	rBV	728	416	0.03%	0.004%
62	10.536	2854	2860	2862	rBV2	427	457	0.03%	0.004%
63	10.594	2875	2878	2880	rBV2	360	199	0.01%	0.002%
64	10.629	2883	2889	2894	rBV2	439	680	0.05%	0.006%
65	10.674	2897	2903	2907	rBV	414	459	0.03%	0.004%
66	10.754	2915	2928	2949	rBV	500903	800720	59.63%	7.404%
67	10.889	2965	2970	2972	rBV3	794	655	0.05%	0.006%
68	10.995	2999	3003	3007	rBV3	270	256	0.02%	0.002%
69	11.044	3015	3018	3022	rVB3	349	245	0.02%	0.002%
70	11.092	3031	3033	3037	rBV2	342	230	0.02%	0.002%
71	11.378	3118	3122	3128	rVB3	453	502	0.04%	0.005%
72	11.471	3149	3151	3157	rVB2	685	498	0.04%	0.005%
73	11.690	3211	3219	3228	rBV6	5684	8054	0.60%	0.074%
74	11.809	3244	3256	3280	rBV	466070	750204	55.87%	6.937%
75	12.063	3324	3335	3348	rBV5	8660	16094	1.20%	0.149%
76	12.130	3353	3356	3358	rVB2	496	248	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
 Data File : VU051009.D
 Acq On : 30 Sep 2022 03:29
 Operator : JC/MD
 Sample : N4880-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGS3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	12.192	3361	3375	3391	rBV	506845	829543	61.77%	7.670%
78	12.301	3407	3409	3415	rVB3	675	475	0.04%	0.004%
79	12.330	3415	3418	3423	rBV3	611	508	0.04%	0.005%
80	12.503	3469	3472	3477	rBV2	472	489	0.04%	0.005%
81	12.574	3492	3494	3498	rBV2	292	241	0.02%	0.002%
82	12.757	3548	3551	3557	rVB2	632	556	0.04%	0.005%
83	12.793	3558	3562	3566	rBV2	390	354	0.03%	0.003%
84	12.886	3584	3591	3604	rBV6	8027	13610	1.01%	0.126%
85	13.220	3692	3695	3700	rVB2	736	560	0.04%	0.005%
86	13.381	3743	3745	3751	rVV2	342	271	0.02%	0.003%
87	13.407	3751	3753	3757	rVB2	332	219	0.02%	0.002%
88	13.593	3808	3811	3813	rBV2	495	307	0.02%	0.003%
89	13.777	3862	3868	3870	rBV2	481	581	0.04%	0.005%
90	13.966	3924	3927	3930	rBV2	338	284	0.02%	0.003%
91	14.044	3947	3951	3953	rBV2	399	371	0.03%	0.003%
92	14.336	4039	4042	4044	rBV2	494	286	0.02%	0.003%
93	14.510	4093	4096	4099	rBV2	558	411	0.03%	0.004%
94	14.661	4141	4143	4145	rBV	400	229	0.02%	0.002%
95	15.320	4346	4348	4351	rBV2	459	284	0.02%	0.003%
96	15.343	4352	4355	4358	rVV2	599	413	0.03%	0.004%
97	15.362	4359	4361	4369	rVB3	799	877	0.07%	0.008%
98	15.690	4461	4463	4467	rVB3	1085	668	0.05%	0.006%
99	15.712	4467	4470	4474	rBB5	566	416	0.03%	0.004%
100	15.735	4474	4477	4478	rBV	811	451	0.03%	0.004%


Sum of corrected areas: 10814728

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
Data File : VU051009.D
Acq On : 30 Sep 2022 03:29
Operator : JC/MD
Sample : N4880-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGS3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

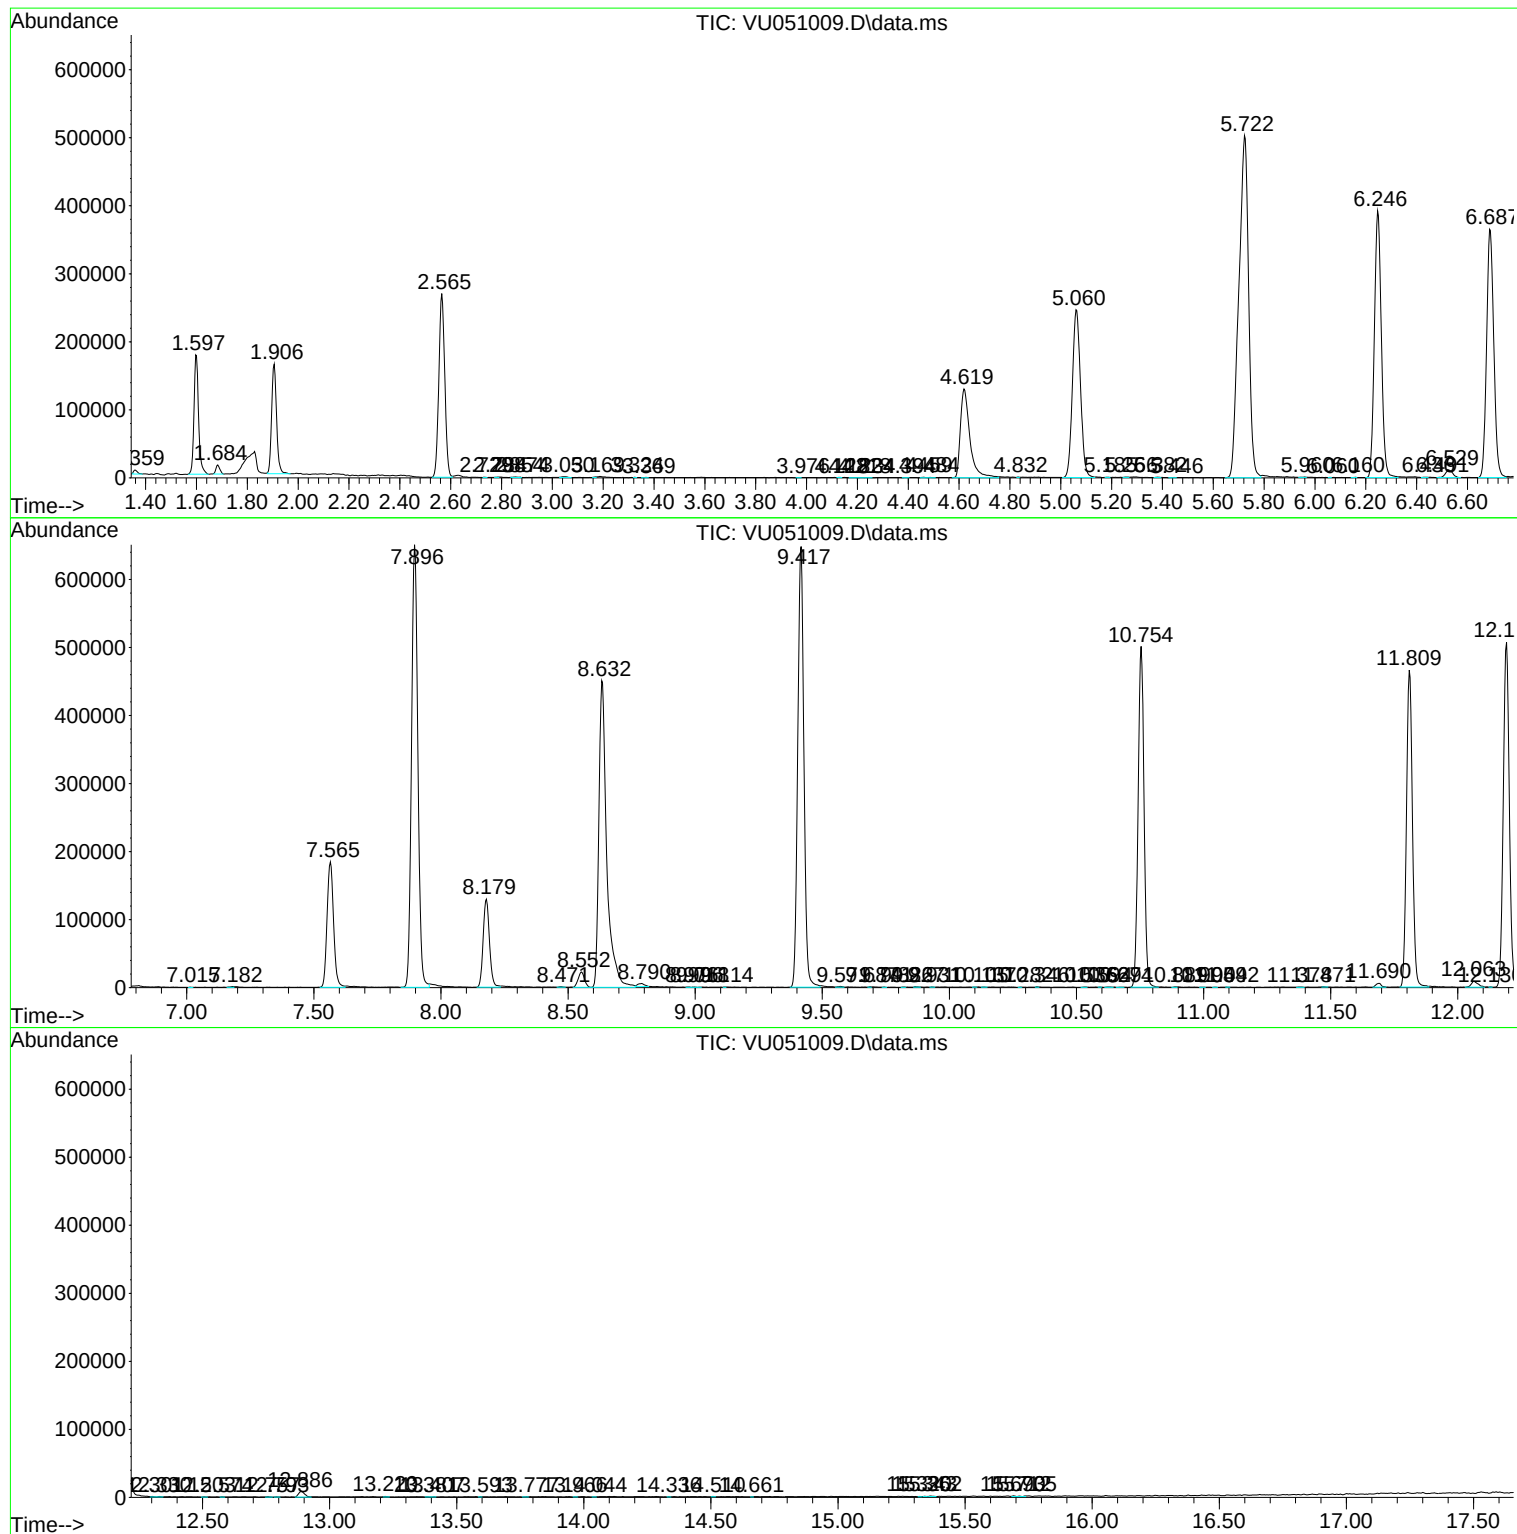

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
Data File : VU051009.D
Acq On : 30 Sep 2022 03:29
Operator : JC/MD
Sample : N4880-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGS3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
Data File : VU051009.D
Acq On : 30 Sep 2022 03:29
Operator : JC/MD
Sample : N4880-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGS3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------