

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
 Data File : VU051010.D
 Acq On : 30 Sep 2022 03:53
 Operator : JC/MD
 Sample : N4880-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGS4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

Signal : TIC: VU051010.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.359	3	6	15	rVB	11231	10104	0.73%	0.092%
2	1.597	72	80	97	rVB	176003	219700	15.86%	2.005%
3	1.684	103	107	115	rVB2	7155	7994	0.58%	0.073%
4	1.906	168	176	189	rVB	165059	219839	15.87%	2.007%
5	2.565	368	381	394	rBV	268544	437183	31.56%	3.991%
6	2.703	420	424	426	rBV2	472	286	0.02%	0.003%
7	2.793	443	452	458	rVV4	1122	1851	0.13%	0.017%
8	2.845	463	468	469	rBV3	1153	816	0.06%	0.007%
9	3.044	525	530	534	rBV4	1166	1218	0.09%	0.011%
10	3.131	552	557	559	rBV2	400	352	0.03%	0.003%
11	3.182	562	573	574	rBV3	1919	2173	0.16%	0.020%
12	3.317	609	615	617	rBV4	394	328	0.02%	0.003%
13	3.353	623	626	629	rVB2	445	224	0.02%	0.002%
14	3.452	653	657	662	rVB	318	306	0.02%	0.003%
15	3.568	687	693	695	rBV3	320	324	0.02%	0.003%
16	3.604	699	704	706	rBV2	270	282	0.02%	0.003%
17	3.877	787	789	793	rVB	404	266	0.02%	0.002%
18	4.105	856	860	869	rVB2	302	443	0.03%	0.004%
19	4.475	969	975	980	rVB3	606	583	0.04%	0.005%
20	4.501	980	983	987	rVB2	421	273	0.02%	0.002%
21	4.533	987	993	997	rBV	258	261	0.02%	0.002%
22	4.623	1008	1021	1057	rBV	128943	341816	24.68%	3.120%
23	5.060	1140	1157	1183	rBV	255655	565387	40.82%	5.161%
24	5.173	1188	1192	1194	rBV2	419	320	0.02%	0.003%
25	5.279	1221	1225	1228	rBV4	546	512	0.04%	0.005%
26	5.337	1239	1243	1246	rVB3	432	391	0.03%	0.004%
27	5.372	1250	1254	1260	rVB3	702	627	0.05%	0.006%
28	5.407	1260	1265	1267	rBV2	276	254	0.02%	0.002%
29	5.722	1341	1363	1389	rBV2	512170	1385035	100.00%	12.643%
30	5.973	1437	1441	1444	rBV4	773	747	0.05%	0.007%
31	6.044	1459	1463	1470	rVB4	371	363	0.03%	0.003%
32	6.195	1505	1510	1512	rBV2	221	226	0.02%	0.002%
33	6.247	1512	1526	1554	rVV	384622	723488	52.24%	6.604%
34	6.398	1569	1573	1580	rVB4	820	920	0.07%	0.008%
35	6.465	1591	1594	1595	rBV2	538	314	0.02%	0.003%
36	6.530	1603	1614	1628	rVB3	10828	21956	1.59%	0.200%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
 Data File : VU051010.D
 Acq On : 30 Sep 2022 03:53
 Operator : JC/MD
 Sample : N4880-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGS4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	6.594	1628	1634	1636	rBV2	604	587	0.04%	0.005%
38	6.690	1649	1664	1687	rBV	343438	664629	47.99%	6.067%
39	6.883	1722	1724	1726	rVB2	730	319	0.02%	0.003%
40	6.964	1745	1749	1754	rVV3	502	532	0.04%	0.005%
41	7.073	1774	1783	1787	rBV	356	477	0.03%	0.004%
42	7.195	1812	1821	1825	rBV4	1145	1789	0.13%	0.016%
43	7.288	1846	1850	1854	rBV3	369	275	0.02%	0.003%
44	7.565	1923	1936	1955	rBV	193909	341786	24.68%	3.120%
45	7.697	1976	1977	1985	rVB5	796	565	0.04%	0.005%
46	7.796	2003	2008	2011	rBV3	1026	1053	0.08%	0.010%
47	7.812	2011	2013	2017	rVB	526	280	0.02%	0.003%
48	7.896	2025	2039	2056	rBV	677201	1160729	83.81%	10.595%
49	8.124	2108	2110	2113	rVB3	476	225	0.02%	0.002%
50	8.179	2115	2127	2150	rBV	135719	232186	16.76%	2.119%
51	8.452	2207	2212	2213	rBV2	330	283	0.02%	0.003%
52	8.504	2225	2228	2232	rVB2	362	267	0.02%	0.002%
53	8.552	2232	2243	2255	rBV2	49163	84683	6.11%	0.773%
54	8.636	2255	2269	2302	rBV2	453539	978412	70.64%	8.931%
55	8.861	2335	2339	2343	rVB3	512	378	0.03%	0.003%
56	8.938	2361	2363	2369	rVB3	287	279	0.02%	0.003%
57	8.970	2369	2373	2375	rVB	362	253	0.02%	0.002%
58	8.986	2375	2378	2380	rBV2	450	305	0.02%	0.003%
59	9.086	2405	2409	2414	rVB2	372	334	0.02%	0.003%
60	9.189	2438	2441	2447	rVB2	299	288	0.02%	0.003%
61	9.230	2451	2454	2456	rBV	416	230	0.02%	0.002%
62	9.417	2496	2512	2534	rBV	582357	958090	69.17%	8.746%
63	9.594	2565	2567	2573	rVB4	627	361	0.03%	0.003%
64	9.645	2581	2583	2587	rBV2	382	288	0.02%	0.003%
65	9.690	2593	2597	2600	rBV4	591	529	0.04%	0.005%
66	9.780	2622	2625	2628	rBV2	431	279	0.02%	0.003%
67	9.896	2657	2661	2665	rBV3	342	323	0.02%	0.003%
68	10.102	2721	2725	2729	rBV3	566	512	0.04%	0.005%
69	10.240	2764	2768	2774	rBV3	329	428	0.03%	0.004%
70	10.484	2841	2844	2849	rBV	253	323	0.02%	0.003%
71	10.754	2915	2928	2946	rVV	559925	904872	65.33%	8.260%
72	10.889	2964	2970	2977	rVB2	818	1118	0.08%	0.010%
73	10.918	2977	2979	2981	rBV2	416	235	0.02%	0.002%
74	11.092	3029	3033	3037	rBV2	371	276	0.02%	0.003%
75	11.118	3037	3041	3045	rVB	388	320	0.02%	0.003%
76	11.330	3103	3107	3111	rVV2	495	371	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
 Data File : VU051010.D
 Acq On : 30 Sep 2022 03:53
 Operator : JC/MD
 Sample : N4880-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGS4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	11.465	3144	3149	3152	rBV2	334	378	0.03%	0.003%
78	11.529	3165	3169	3171	rVB2	360	267	0.02%	0.002%
79	11.549	3171	3175	3179	rVB	459	344	0.02%	0.003%
80	11.574	3179	3183	3187	rBV	366	369	0.03%	0.003%
81	11.687	3210	3218	3229	rVB5	3518	4788	0.35%	0.044%
82	11.809	3244	3256	3280	rBV	478076	731047	52.78%	6.673%
83	11.899	3282	3284	3287	rVB3	867	417	0.03%	0.004%
84	12.066	3327	3336	3351	rVV5	5642	11722	0.85%	0.107%
85	12.192	3362	3375	3399	rBV	546077	902588	65.17%	8.239%
86	12.378	3430	3433	3435	rBV2	631	446	0.03%	0.004%
87	12.603	3500	3503	3506	rBV	342	231	0.02%	0.002%
88	12.886	3584	3591	3601	rVB6	6716	10627	0.77%	0.097%
89	12.934	3601	3606	3609	rBV	394	309	0.02%	0.003%
90	13.150	3670	3673	3675	rBV	363	272	0.02%	0.002%
91	13.227	3694	3697	3700	rBV	569	381	0.03%	0.003%
92	13.291	3713	3717	3720	rBV2	331	265	0.02%	0.002%
93	13.648	3825	3828	3834	rVB3	477	379	0.03%	0.003%
94	13.729	3851	3853	3857	rBV	370	257	0.02%	0.002%
95	13.854	3888	3892	3896	rVB2	695	490	0.04%	0.004%
96	13.925	3910	3914	3917	rBV2	534	400	0.03%	0.004%
97	14.034	3946	3948	3954	rVB2	395	281	0.02%	0.003%
98	15.555	4417	4421	4423	rBV	758	587	0.04%	0.005%
99	15.700	4463	4466	4470	rBV3	715	560	0.04%	0.005%
100	15.767	4484	4487	4492	rVV4	919	915	0.07%	0.008%




Sum of corrected areas: 10954951

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
Data File : VU051010.D
Acq On : 30 Sep 2022 03:53
Operator : JC/MD
Sample : N4880-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGS4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

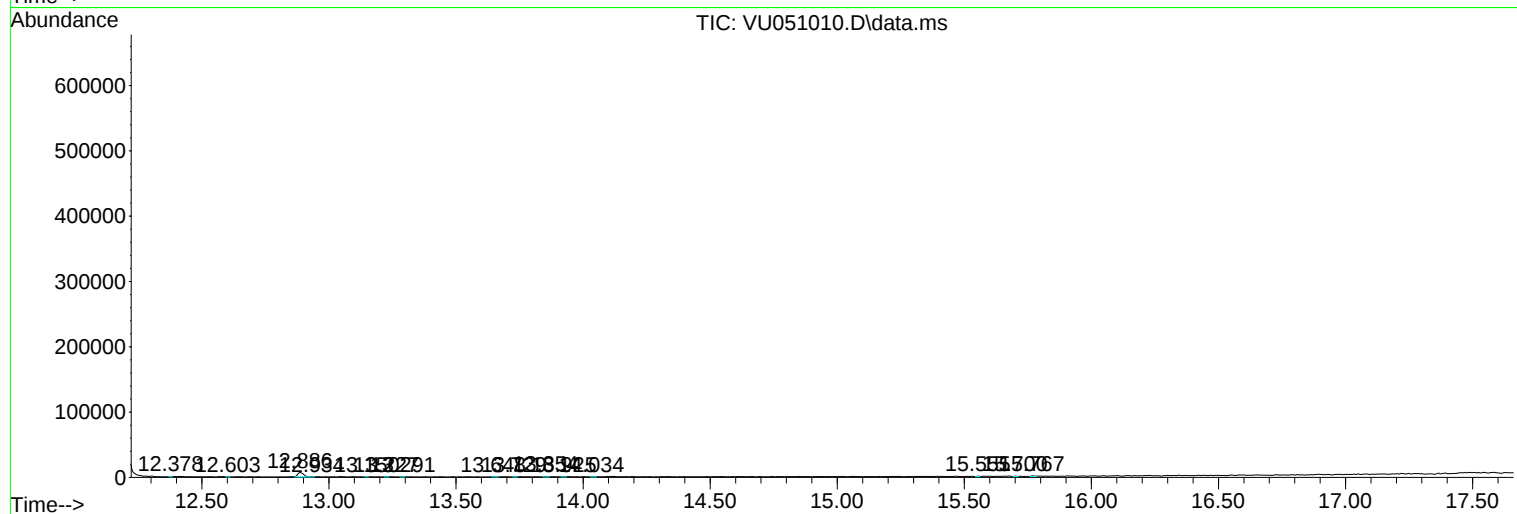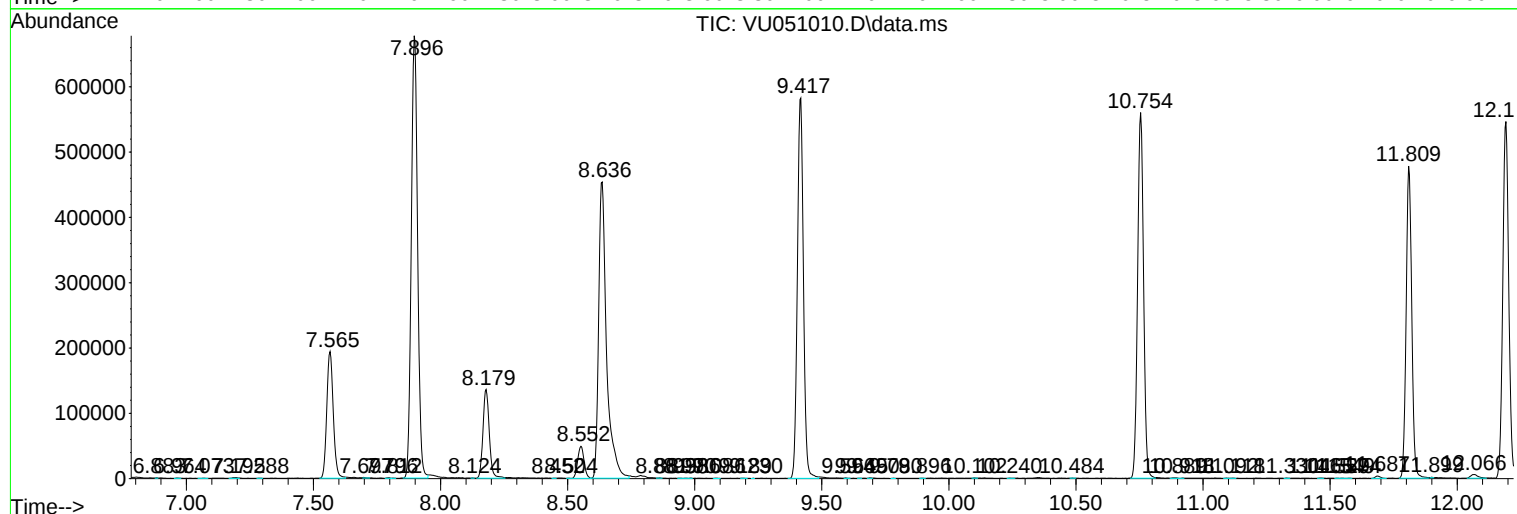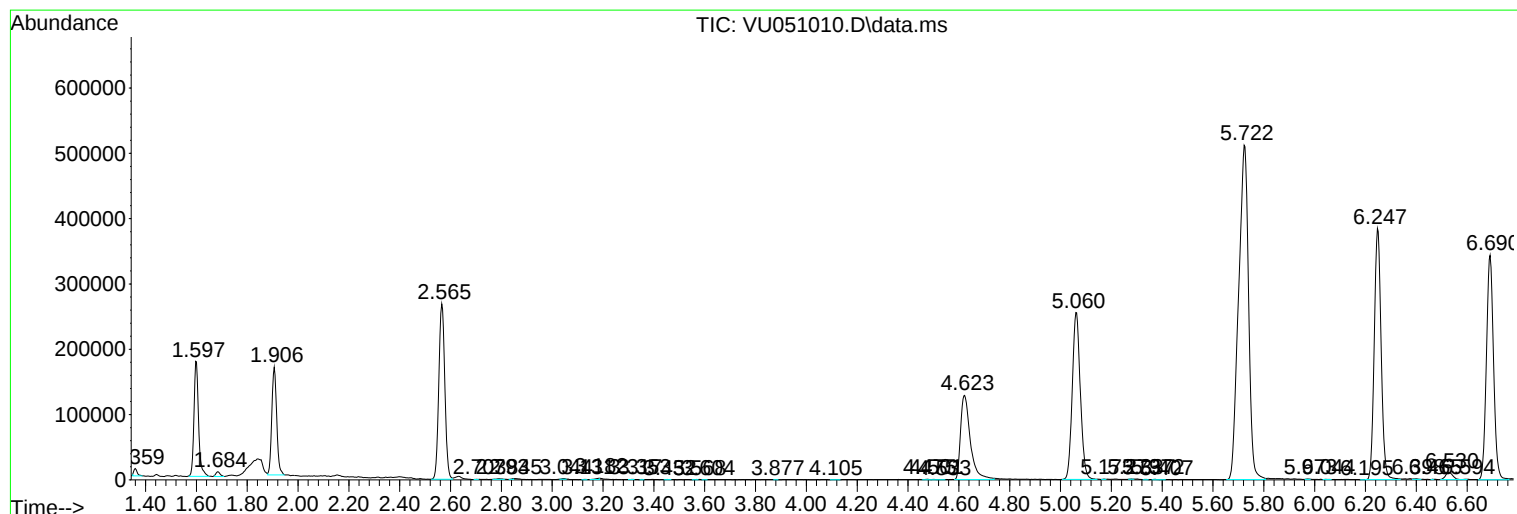

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
Data File : VU051010.D
Acq On : 30 Sep 2022 03:53
Operator : JC/MD
Sample : N4880-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGS4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
Data File : VU051010.D
Acq On : 30 Sep 2022 03:53
Operator : JC/MD
Sample : N4880-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGS4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc