

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
 Data File : VU051011.D
 Acq On : 30 Sep 2022 04:16
 Operator : JC/MD
 Sample : N4880-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGS5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

Signal : TIC: VU051011.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.359	3	6	16	rVB	11677	11633	0.84%	0.094%
2	1.597	72	80	98	rVB	182623	221571	15.96%	1.788%
3	1.906	169	176	199	rVB	214647	289101	20.83%	2.334%
4	2.565	367	381	396	rBV	272109	437462	31.52%	3.531%
5	2.700	420	423	428	rBV2	309	237	0.02%	0.002%
6	2.790	448	451	453	rVV2	465	230	0.02%	0.002%
7	3.041	522	529	536	rBV5	1424	2369	0.17%	0.019%
8	3.186	566	574	575	rBV2	1020	1228	0.09%	0.010%
9	3.369	622	631	638	rVB5	1318	2647	0.19%	0.021%
10	3.639	709	715	717	rBV	245	229	0.02%	0.002%
11	3.707	733	736	738	rVV2	492	274	0.02%	0.002%
12	3.787	757	761	765	rVB	384	375	0.03%	0.003%
13	3.822	765	772	775	rBV2	334	481	0.03%	0.004%
14	3.838	775	777	784	rVB2	304	258	0.02%	0.002%
15	4.173	877	881	885	rBV2	314	373	0.03%	0.003%
16	4.231	893	899	902	rVB	324	257	0.02%	0.002%
17	4.292	915	918	922	rVB	357	224	0.02%	0.002%
18	4.408	951	954	958	rBV2	307	248	0.02%	0.002%
19	4.623	1009	1021	1055	rBV	129192	344751	24.84%	2.783%
20	5.060	1140	1157	1181	rVV	256881	561904	40.48%	4.535%
21	5.195	1197	1199	1203	rVB3	605	331	0.02%	0.003%
22	5.218	1203	1206	1209	rBV2	459	305	0.02%	0.002%
23	5.276	1221	1224	1225	rBV2	632	323	0.02%	0.003%
24	5.350	1244	1247	1249	rBV2	455	314	0.02%	0.003%
25	5.433	1267	1273	1278	rVB	214	239	0.02%	0.002%
26	5.723	1340	1363	1392	rBV2	510689	1388040	100.00%	11.204%
27	5.851	1402	1403	1406	rBV3	554	243	0.02%	0.002%
28	5.961	1436	1437	1441	rVB3	397	230	0.02%	0.002%
29	5.980	1441	1443	1445	rBV2	608	291	0.02%	0.002%
30	6.038	1458	1461	1464	rVV3	522	415	0.03%	0.003%
31	6.163	1494	1500	1506	rVB2	283	372	0.03%	0.003%
32	6.247	1512	1526	1546	rBV	369926	708181	51.02%	5.716%
33	6.372	1560	1565	1572	rVB5	869	907	0.07%	0.007%
34	6.488	1597	1601	1604	rBV2	348	259	0.02%	0.002%
35	6.539	1604	1617	1632	rVB6	32574	70831	5.10%	0.572%
36	6.690	1650	1664	1685	rBV	338541	659396	47.51%	5.322%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
 Data File : VU051011.D
 Acq On : 30 Sep 2022 04:16
 Operator : JC/MD
 Sample : N4880-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGS5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	6.961	1744	1748	1752	rBV	403	361	0.03%	0.003%
38	7.006	1756	1762	1764	rBV	242	241	0.02%	0.002%
39	7.079	1779	1785	1787	rBV2	376	321	0.02%	0.003%
40	7.186	1812	1818	1819	rBV3	1029	939	0.07%	0.008%
41	7.250	1834	1838	1845	rVB2	324	260	0.02%	0.002%
42	7.565	1923	1936	1953	rBV	185681	331640	23.89%	2.677%
43	7.671	1967	1969	1973	rBV2	384	245	0.02%	0.002%
44	7.697	1975	1977	1982	rVB4	756	605	0.04%	0.005%
45	7.777	1999	2002	2004	rBV2	524	415	0.03%	0.003%
46	7.896	2025	2039	2060	rBV	687986	1183895	85.29%	9.556%
47	8.179	2115	2127	2145	rBV	135841	233161	16.80%	1.882%
48	8.462	2209	2215	2221	rBV5	697	930	0.07%	0.008%
49	8.552	2229	2243	2257	rBV	717617	1213161	87.40%	9.792%
50	8.636	2258	2269	2303	rVB3	447729	968244	69.76%	7.815%
51	8.845	2331	2334	2336	rBV2	409	327	0.02%	0.003%
52	9.417	2497	2512	2532	rBV	688015	1140723	82.18%	9.207%
53	9.610	2566	2572	2575	rBV4	533	679	0.05%	0.005%
54	9.684	2590	2595	2596	rBV2	594	421	0.03%	0.003%
55	9.694	2596	2598	2601	rVV2	478	301	0.02%	0.002%
56	9.796	2627	2630	2635	rVV2	419	386	0.03%	0.003%
57	9.883	2655	2657	2663	rBV3	344	276	0.02%	0.002%
58	9.922	2666	2669	2680	rVB3	490	732	0.05%	0.006%
59	10.202	2753	2756	2762	rVB3	259	236	0.02%	0.002%
60	10.256	2769	2773	2776	rBV3	252	242	0.02%	0.002%
61	10.272	2776	2778	2783	rVB	360	248	0.02%	0.002%
62	10.439	2823	2830	2831	rBV2	312	304	0.02%	0.002%
63	10.594	2874	2878	2884	rVB3	483	506	0.04%	0.004%
64	10.642	2889	2893	2895	rBV	263	249	0.02%	0.002%
65	10.755	2915	2928	2949	rBV	544800	891654	64.24%	7.197%
66	11.005	3001	3006	3007	rBV	355	238	0.02%	0.002%
67	11.057	3018	3022	3026	rBV2	353	382	0.03%	0.003%
68	11.176	3052	3059	3060	rBV2	292	313	0.02%	0.003%
69	11.221	3069	3073	3080	rVB2	223	237	0.02%	0.002%
70	11.687	3212	3218	3219	rBV4	883	677	0.05%	0.005%
71	11.809	3244	3256	3277	rBV	471433	758113	54.62%	6.119%
72	12.063	3326	3335	3351	rVV2	13019	23483	1.69%	0.190%
73	12.192	3362	3375	3404	rBV	557660	910873	65.62%	7.352%
74	12.703	3530	3534	3538	rBV3	342	362	0.03%	0.003%
75	12.838	3573	3576	3579	rBV2	330	266	0.02%	0.002%
76	12.890	3584	3592	3602	rVV4	4922	7103	0.51%	0.057%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
 Data File : VU051011.D
 Acq On : 30 Sep 2022 04:16
 Operator : JC/MD
 Sample : N4880-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGS5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	13.015	3628	3631	3633	rBV2	367	300	0.02%	0.002%
78	13.028	3633	3635	3639	rVB3	542	319	0.02%	0.003%
79	13.153	3671	3674	3676	rBV2	367	250	0.02%	0.002%
80	13.189	3683	3685	3692	rBV3	241	248	0.02%	0.002%
81	13.224	3692	3696	3698	rBV3	407	282	0.02%	0.002%
82	13.253	3703	3705	3708	rVV2	334	267	0.02%	0.002%
83	13.285	3712	3715	3719	rBV2	498	309	0.02%	0.002%
84	13.327	3724	3728	3732	rVB2	533	438	0.03%	0.004%
85	13.404	3749	3752	3756	rBV	372	343	0.02%	0.003%
86	13.600	3810	3813	3817	rVB3	357	303	0.02%	0.002%
87	13.729	3850	3853	3855	rBV2	455	289	0.02%	0.002%
88	13.793	3867	3873	3881	rVB3	662	1014	0.07%	0.008%
89	14.189	3992	3996	3999	rBV2	346	316	0.02%	0.003%
90	14.359	4046	4049	4051	rBV2	336	239	0.02%	0.002%
91	14.375	4052	4054	4057	rVV2	462	304	0.02%	0.002%
92	14.468	4080	4083	4086	rBV2	479	377	0.03%	0.003%
93	14.536	4100	4104	4106	rBV	284	231	0.02%	0.002%
94	14.607	4123	4126	4129	rBV2	367	305	0.02%	0.002%
95	15.073	4267	4271	4275	rBV3	505	537	0.04%	0.004%
96	15.246	4319	4325	4326	rBV2	488	483	0.03%	0.004%
97	15.616	4437	4440	4441	rBV2	608	366	0.03%	0.003%
98	15.745	4478	4480	4483	rBV2	578	377	0.03%	0.003%
99	15.838	4507	4509	4515	rVB3	669	549	0.04%	0.004%
100	16.131	4598	4600	4603	rBV4	706	431	0.03%	0.003%




Sum of corrected areas: 12389155

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
Data File : VU051011.D
Acq On : 30 Sep 2022 04:16
Operator : JC/MD
Sample : N4880-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGS5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

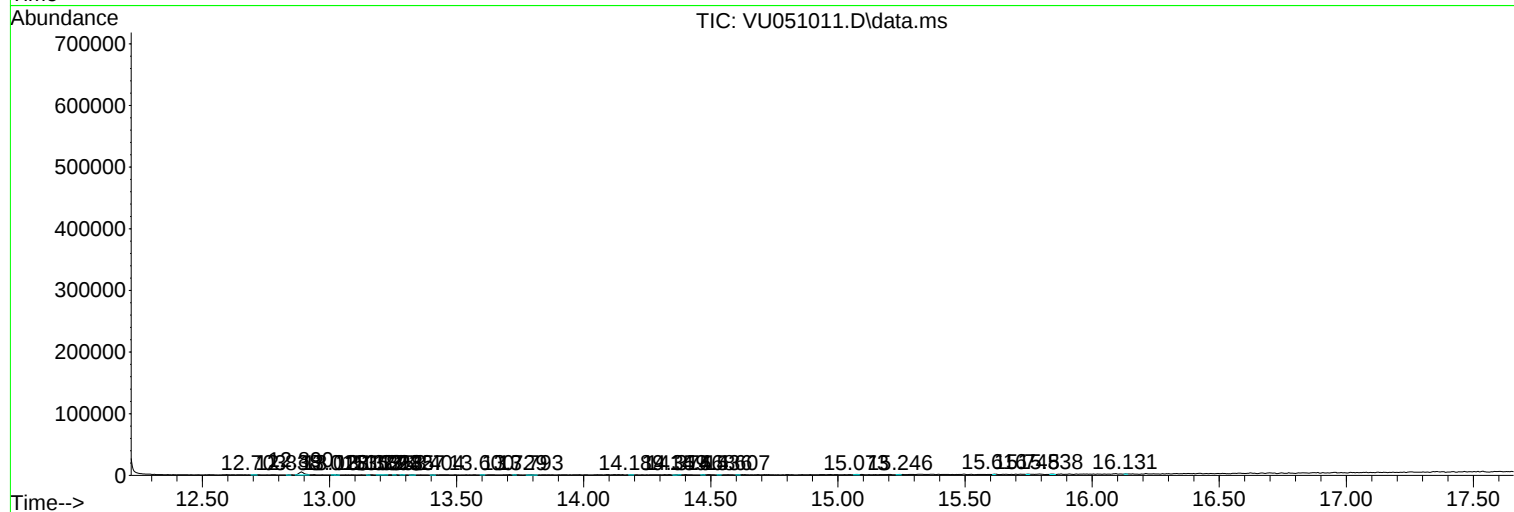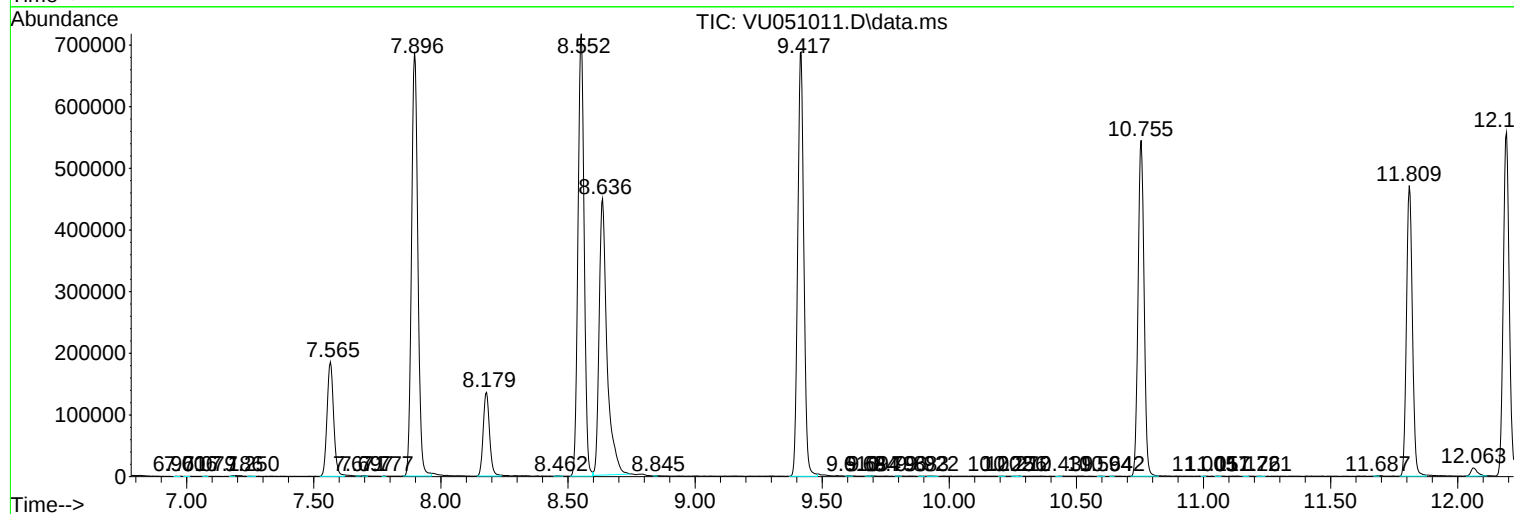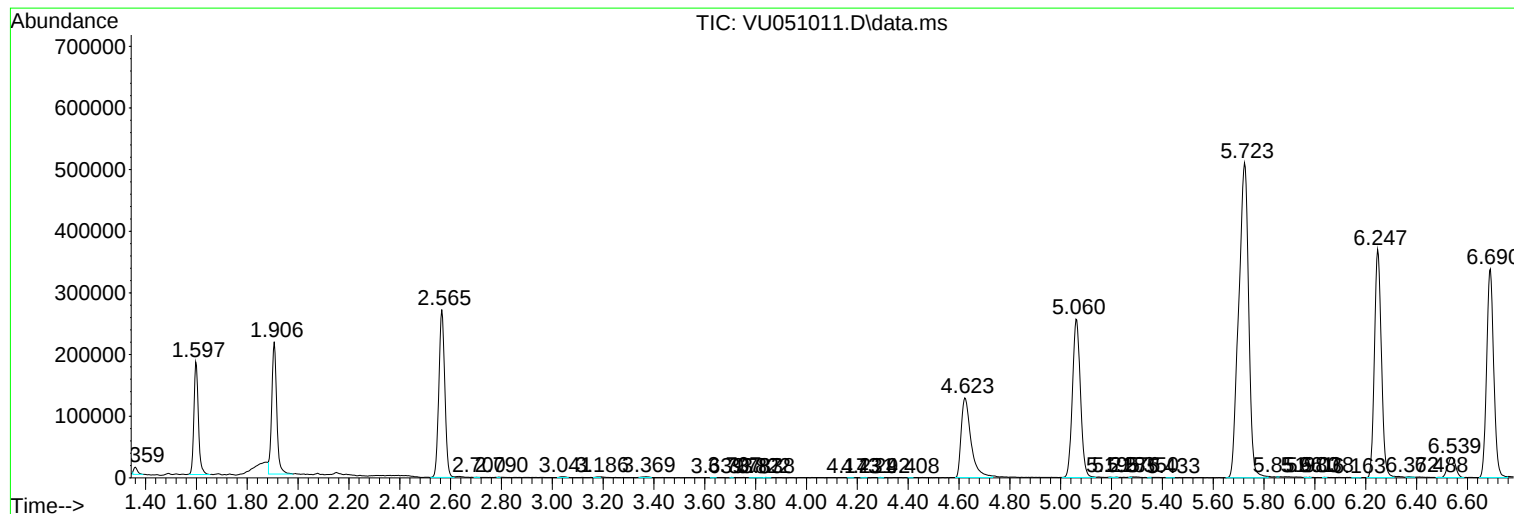

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
Data File : VU051011.D
Acq On : 30 Sep 2022 04:16
Operator : JC/MD
Sample : N4880-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGS5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
Data File : VU051011.D
Acq On : 30 Sep 2022 04:16
Operator : JC/MD
Sample : N4880-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGS5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc