

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
 Data File : VU051012.D
 Acq On : 30 Sep 2022 04:39
 Operator : JC/MD
 Sample : N4880-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGS6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M

Title : VOC Analysis

Signal : TIC: VU051012.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	99	rVB	179140	221102	16.13%	2.119%
2	1.906	169	176	194	rVB	166687	225298	16.44%	2.159%
3	2.565	366	381	393	rBV	273151	445220	32.48%	4.266%
4	2.954	499	502	505	rBV2	660	494	0.04%	0.005%
5	3.041	522	529	531	rBV4	1779	1618	0.12%	0.016%
6	3.112	548	551	554	rVB	312	202	0.01%	0.002%
7	3.182	561	573	576	rBV5	3192	5133	0.37%	0.049%
8	3.282	601	604	605	rBV	169	87	0.01%	0.001%
9	3.308	609	612	614	rBV2	263	168	0.01%	0.002%
10	3.417	644	646	649	rBV	239	119	0.01%	0.001%
11	3.459	656	659	664	rBV	341	231	0.02%	0.002%
12	3.543	682	685	686	rBV2	144	71	0.01%	0.001%
13	3.575	687	695	697	rBV3	2069	2404	0.18%	0.023%
14	3.642	713	716	717	rBV	154	90	0.01%	0.001%
15	3.687	728	730	732	rVB	269	124	0.01%	0.001%
16	3.710	732	737	741	rBV3	514	524	0.04%	0.005%
17	3.787	760	761	764	rVB	221	89	0.01%	0.001%
18	3.842	774	778	783	rVB3	456	484	0.04%	0.005%
19	3.880	786	790	794	rBV	357	327	0.02%	0.003%
20	3.944	809	810	813	rBV2	136	67	0.00%	0.001%
21	3.964	813	816	820	rVB2	230	182	0.01%	0.002%
22	3.983	820	822	827	rBV2	221	203	0.01%	0.002%
23	4.047	840	842	846	rBV2	295	168	0.01%	0.002%
24	4.118	861	864	866	rBV	137	109	0.01%	0.001%
25	4.173	880	881	883	rBV	155	50	0.00%	0.000%
26	4.192	884	887	889	rVV2	196	138	0.01%	0.001%
27	4.218	892	895	897	rVB2	258	139	0.01%	0.001%
28	4.333	928	931	933	rBV	153	108	0.01%	0.001%
29	4.369	938	942	948	rBV2	275	380	0.03%	0.004%
30	4.452	957	968	982	rBV4	3261	7770	0.57%	0.074%
31	4.620	1008	1020	1044	rBV	130583	338826	24.72%	3.247%
32	4.925	1113	1115	1117	rBV	487	171	0.01%	0.002%
33	5.060	1142	1157	1182	rBV	248798	552335	40.30%	5.292%
34	5.414	1264	1267	1271	rBV3	236	208	0.02%	0.002%
35	5.587	1319	1321	1324	rVB2	251	111	0.01%	0.001%
36	5.723	1341	1363	1390	rBV2	505980	1370665	100.00%	13.133%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
 Data File : VU051012.D
 Acq On : 30 Sep 2022 04:39
 Operator : JC/MD
 Sample : N4880-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGS6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	6.102	1478	1481	1482	rBV	305	152	0.01%	0.001%
38	6.247	1512	1526	1549	rBV	380685	721436	52.63%	6.913%
39	6.530	1602	1614	1629	rVB6	11191	21033	1.53%	0.202%
40	6.591	1629	1633	1635	rBV	318	214	0.02%	0.002%
41	6.639	1643	1648	1649	rBV2	413	342	0.02%	0.003%
42	6.690	1649	1664	1685	rVV	327981	641698	46.82%	6.149%
43	6.886	1716	1725	1738	rVV6	4405	8241	0.60%	0.079%
44	6.935	1738	1740	1742	rVB	576	248	0.02%	0.002%
45	6.989	1755	1757	1759	rBV	211	107	0.01%	0.001%
46	7.025	1766	1768	1770	rBV	220	118	0.01%	0.001%
47	7.070	1779	1782	1785	rVB	191	109	0.01%	0.001%
48	7.089	1785	1788	1789	rBV	180	85	0.01%	0.001%
49	7.102	1789	1792	1793	rVV	144	61	0.00%	0.001%
50	7.112	1793	1795	1797	rVB	192	62	0.00%	0.001%
51	7.124	1797	1799	1803	rBV2	323	244	0.02%	0.002%
52	7.189	1812	1819	1825	rBV5	1253	1646	0.12%	0.016%
53	7.359	1869	1872	1876	rBV2	366	238	0.02%	0.002%
54	7.394	1881	1883	1887	rVB2	238	144	0.01%	0.001%
55	7.417	1887	1890	1896	rBV2	253	334	0.02%	0.003%
56	7.494	1912	1914	1917	rVB	210	115	0.01%	0.001%
57	7.513	1917	1920	1922	rBV	373	291	0.02%	0.003%
58	7.565	1923	1936	1952	rBV	163958	292151	21.31%	2.799%
59	7.896	2026	2039	2055	rBV	704425	1217676	88.84%	11.667%
60	8.179	2115	2127	2139	rBV	127557	215031	15.69%	2.060%
61	8.552	2234	2243	2251	rBV4	8654	13948	1.02%	0.134%
62	8.632	2256	2268	2306	rBV3	421608	931550	67.96%	8.926%
63	8.886	2343	2347	2348	rBV2	734	481	0.04%	0.005%
64	9.031	2386	2392	2395	rBV2	358	377	0.03%	0.004%
65	9.176	2435	2437	2441	rBV	331	184	0.01%	0.002%
66	9.414	2499	2511	2543	rBV	588922	975187	71.15%	9.344%
67	9.767	2618	2621	2623	rBV3	396	269	0.02%	0.003%
68	9.880	2653	2656	2658	rBV2	198	164	0.01%	0.002%
69	10.034	2700	2704	2709	rBV2	437	417	0.03%	0.004%
70	10.179	2745	2749	2751	rBV2	286	204	0.01%	0.002%
71	10.237	2763	2767	2768	rBV	499	327	0.02%	0.003%
72	10.346	2787	2801	2810	rBV4	2588	4003	0.29%	0.038%
73	10.401	2816	2818	2820	rBV	150	73	0.01%	0.001%
74	10.626	2885	2888	2892	rBV	385	265	0.02%	0.003%
75	10.754	2914	2928	2950	rBV	467550	750405	54.75%	7.190%
76	10.960	2990	2992	2996	rVB2	245	148	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
 Data File : VU051012.D
 Acq On : 30 Sep 2022 04:39
 Operator : JC/MD
 Sample : N4880-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGS6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	10.992	2996	3002	3006	rBV2	310	335	0.02%	0.003%
78	11.012	3006	3008	3010	rBV2	224	124	0.01%	0.001%
79	11.034	3012	3015	3016	rBV	291	138	0.01%	0.001%
80	11.102	3033	3036	3037	rBV	325	166	0.01%	0.002%
81	11.459	3144	3147	3148	rBV	211	119	0.01%	0.001%
82	11.533	3169	3170	3172	rBV	268	127	0.01%	0.001%
83	11.568	3178	3181	3185	rBV	381	351	0.03%	0.003%
84	11.687	3208	3218	3229	rVB4	6462	9509	0.69%	0.091%
85	11.809	3244	3256	3276	rBV	407266	654166	47.73%	6.268%
86	12.063	3327	3335	3351	rBV5	6615	12152	0.89%	0.116%
87	12.192	3363	3375	3401	rVB	471225	770616	56.22%	7.384%
88	12.324	3414	3416	3418	rBV3	402	152	0.01%	0.001%
89	12.394	3435	3438	3442	rVB	427	238	0.02%	0.002%
90	12.803	3563	3565	3566	rBV	245	108	0.01%	0.001%
91	12.889	3584	3592	3607	rVB7	6992	12331	0.90%	0.118%
92	14.163	3984	3988	3992	rBV2	687	730	0.05%	0.007%




Sum of corrected areas: 10436555

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
Data File : VU051012.D
Acq On : 30 Sep 2022 04:39
Operator : JC/MD
Sample : N4880-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGS6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

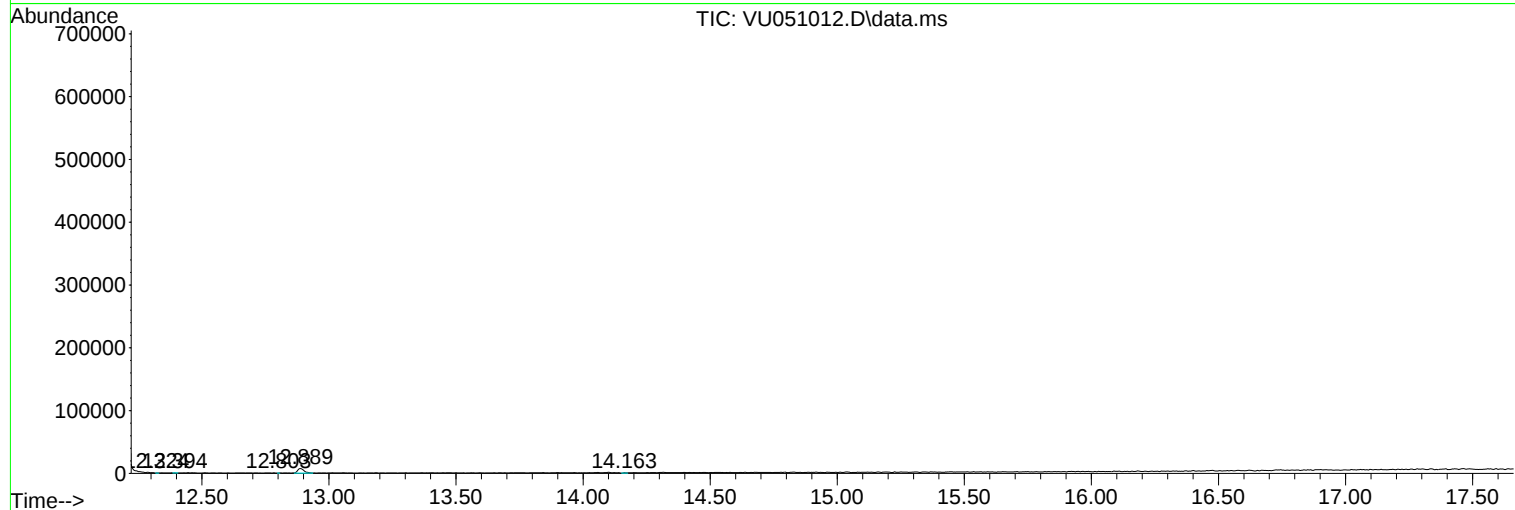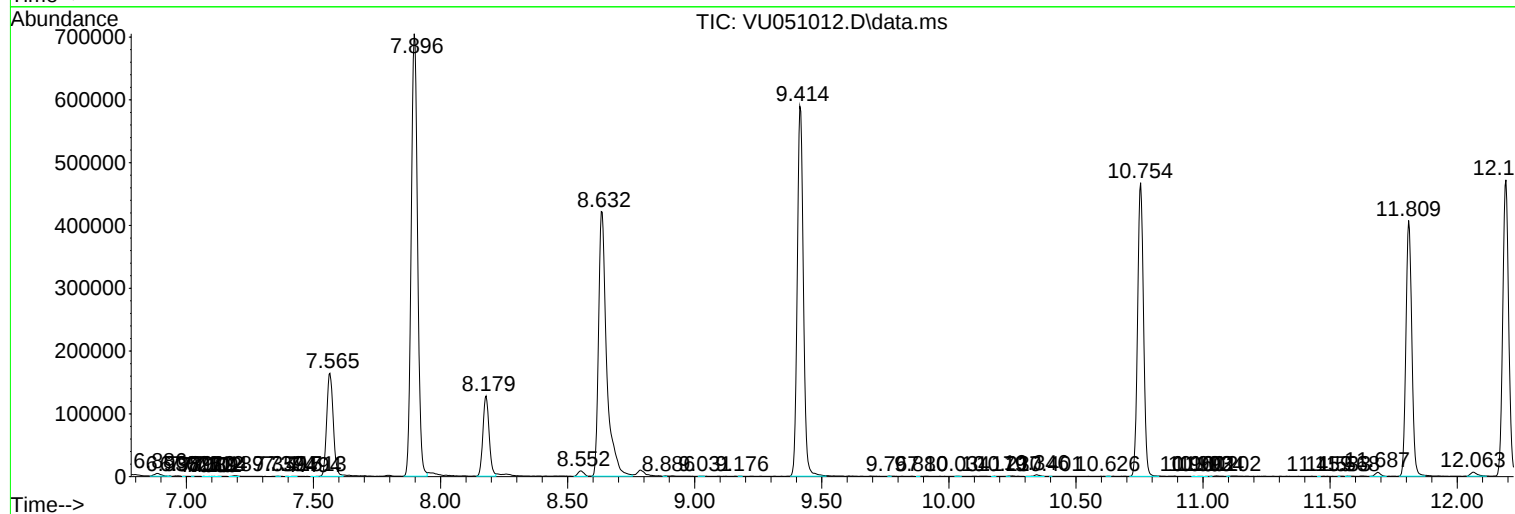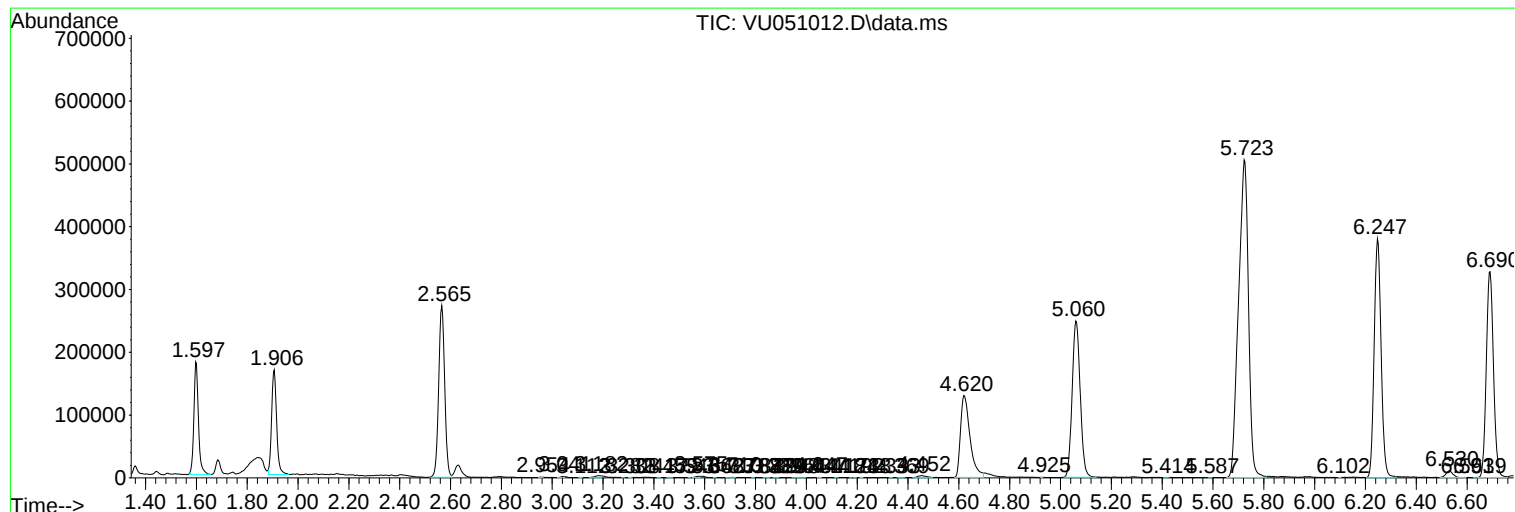

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
Data File : VU051012.D
Acq On : 30 Sep 2022 04:39
Operator : JC/MD
Sample : N4880-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGSH6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
Data File : VU051012.D
Acq On : 30 Sep 2022 04:39
Operator : JC/MD
Sample : N4880-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGSH6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------