

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
 Data File : VU051013.D
 Acq On : 30 Sep 2022 05:03
 Operator : JC/MD
 Sample : N4880-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGSJ1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

Signal : TIC: VU051013.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	99	rVB	169090	206348	15.64%	1.988%
2	1.906	168	176	191	rVB	159257	213136	16.15%	2.053%
3	2.565	368	381	394	rBV	259997	422486	32.01%	4.069%
4	2.629	397	401	409	rVB	3168	4406	0.33%	0.042%
5	2.793	442	452	464	rBV	4613	7675	0.58%	0.074%
6	3.047	520	531	537	rBV6	1777	3097	0.23%	0.030%
7	3.112	546	551	555	rVB2	359	375	0.03%	0.004%
8	3.173	566	570	572	rBV2	799	651	0.05%	0.006%
9	3.581	689	697	702	rVV4	821	1136	0.09%	0.011%
10	3.604	702	704	711	rVB4	553	535	0.04%	0.005%
11	3.645	711	717	721	rBV2	328	438	0.03%	0.004%
12	4.462	968	971	974	rVV3	555	396	0.03%	0.004%
13	4.620	1007	1020	1064	rBV	126233	340226	25.78%	3.277%
14	4.806	1075	1078	1081	rVB2	477	276	0.02%	0.003%
15	5.060	1142	1157	1177	rVV	249101	543668	41.20%	5.237%
16	5.372	1251	1254	1257	rVB3	687	503	0.04%	0.005%
17	5.649	1334	1340	1342	rBV	251	274	0.02%	0.003%
18	5.723	1342	1363	1398	rVV2	487133	1319658	100.00%	12.711%
19	6.034	1455	1460	1463	rBV	501	378	0.03%	0.004%
20	6.169	1496	1502	1506	rBV3	432	568	0.04%	0.005%
21	6.247	1510	1526	1550	rBV	367397	702720	53.25%	6.769%
22	6.530	1604	1614	1628	rVB4	11639	22834	1.73%	0.220%
23	6.584	1628	1631	1635	rBV2	446	394	0.03%	0.004%
24	6.607	1635	1638	1642	rVB2	413	286	0.02%	0.003%
25	6.687	1648	1663	1682	rBV	311198	611267	46.32%	5.888%
26	6.886	1720	1725	1726	rBV3	1124	924	0.07%	0.009%
27	6.941	1737	1742	1746	rBV2	276	283	0.02%	0.003%
28	6.967	1746	1750	1752	rBV2	639	576	0.04%	0.006%
29	7.131	1793	1801	1805	rBV3	525	683	0.05%	0.007%
30	7.189	1811	1819	1825	rVB3	982	1207	0.09%	0.012%
31	7.439	1891	1897	1902	rBV2	361	518	0.04%	0.005%
32	7.485	1907	1911	1916	rBV2	265	325	0.02%	0.003%
33	7.565	1919	1936	1955	rBV	144514	257365	19.50%	2.479%
34	7.787	1999	2005	2007	rBV3	435	387	0.03%	0.004%
35	7.796	2007	2008	2013	rVB	600	429	0.03%	0.004%
36	7.896	2026	2039	2056	rBV	542701	933471	70.74%	8.991%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
 Data File : VU051013.D
 Acq On : 30 Sep 2022 05:03
 Operator : JC/MD
 Sample : N4880-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGSJ1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	8.041	2082	2084	2092	rVB2	456	421	0.03%	0.004%
38	8.179	2115	2127	2143	rBV	103491	178305	13.51%	1.717%
39	8.330	2172	2174	2178	rVB3	366	274	0.02%	0.003%
40	8.411	2196	2199	2205	rVB3	390	415	0.03%	0.004%
41	8.443	2205	2209	2212	rVB3	485	306	0.02%	0.003%
42	8.552	2232	2243	2254	rVV2	32980	54641	4.14%	0.526%
43	8.632	2255	2268	2303	rBV3	335295	730886	55.38%	7.040%
44	8.935	2360	2362	2366	rBV3	439	342	0.03%	0.003%
45	9.195	2439	2443	2448	rBV	394	450	0.03%	0.004%
46	9.295	2470	2474	2478	rBV2	357	316	0.02%	0.003%
47	9.417	2498	2512	2536	rBV	554994	922586	69.91%	8.886%
48	9.539	2546	2550	2555	rVB3	547	518	0.04%	0.005%
49	9.642	2577	2582	2583	rBV3	336	282	0.02%	0.003%
50	9.687	2593	2596	2599	rBV2	484	434	0.03%	0.004%
51	10.211	2756	2759	2762	rBV2	373	286	0.02%	0.003%
52	10.308	2785	2789	2795	rBV2	340	429	0.03%	0.004%
53	10.346	2795	2801	2809	rBV6	2862	4513	0.34%	0.043%
54	10.484	2839	2844	2846	rBV2	398	394	0.03%	0.004%
55	10.542	2859	2862	2868	rVB2	388	350	0.03%	0.003%
56	10.574	2868	2872	2873	rBV	558	329	0.02%	0.003%
57	10.645	2886	2894	2899	rBV5	1218	1662	0.13%	0.016%
58	10.754	2915	2928	2951	rBV	558862	904110	68.51%	8.708%
59	10.902	2971	2974	2978	rVB3	534	479	0.04%	0.005%
60	10.999	2997	3004	3012	rBV6	2271	3789	0.29%	0.036%
61	11.086	3023	3031	3038	rBV4	3202	4665	0.35%	0.045%
62	11.144	3046	3049	3052	rBV	503	310	0.02%	0.003%
63	11.256	3081	3084	3089	rVB2	498	464	0.04%	0.004%
64	11.282	3089	3092	3094	rBV	470	328	0.02%	0.003%
65	11.298	3094	3097	3103	rVB4	1216	1167	0.09%	0.011%
66	11.375	3118	3121	3127	rBV3	616	572	0.04%	0.006%
67	11.433	3135	3139	3141	rBV2	378	296	0.02%	0.003%
68	11.468	3141	3150	3161	rVB2	6641	9435	0.71%	0.091%
69	11.513	3161	3164	3168	rBV3	700	467	0.04%	0.004%
70	11.632	3196	3201	3209	rVB3	1019	1346	0.10%	0.013%
71	11.687	3210	3218	3228	rBV4	7961	12073	0.91%	0.116%
72	11.745	3228	3236	3244	rVB4	11530	16546	1.25%	0.159%
73	11.809	3244	3256	3276	rBV	504966	825502	62.55%	7.951%
74	11.889	3278	3281	3283	rBV3	1941	1180	0.09%	0.011%
75	11.938	3292	3296	3298	rBV3	901	764	0.06%	0.007%
76	12.063	3325	3335	3346	rBV2	9212	18454	1.40%	0.178%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
 Data File : VU051013.D
 Acq On : 30 Sep 2022 05:03
 Operator : JC/MD
 Sample : N4880-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGSJ1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	12.192	3363	3375	3399	rBV	584608	995805	75.46%	9.592%
78	12.343	3420	3422	3426	rBV3	673	553	0.04%	0.005%
79	12.375	3427	3432	3436	rVV5	1715	1711	0.13%	0.016%
80	12.462	3451	3459	3464	rBV9	2708	4064	0.31%	0.039%
81	12.549	3482	3486	3487	rBV3	938	583	0.04%	0.006%
82	12.568	3487	3492	3501	rVB3	3501	4793	0.36%	0.046%
83	12.700	3528	3533	3536	rBV4	1304	1427	0.11%	0.014%
84	12.886	3581	3591	3605	rBV6	14661	25131	1.90%	0.242%
85	12.973	3616	3618	3626	rVB5	1232	1036	0.08%	0.010%
86	13.028	3628	3635	3648	rVB7	3108	5037	0.38%	0.049%
87	13.131	3664	3667	3674	rBV5	762	941	0.07%	0.009%
88	13.208	3685	3691	3694	rBV5	688	698	0.05%	0.007%
89	13.250	3701	3704	3706	rBV2	673	410	0.03%	0.004%
90	13.278	3710	3713	3718	rVV4	542	519	0.04%	0.005%
91	13.449	3759	3766	3776	rVB5	2000	2798	0.21%	0.027%
92	13.513	3780	3786	3790	rBV6	1167	1243	0.09%	0.012%
93	13.619	3816	3819	3823	rBV3	772	554	0.04%	0.005%
94	13.777	3860	3868	3872	rBV2	548	868	0.07%	0.008%
95	13.841	3879	3888	3901	rBV3	12831	21111	1.60%	0.203%
96	14.028	3943	3946	3948	rBV3	351	276	0.02%	0.003%
97	14.089	3958	3965	3976	rBV	2331	4243	0.32%	0.041%
98	14.330	4033	4040	4052	rVB4	4239	7242	0.55%	0.070%
99	14.950	4231	4233	4239	rBV3	508	462	0.04%	0.004%
100	15.150	4292	4295	4299	rBV2	591	577	0.04%	0.006%




Sum of corrected areas: 10382067

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
Data File : VU051013.D
Acq On : 30 Sep 2022 05:03
Operator : JC/MD
Sample : N4880-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGSJ1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

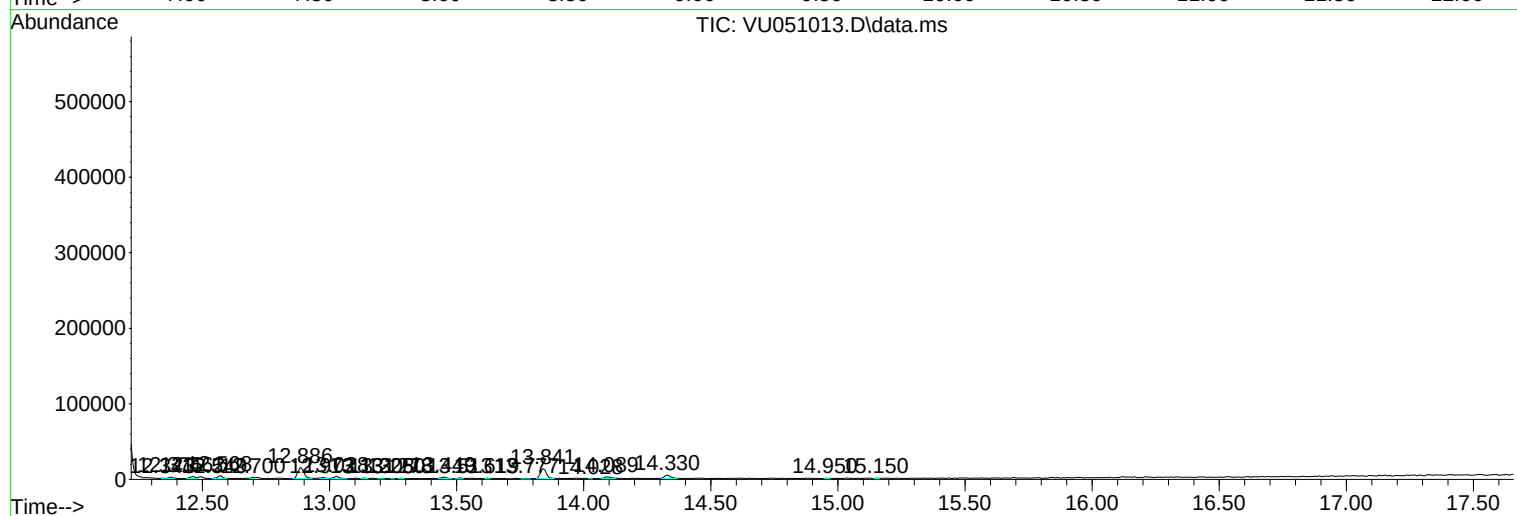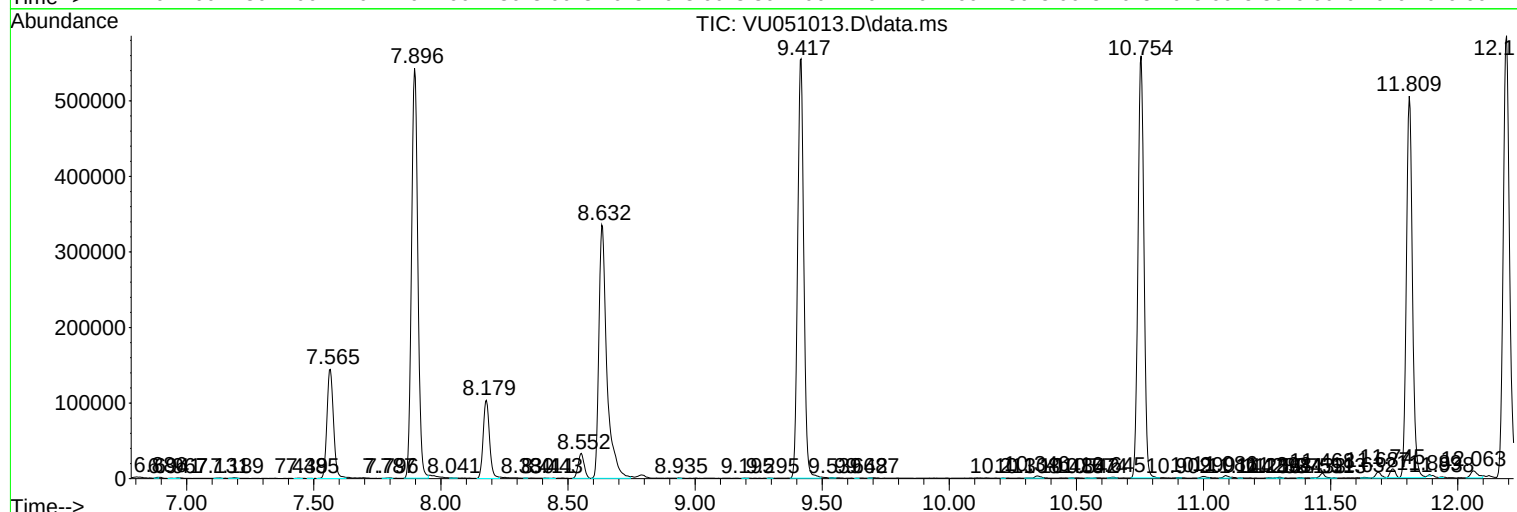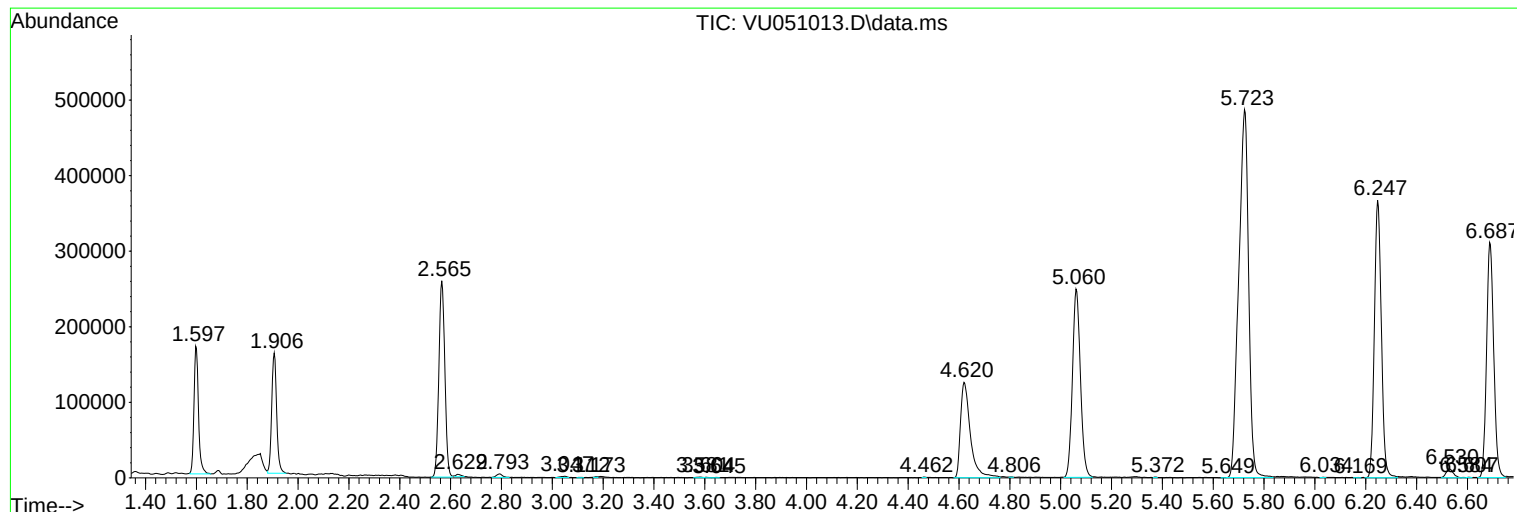

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
Data File : VU051013.D
Acq On : 30 Sep 2022 05:03
Operator : JC/MD
Sample : N4880-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGSJ1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
Data File : VU051013.D
Acq On : 30 Sep 2022 05:03
Operator : JC/MD
Sample : N4880-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGSJ1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc