

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
 Data File : VU051014.D
 Acq On : 30 Sep 2022 05:26
 Operator : JC/MD
 Sample : N4880-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGSJ2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

Signal : TIC: VU051014.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.359	3	6	15	rVB4	5638	5431	0.41%	0.053%
2	1.597	72	80	97	rVB	176095	214456	16.12%	2.096%
3	1.684	102	107	117	rBV	9273	10159	0.76%	0.099%
4	1.906	167	176	190	rVB	163495	212934	16.00%	2.081%
5	2.565	367	381	394	rBV	265208	431740	32.45%	4.219%
6	2.633	394	402	412	rVB2	5938	11227	0.84%	0.110%
7	2.793	443	452	464	rVV	4127	7112	0.53%	0.070%
8	2.845	465	468	469	rVV2	417	259	0.02%	0.003%
9	2.858	469	472	478	rVB5	793	752	0.06%	0.007%
10	2.954	494	502	506	rBV2	584	620	0.05%	0.006%
11	3.041	523	529	531	rBV4	1520	1475	0.11%	0.014%
12	3.166	564	568	569	rBV2	1017	597	0.04%	0.006%
13	3.588	692	699	703	rBV2	528	748	0.06%	0.007%
14	3.819	765	771	777	rBV2	299	430	0.03%	0.004%
15	4.250	898	905	911	rBV2	524	815	0.06%	0.008%
16	4.456	964	969	970	rBV2	785	661	0.05%	0.006%
17	4.620	1007	1020	1048	rBV	129812	333085	25.04%	3.255%
18	4.819	1077	1082	1084	rBV3	817	593	0.04%	0.006%
19	5.060	1140	1157	1184	rBV	249794	549859	41.33%	5.374%
20	5.237	1209	1212	1218	rVB3	489	479	0.04%	0.005%
21	5.285	1223	1227	1229	rBV2	601	550	0.04%	0.005%
22	5.362	1249	1251	1255	rVB2	384	260	0.02%	0.003%
23	5.723	1342	1363	1390	rBV2	493841	1330449	100.00%	13.002%
24	6.125	1482	1488	1491	rVV3	485	511	0.04%	0.005%
25	6.247	1512	1526	1548	rBV	358479	684479	51.45%	6.689%
26	6.469	1593	1595	1599	rBV2	489	363	0.03%	0.004%
27	6.530	1604	1614	1627	rVB4	10095	19906	1.50%	0.195%
28	6.690	1648	1664	1685	rBV	318895	619639	46.57%	6.056%
29	6.864	1716	1718	1720	rBV	495	278	0.02%	0.003%
30	6.890	1720	1726	1733	rVB4	1950	2367	0.18%	0.023%
31	6.986	1749	1756	1761	rBV2	249	324	0.02%	0.003%
32	7.128	1795	1800	1807	rBV4	641	851	0.06%	0.008%
33	7.182	1812	1817	1819	rBV3	526	473	0.04%	0.005%
34	7.269	1837	1844	1851	rBV	442	611	0.05%	0.006%
35	7.388	1876	1881	1885	rBV	285	367	0.03%	0.004%
36	7.520	1917	1922	1923	rBV	338	301	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
 Data File : VU051014.D
 Acq On : 30 Sep 2022 05:26
 Operator : JC/MD
 Sample : N4880-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGSJ2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	7.565	1923	1936	1954	rVV2	145454	259129	19.48%	2.532%
38	7.697	1972	1977	1982	rVB3	892	1073	0.08%	0.010%
39	7.768	1995	1999	2002	rVB2	463	350	0.03%	0.003%
40	7.790	2002	2006	2013	rBV3	652	773	0.06%	0.008%
41	7.896	2026	2039	2060	rBV	555589	952274	71.58%	9.307%
42	8.179	2115	2127	2143	rBV	104717	180013	13.53%	1.759%
43	8.353	2179	2181	2185	rVB2	378	282	0.02%	0.003%
44	8.443	2201	2209	2212	rBV2	382	479	0.04%	0.005%
45	8.468	2212	2217	2222	rBV2	410	565	0.04%	0.006%
46	8.552	2231	2243	2256	rBV2	31869	51887	3.90%	0.507%
47	8.632	2256	2268	2305	rBV2	348753	753395	56.63%	7.363%
48	8.861	2337	2339	2345	rVB3	724	677	0.05%	0.007%
49	8.954	2363	2368	2372	rBV	304	306	0.02%	0.003%
50	9.108	2414	2416	2420	rVB2	503	357	0.03%	0.003%
51	9.134	2420	2424	2426	rBV3	412	297	0.02%	0.003%
52	9.150	2426	2429	2439	rVB4	431	394	0.03%	0.004%
53	9.285	2467	2471	2475	rBV3	606	548	0.04%	0.005%
54	9.417	2499	2512	2540	rBV	627964	1058801	79.58%	10.348%
55	9.578	2555	2562	2565	rBV4	727	780	0.06%	0.008%
56	9.694	2594	2598	2605	rVB3	694	724	0.05%	0.007%
57	9.748	2613	2615	2620	rVB	466	299	0.02%	0.003%
58	9.777	2620	2624	2627	rBV2	505	452	0.03%	0.004%
59	10.095	2716	2723	2725	rBV4	670	658	0.05%	0.006%
60	10.128	2731	2733	2738	rVB4	455	367	0.03%	0.004%
61	10.346	2795	2801	2810	rBV7	2946	4577	0.34%	0.045%
62	10.639	2889	2892	2898	rVB5	1418	1510	0.11%	0.015%
63	10.710	2911	2914	2916	rBV2	443	285	0.02%	0.003%
64	10.755	2916	2928	2947	rBV	584923	936138	70.36%	9.149%
65	10.890	2967	2970	2973	rVB2	495	284	0.02%	0.003%
66	10.928	2978	2982	2985	rBV2	285	279	0.02%	0.003%
67	11.063	3018	3024	3025	rBV2	360	351	0.03%	0.003%
68	11.118	3038	3041	3047	rVB4	1093	1017	0.08%	0.010%
69	11.468	3145	3150	3160	rVB3	661	958	0.07%	0.009%
70	11.529	3166	3169	3175	rVB2	455	387	0.03%	0.004%
71	11.629	3197	3200	3208	rBV3	599	707	0.05%	0.007%
72	11.687	3211	3218	3226	rBV6	7783	11165	0.84%	0.109%
73	11.742	3231	3235	3244	rVB4	1283	1649	0.12%	0.016%
74	11.809	3244	3256	3280	rBV	431853	685848	51.55%	6.703%
75	12.063	3322	3335	3348	rBV3	14680	28156	2.12%	0.275%
76	12.192	3362	3375	3393	rBV	500787	816259	61.35%	7.977%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
 Data File : VU051014.D
 Acq On : 30 Sep 2022 05:26
 Operator : JC/MD
 Sample : N4880-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGSJ2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	12.398	3437	3439	3445	rVB2	414	356	0.03%	0.003%
78	12.436	3445	3451	3452	rBV2	414	363	0.03%	0.004%
79	12.472	3459	3462	3466	rBV2	334	264	0.02%	0.003%
80	12.783	3552	3559	3565	rBV2	452	840	0.06%	0.008%
81	12.886	3583	3591	3608	rBV5	12262	19718	1.48%	0.193%
82	13.150	3668	3673	3675	rBV2	416	305	0.02%	0.003%
83	13.391	3745	3748	3755	rVB3	506	577	0.04%	0.006%
84	13.423	3755	3758	3760	rBV	499	275	0.02%	0.003%
85	13.526	3788	3790	3798	rVB2	696	588	0.04%	0.006%
86	13.565	3798	3802	3803	rBV	372	275	0.02%	0.003%
87	13.697	3838	3843	3846	rBV2	396	358	0.03%	0.003%
88	13.841	3884	3888	3895	rVV6	1535	1931	0.15%	0.019%
89	13.896	3902	3905	3908	rBV	534	348	0.03%	0.003%
90	14.037	3946	3949	3955	rBV2	435	357	0.03%	0.003%
91	14.089	3958	3965	3969	rBV3	762	1088	0.08%	0.011%
92	15.201	4309	4311	4314	rVB3	605	359	0.03%	0.004%
93	15.221	4314	4317	4319	rBV	631	400	0.03%	0.004%
94	15.465	4390	4393	4397	rBV2	686	651	0.05%	0.006%
95	15.574	4425	4427	4430	rBV	689	459	0.03%	0.004%
96	15.796	4493	4496	4498	rBV	534	413	0.03%	0.004%
97	15.928	4534	4537	4540	rBV2	846	779	0.06%	0.008%
98	16.031	4566	4569	4572	rBV3	639	549	0.04%	0.005%
99	16.111	4591	4594	4598	rBV5	1234	1042	0.08%	0.010%
100	16.156	4605	4608	4609	rBV3	738	439	0.03%	0.004%




Sum of corrected areas: 10232345

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
Data File : VU051014.D
Acq On : 30 Sep 2022 05:26
Operator : JC/MD
Sample : N4880-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGSJ2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

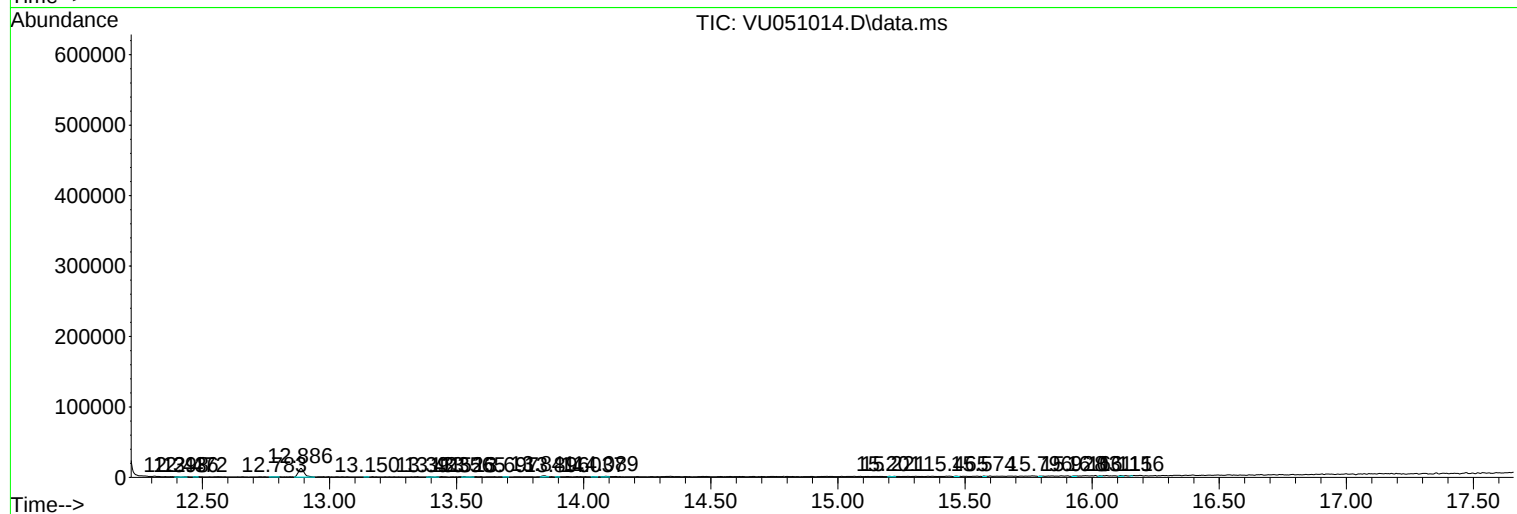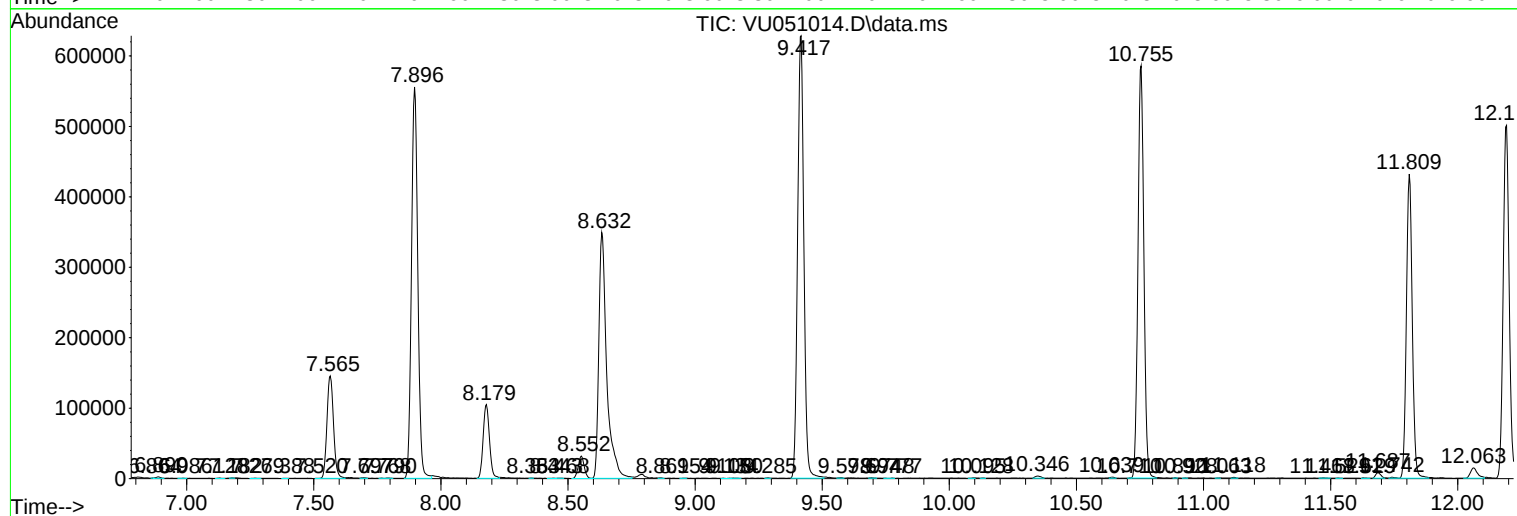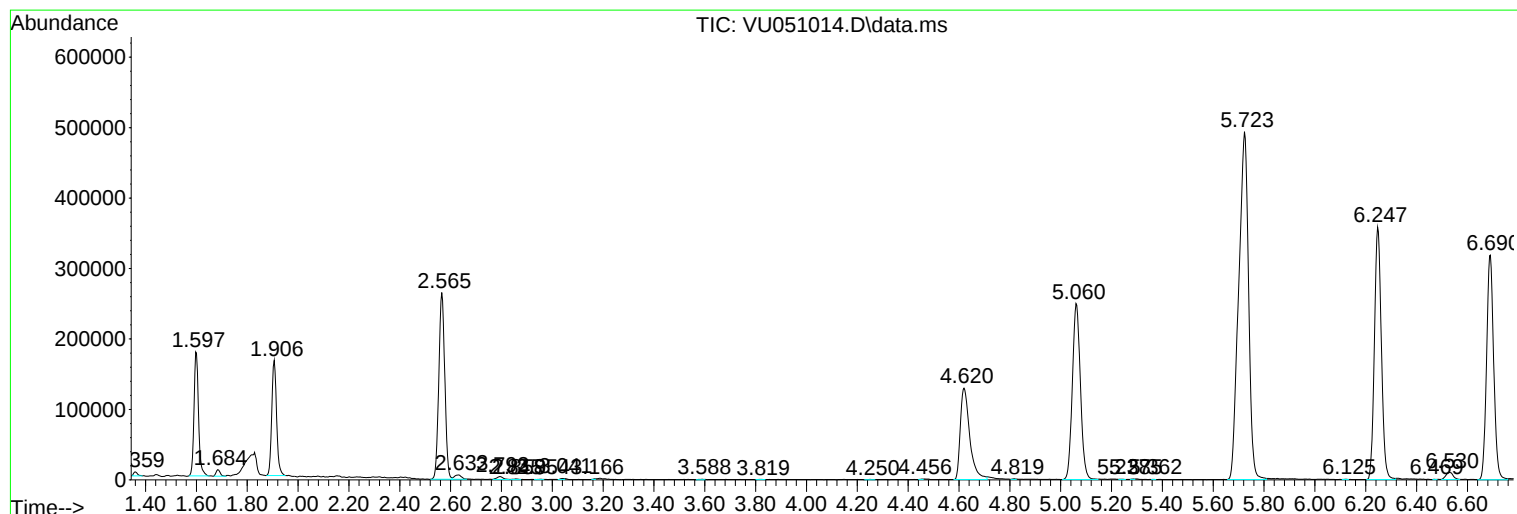

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
Data File : VU051014.D
Acq On : 30 Sep 2022 05:26
Operator : JC/MD
Sample : N4880-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGSJ2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
Data File : VU051014.D
Acq On : 30 Sep 2022 05:26
Operator : JC/MD
Sample : N4880-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGSJ2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------