

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
 Data File : VU051015.D
 Acq On : 30 Sep 2022 05:50
 Operator : JC/MD
 Sample : N4880-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGSJ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

Signal : TIC: VU051015.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	98	rVB	180527	215282	15.61%	1.836%
2	1.912	170	178	192	rBV	205422	264825	19.21%	2.258%
3	2.504	360	362	366	rVB2	365	239	0.02%	0.002%
4	2.565	369	381	397	rBV	269619	434865	31.54%	3.708%
5	2.790	446	451	457	rBV2	1380	1748	0.13%	0.015%
6	2.935	493	496	501	rBV2	432	389	0.03%	0.003%
7	2.967	503	506	509	rVB2	335	220	0.02%	0.002%
8	3.186	567	574	580	rVV3	916	1471	0.11%	0.013%
9	3.446	653	655	659	rVB2	354	230	0.02%	0.002%
10	3.681	724	728	731	rBV2	405	419	0.03%	0.004%
11	3.697	731	733	736	rVV	333	220	0.02%	0.002%
12	3.716	736	739	744	rVV2	230	246	0.02%	0.002%
13	3.858	779	783	788	rBV	223	214	0.02%	0.002%
14	3.909	792	799	801	rBV2	348	388	0.03%	0.003%
15	4.067	845	848	857	rVB2	562	785	0.06%	0.007%
16	4.112	857	862	864	rBV	360	334	0.02%	0.003%
17	4.253	901	906	912	rBV2	292	473	0.03%	0.004%
18	4.285	912	916	922	rVV2	236	267	0.02%	0.002%
19	4.488	973	979	981	rBV	308	242	0.02%	0.002%
20	4.555	997	1000	1004	rVB2	335	267	0.02%	0.002%
21	4.626	1010	1022	1062	rBV	127880	361677	26.23%	3.084%
22	4.928	1112	1116	1117	rBV2	582	336	0.02%	0.003%
23	5.060	1141	1157	1180	rBV	258229	565213	41.00%	4.819%
24	5.211	1202	1204	1207	rBV3	365	229	0.02%	0.002%
25	5.256	1215	1218	1222	rBV	419	292	0.02%	0.002%
26	5.526	1297	1302	1305	rVV2	354	305	0.02%	0.003%
27	5.723	1340	1363	1387	rBV2	506957	1378726	100.00%	11.756%
28	6.247	1512	1526	1548	rBV	376661	717737	52.06%	6.120%
29	6.530	1602	1614	1626	rBV6	10753	20638	1.50%	0.176%
30	6.690	1649	1664	1683	rBV	332432	673371	48.84%	5.742%
31	6.896	1724	1728	1734	rBV2	672	620	0.04%	0.005%
32	7.157	1807	1809	1814	rBV2	275	236	0.02%	0.002%
33	7.182	1814	1817	1819	rBV3	573	419	0.03%	0.004%
34	7.456	1899	1902	1910	rVV	290	380	0.03%	0.003%
35	7.565	1923	1936	1959	rBV	187976	335199	24.31%	2.858%
36	7.745	1987	1992	1995	rBV2	392	364	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
 Data File : VU051015.D
 Acq On : 30 Sep 2022 05:50
 Operator : JC/MD
 Sample : N4880-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGSJ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	7.896	2025	2039	2061	rBV	719773	1257059	91.18%	10.719%
38	8.179	2115	2127	2153	rBV	135474	241067	17.48%	2.056%
39	8.468	2215	2217	2221	rBV2	335	256	0.02%	0.002%
40	8.552	2231	2243	2257	rBV	175079	296880	21.53%	2.531%
41	8.636	2257	2269	2301	rBV3	468931	1048251	76.03%	8.938%
42	8.835	2329	2331	2334	rBV3	605	233	0.02%	0.002%
43	8.996	2379	2381	2386	rBV2	320	293	0.02%	0.002%
44	9.054	2396	2399	2402	rVB2	525	315	0.02%	0.003%
45	9.211	2446	2448	2453	rVB2	303	223	0.02%	0.002%
46	9.240	2453	2457	2460	rVB2	423	298	0.02%	0.003%
47	9.263	2460	2464	2468	rBV2	345	314	0.02%	0.003%
48	9.414	2498	2511	2548	rBV	691485	1154733	83.75%	9.846%
49	9.745	2611	2614	2618	rVB3	385	226	0.02%	0.002%
50	9.825	2634	2639	2640	rBV2	304	248	0.02%	0.002%
51	10.028	2699	2702	2704	rBV	373	253	0.02%	0.002%
52	10.079	2715	2718	2721	rBV2	318	236	0.02%	0.002%
53	10.340	2796	2799	2803	rVB	335	212	0.02%	0.002%
54	10.362	2803	2806	2810	rBV	472	303	0.02%	0.003%
55	10.497	2844	2848	2851	rBV	370	307	0.02%	0.003%
56	10.755	2915	2928	2951	rBV	596027	957358	69.44%	8.163%
57	10.915	2975	2978	2981	rBV2	400	239	0.02%	0.002%
58	11.118	3038	3041	3044	rVB2	584	404	0.03%	0.003%
59	11.565	3176	3180	3183	rVB2	358	252	0.02%	0.002%
60	11.587	3184	3187	3189	rBV	323	225	0.02%	0.002%
61	11.623	3196	3198	3208	rVB3	413	423	0.03%	0.004%
62	11.684	3212	3217	3224	rBV4	1239	1305	0.09%	0.011%
63	11.745	3232	3236	3244	rVB2	932	922	0.07%	0.008%
64	11.809	3244	3256	3277	rBV	494824	801388	58.13%	6.833%
65	11.992	3310	3313	3316	rBV2	463	248	0.02%	0.002%
66	12.066	3326	3336	3347	rBV4	8037	15174	1.10%	0.129%
67	12.137	3356	3358	3360	rBV2	350	230	0.02%	0.002%
68	12.192	3360	3375	3393	rBV	586643	954463	69.23%	8.138%
69	12.369	3427	3430	3433	rBV2	366	282	0.02%	0.002%
70	12.517	3469	3476	3479	rBV2	362	434	0.03%	0.004%
71	12.777	3553	3557	3559	rBV	308	251	0.02%	0.002%
72	12.828	3570	3573	3581	rVB2	439	414	0.03%	0.004%
73	12.896	3585	3594	3602	rVB5	1949	2344	0.17%	0.020%
74	12.976	3616	3619	3622	rBV2	318	229	0.02%	0.002%
75	13.057	3642	3644	3649	rBV3	320	314	0.02%	0.003%
76	13.134	3663	3668	3672	rVV	420	402	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
 Data File : VU051015.D
 Acq On : 30 Sep 2022 05:50
 Operator : JC/MD
 Sample : N4880-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGSJ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	13.153	3672	3674	3676	rVV	404	229	0.02%	0.002%
78	13.185	3679	3684	3689	rVV2	583	712	0.05%	0.006%
79	13.211	3689	3692	3697	rVB3	738	552	0.04%	0.005%
80	13.404	3750	3752	3755	rVB2	416	234	0.02%	0.002%
81	13.430	3757	3760	3767	rVB2	235	206	0.01%	0.002%
82	13.545	3793	3796	3799	rVB2	372	246	0.02%	0.002%
83	13.607	3813	3815	3819	rBV2	396	225	0.02%	0.002%
84	13.655	3828	3830	3835	rBV2	232	216	0.02%	0.002%
85	13.716	3846	3849	3852	rBV3	341	266	0.02%	0.002%
86	13.848	3886	3890	3893	rBV2	787	653	0.05%	0.006%
87	13.906	3905	3908	3910	rBV	299	215	0.02%	0.002%
88	13.983	3922	3932	3934	rBV3	592	872	0.06%	0.007%
89	14.195	3995	3998	4001	rVB3	427	306	0.02%	0.003%
90	14.404	4060	4063	4067	rVB3	295	237	0.02%	0.002%
91	14.426	4067	4070	4074	rVB	541	419	0.03%	0.004%
92	14.742	4164	4168	4169	rBV	449	309	0.02%	0.003%
93	14.835	4194	4197	4198	rBV	559	318	0.02%	0.003%
94	14.992	4243	4246	4251	rBV	487	343	0.02%	0.003%
95	15.674	4455	4458	4460	rBV2	753	459	0.03%	0.004%
96	15.777	4488	4490	4493	rVB2	675	363	0.03%	0.003%
97	15.957	4543	4546	4548	rBV3	593	368	0.03%	0.003%
98	16.015	4561	4564	4568	rBV3	760	614	0.04%	0.005%
99	16.050	4573	4575	4577	rBV2	653	355	0.03%	0.003%
100	16.176	4610	4614	4621	rBV5	905	1238	0.09%	0.011%




Sum of corrected areas: 11727829

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
Data File : VU051015.D
Acq On : 30 Sep 2022 05:50
Operator : JC/MD
Sample : N4880-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGSJ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

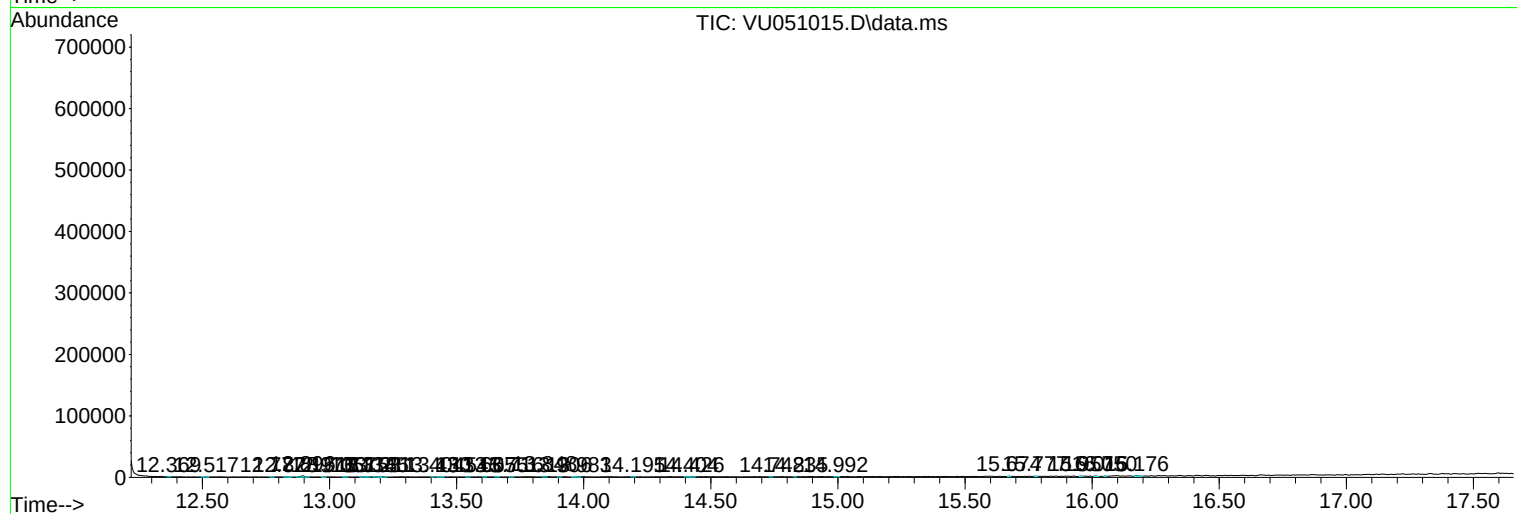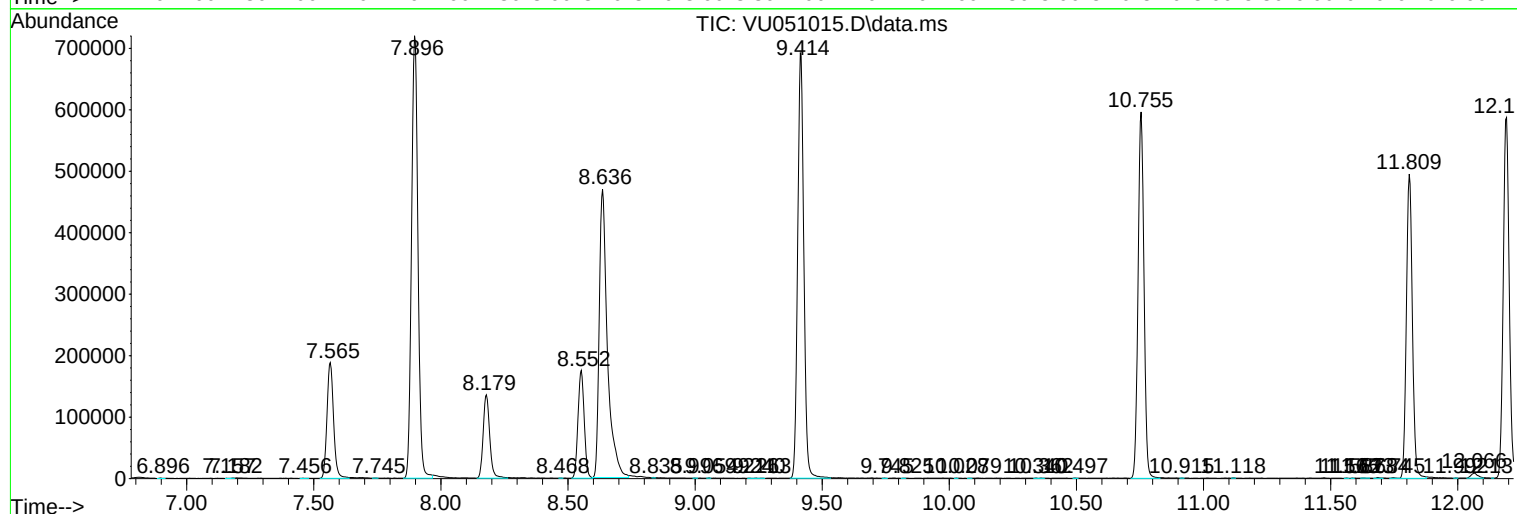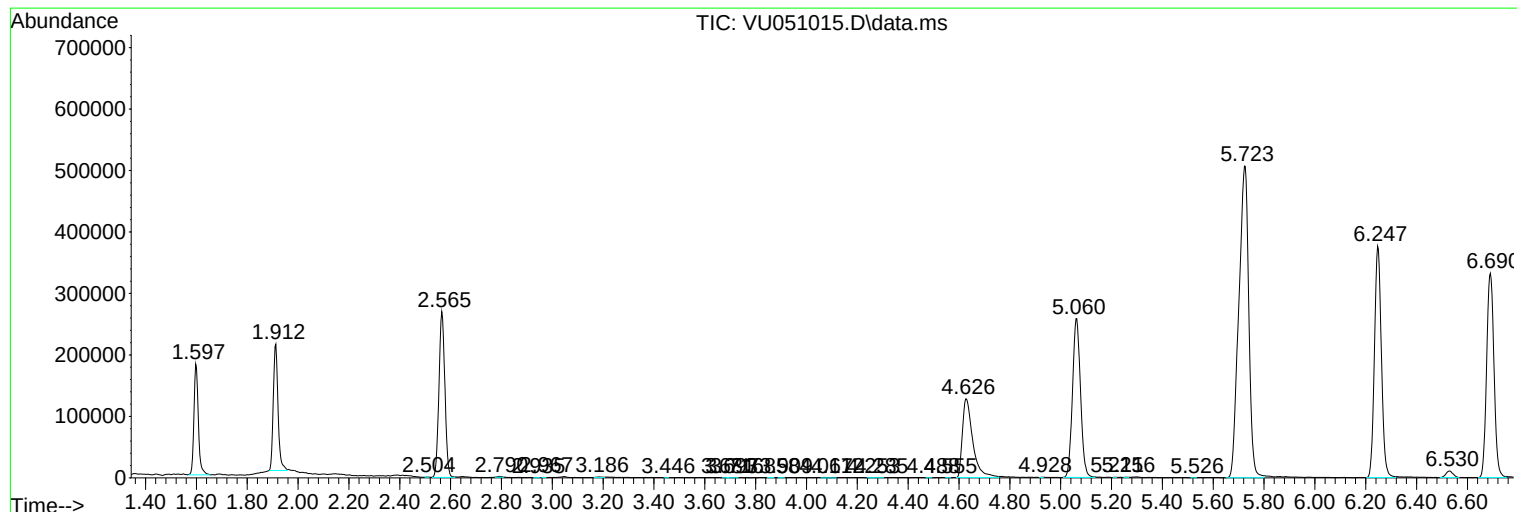

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
Data File : VU051015.D
Acq On : 30 Sep 2022 05:50
Operator : JC/MD
Sample : N4880-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGSJ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
Data File : VU051015.D
Acq On : 30 Sep 2022 05:50
Operator : JC/MD
Sample : N4880-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGSJ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------