

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
 Data File : VU051016.D
 Acq On : 30 Sep 2022 06:13
 Operator : JC/MD
 Sample : N4880-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGSJ4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

Signal : TIC: VU051016.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	72	81	100	rVB	177809	218091	16.14%	2.057%
2	1.906	169	176	196	rVB	203420	276210	20.44%	2.605%
3	2.520	365	367	368	rBV	428	202	0.01%	0.002%
4	2.565	368	381	396	rVV	342468	552992	40.92%	5.215%
5	2.790	443	451	459	rBV4	1999	3688	0.27%	0.035%
6	2.864	472	474	478	rBV4	310	153	0.01%	0.001%
7	3.044	523	530	539	rVB6	1316	2143	0.16%	0.020%
8	3.105	546	549	551	rBV	563	394	0.03%	0.004%
9	3.186	559	574	588	rBV3	3164	7563	0.56%	0.071%
10	3.363	619	629	637	rBV5	1917	3653	0.27%	0.034%
11	3.395	637	639	642	rVB	434	220	0.02%	0.002%
12	3.446	653	655	660	rBV2	358	295	0.02%	0.003%
13	3.665	721	723	725	rVV	309	143	0.01%	0.001%
14	3.678	725	727	729	rVB	285	136	0.01%	0.001%
15	3.755	749	751	755	rBV	263	202	0.01%	0.002%
16	3.822	767	772	777	rBV2	562	893	0.07%	0.008%
17	3.861	781	784	786	rBV2	362	252	0.02%	0.002%
18	4.028	833	836	841	rBV2	219	238	0.02%	0.002%
19	4.070	846	849	851	rBV	314	225	0.02%	0.002%
20	4.517	982	988	990	rBV2	207	218	0.02%	0.002%
21	4.623	1008	1021	1047	rBV	133674	347994	25.75%	3.282%
22	4.829	1081	1085	1086	rBV2	453	277	0.02%	0.003%
23	5.060	1141	1157	1179	rBV	250822	553246	40.94%	5.217%
24	5.215	1200	1205	1206	rBV3	594	523	0.04%	0.005%
25	5.282	1221	1226	1237	rVB6	976	1904	0.14%	0.018%
26	5.327	1237	1240	1244	rVB3	414	330	0.02%	0.003%
27	5.375	1251	1255	1257	rBV2	342	244	0.02%	0.002%
28	5.388	1257	1259	1262	rBV2	364	226	0.02%	0.002%
29	5.723	1342	1363	1390	rBV2	498703	1351346	100.00%	12.743%
30	5.858	1402	1405	1408	rBV4	452	328	0.02%	0.003%
31	6.015	1450	1454	1456	rBV2	325	231	0.02%	0.002%
32	6.247	1512	1526	1551	rBV	373837	702697	52.00%	6.626%
33	6.343	1554	1556	1563	rVB4	664	492	0.04%	0.005%
34	6.436	1583	1585	1588	rBV3	312	232	0.02%	0.002%
35	6.526	1603	1613	1628	rVB5	10137	18879	1.40%	0.178%
36	6.690	1649	1664	1682	rBV	321553	632832	46.83%	5.968%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
 Data File : VU051016.D
 Acq On : 30 Sep 2022 06:13
 Operator : JC/MD
 Sample : N4880-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGSJ4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	6.797	1694	1697	1700	rBV4	1071	934	0.07%	0.009%
38	6.867	1717	1719	1721	rVB2	356	170	0.01%	0.002%
39	6.883	1721	1724	1729	rBV2	631	562	0.04%	0.005%
40	6.989	1754	1757	1760	rVV2	256	150	0.01%	0.001%
41	7.022	1763	1767	1769	rVV2	440	294	0.02%	0.003%
42	7.131	1798	1801	1802	rBV2	436	212	0.02%	0.002%
43	7.186	1813	1818	1819	rBV3	659	518	0.04%	0.005%
44	7.221	1826	1829	1834	rVB4	433	365	0.03%	0.003%
45	7.285	1842	1849	1852	rBV2	396	555	0.04%	0.005%
46	7.501	1913	1916	1919	rBV2	265	188	0.01%	0.002%
47	7.565	1923	1936	1959	rVV	147469	264539	19.58%	2.495%
48	7.681	1970	1972	1976	rBV3	445	390	0.03%	0.004%
49	7.739	1987	1990	1994	rBV	659	394	0.03%	0.004%
50	7.793	2003	2007	2009	rVV	590	485	0.04%	0.005%
51	7.809	2009	2012	2019	rVB2	837	865	0.06%	0.008%
52	7.896	2026	2039	2062	rBV	562176	976866	72.29%	9.212%
53	8.179	2114	2127	2145	rBV	107256	181427	13.43%	1.711%
54	8.501	2225	2227	2230	rVB2	323	148	0.01%	0.001%
55	8.552	2235	2243	2252	rVB4	3927	5956	0.44%	0.056%
56	8.636	2256	2269	2301	rBV3	351703	769864	56.97%	7.260%
57	8.886	2346	2347	2350	rVB3	542	200	0.01%	0.002%
58	8.909	2350	2354	2357	rBV2	543	386	0.03%	0.004%
59	9.063	2399	2402	2404	rVV	316	174	0.01%	0.002%
60	9.340	2485	2488	2491	rBV	268	195	0.01%	0.002%
61	9.417	2498	2512	2538	rBV	547017	908132	67.20%	8.564%
62	9.587	2562	2565	2569	rVB3	366	239	0.02%	0.002%
63	9.652	2582	2585	2586	rBV3	406	243	0.02%	0.002%
64	9.697	2596	2599	2603	rVB3	322	247	0.02%	0.002%
65	10.009	2693	2696	2699	rBV	300	204	0.02%	0.002%
66	10.028	2699	2702	2704	rBV	212	152	0.01%	0.001%
67	10.150	2738	2740	2743	rVV2	303	174	0.01%	0.002%
68	10.240	2765	2768	2770	rBV	193	140	0.01%	0.001%
69	10.346	2796	2801	2807	rVB4	1218	1463	0.11%	0.014%
70	10.369	2807	2808	2812	rVB2	455	190	0.01%	0.002%
71	10.394	2812	2816	2817	rBV	400	275	0.02%	0.003%
72	10.485	2841	2844	2846	rBV	422	245	0.02%	0.002%
73	10.755	2915	2928	2952	rBV	583225	939445	69.52%	8.859%
74	10.857	2956	2960	2965	rVV3	552	497	0.04%	0.005%
75	11.115	3036	3040	3046	rVB2	1237	1127	0.08%	0.011%
76	11.266	3084	3087	3091	rVB	544	352	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
 Data File : VU051016.D
 Acq On : 30 Sep 2022 06:13
 Operator : JC/MD
 Sample : N4880-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGSJ4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	11.375	3119	3121	3125	rVB	361	243	0.02%	0.002%
78	11.629	3196	3200	3206	rBV2	497	538	0.04%	0.005%
79	11.687	3213	3218	3230	rVB5	4165	6142	0.45%	0.058%
80	11.745	3230	3236	3243	rBV6	1365	1914	0.14%	0.018%
81	11.809	3244	3256	3279	rBV	526776	828422	61.30%	7.812%
82	12.063	3327	3335	3341	rBV6	5345	8648	0.64%	0.082%
83	12.192	3362	3375	3397	rBV	609864	993888	73.55%	9.372%
84	12.890	3584	3592	3603	rVB5	9718	15184	1.12%	0.143%
85	13.002	3625	3627	3629	rBV	337	173	0.01%	0.002%
86	13.028	3629	3635	3638	rVV4	888	959	0.07%	0.009%
87	13.044	3638	3640	3644	rVV2	378	207	0.02%	0.002%
88	13.841	3882	3888	3898	rBV7	1815	2911	0.22%	0.027%
89	13.957	3921	3924	3928	rBV2	401	424	0.03%	0.004%
90	14.076	3958	3961	3963	rBV2	640	340	0.03%	0.003%
91	14.095	3963	3967	3977	rVB4	1151	1557	0.12%	0.015%
92	14.330	4037	4040	4047	rVB3	1242	1148	0.08%	0.011%
93	14.542	4103	4106	4109	rBV	550	370	0.03%	0.003%
94	14.600	4121	4124	4127	rVB2	670	417	0.03%	0.004%
95	14.632	4132	4134	4136	rBV3	530	304	0.02%	0.003%
96	14.809	4186	4189	4195	rVB	539	464	0.03%	0.004%
97	14.973	4238	4240	4244	rVB2	598	239	0.02%	0.002%
98	15.217	4314	4316	4320	rBV3	551	373	0.03%	0.004%
99	15.314	4344	4346	4348	rBV2	477	291	0.02%	0.003%
100	16.288	4647	4649	4654	rBV3	1033	792	0.06%	0.007%



Sum of corrected areas: 10604602

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
Data File : VU051016.D
Acq On : 30 Sep 2022 06:13
Operator : JC/MD
Sample : N4880-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGSJ4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

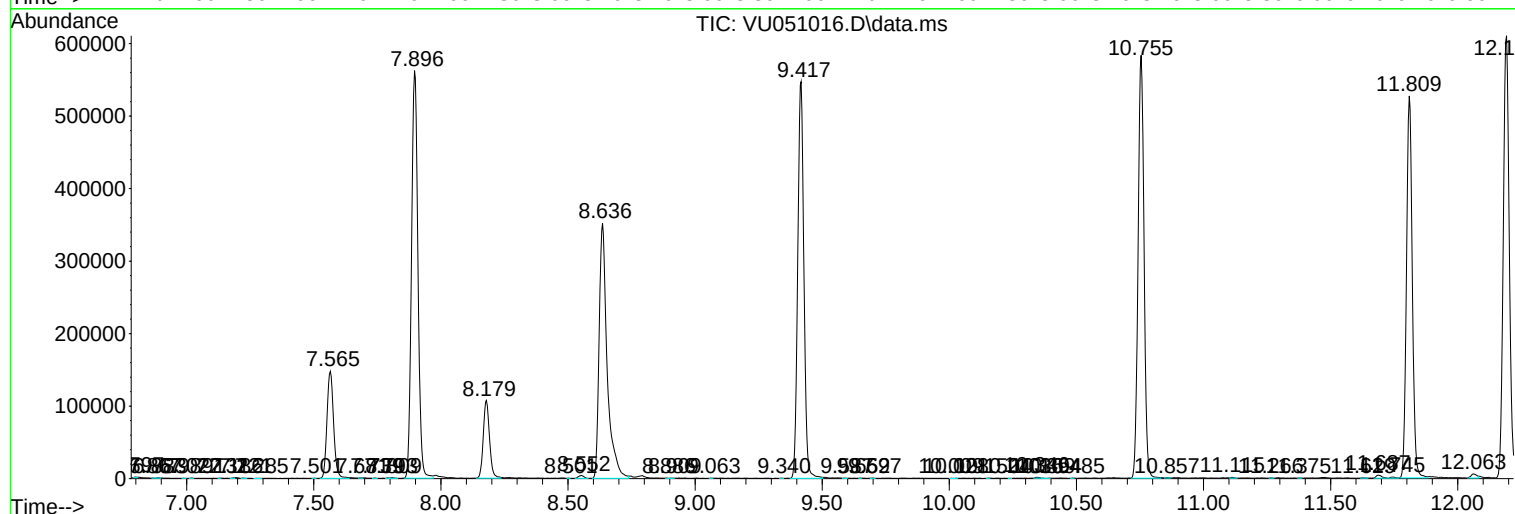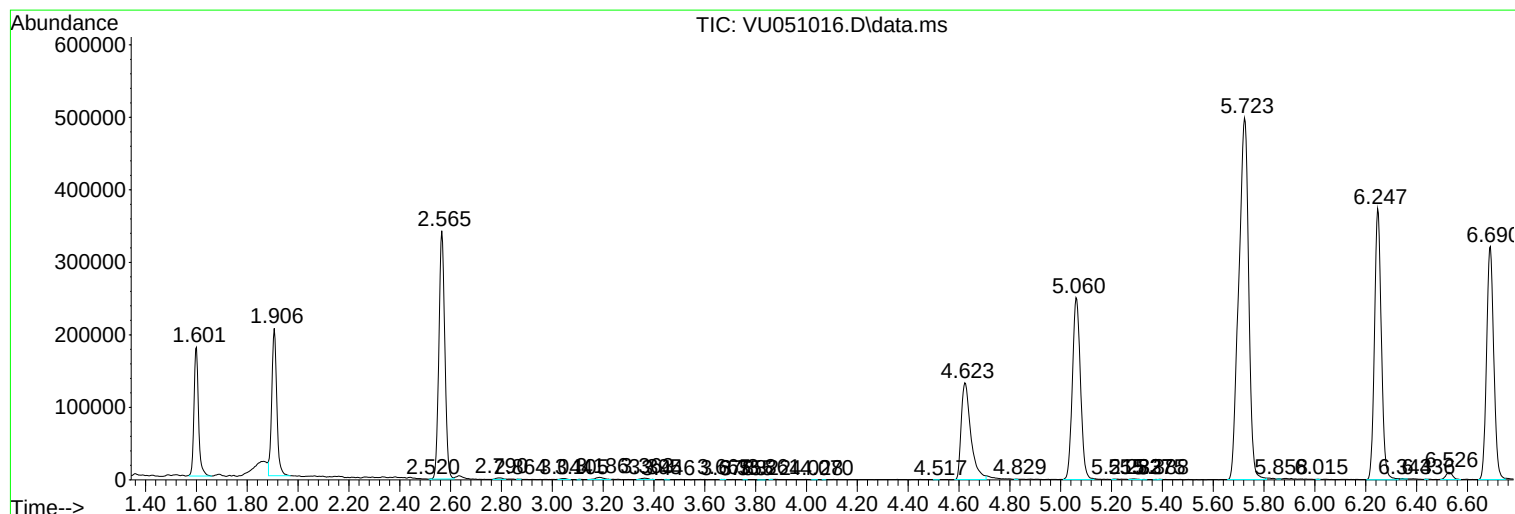

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
Data File : VU051016.D
Acq On : 30 Sep 2022 06:13
Operator : JC/MD
Sample : N4880-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGSJ4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
Data File : VU051016.D
Acq On : 30 Sep 2022 06:13
Operator : JC/MD
Sample : N4880-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGSJ4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc