

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
 Data File : VU051017.D
 Acq On : 30 Sep 2022 06:37
 Operator : JC/MD
 Sample : N4859-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E10017

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

Signal : TIC: VU051017.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	100	rVB	162906	199170	15.61%	2.007%
2	1.906	169	176	194	rVB	227427	303038	23.76%	3.054%
3	2.565	368	381	396	rBV	247611	402659	31.56%	4.058%
4	2.793	441	452	453	rBV3	1245	1806	0.14%	0.018%
5	2.980	506	510	513	rBV2	311	288	0.02%	0.003%
6	3.044	523	530	540	rVB6	2260	3650	0.29%	0.037%
7	3.179	558	572	575	rBV3	1535	2298	0.18%	0.023%
8	3.485	662	667	669	rBV	366	309	0.02%	0.003%
9	3.867	776	786	800	rVB3	1347	2898	0.23%	0.029%
10	3.954	809	813	818	rBV2	214	234	0.02%	0.002%
11	4.038	835	839	844	rBV2	206	240	0.02%	0.002%
12	4.202	886	890	896	rBV2	289	314	0.02%	0.003%
13	4.231	896	899	902	rVV2	325	227	0.02%	0.002%
14	4.346	927	935	938	rBV2	318	356	0.03%	0.004%
15	4.626	1005	1022	1049	rBV	128479	346353	27.15%	3.491%
16	4.990	1133	1135	1141	rVB2	291	245	0.02%	0.002%
17	5.060	1141	1157	1178	rBV	237035	519974	40.76%	5.241%
18	5.272	1218	1223	1224	rBV2	552	445	0.03%	0.004%
19	5.385	1252	1258	1265	rVB3	638	798	0.06%	0.008%
20	5.481	1285	1288	1290	rBV	307	249	0.02%	0.003%
21	5.552	1306	1310	1312	rBV	269	254	0.02%	0.003%
22	5.723	1340	1363	1391	rBV2	468409	1275673	100.00%	12.857%
23	5.964	1434	1438	1441	rBV3	473	310	0.02%	0.003%
24	6.025	1454	1457	1461	rBV2	626	711	0.06%	0.007%
25	6.115	1482	1485	1490	rVB2	513	313	0.02%	0.003%
26	6.247	1512	1526	1547	rBV	350740	664590	52.10%	6.698%
27	6.530	1604	1614	1626	rVV4	8179	14601	1.14%	0.147%
28	6.690	1650	1664	1683	rBV	310911	595874	46.71%	6.006%
29	6.790	1692	1695	1697	rBV2	720	510	0.04%	0.005%
30	7.022	1763	1767	1770	rBV2	280	250	0.02%	0.003%
31	7.192	1815	1820	1822	rBV3	821	704	0.06%	0.007%
32	7.565	1923	1936	1960	rBV	139115	246896	19.35%	2.488%
33	7.649	1960	1962	1964	rBV3	424	228	0.02%	0.002%
34	7.703	1976	1979	1984	rVB3	657	526	0.04%	0.005%
35	7.739	1984	1990	1996	rBV4	419	453	0.04%	0.005%
36	7.793	2004	2007	2009	rBV2	404	233	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
 Data File : VU051017.D
 Acq On : 30 Sep 2022 06:37
 Operator : JC/MD
 Sample : N4859-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E10017

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	7.896	2024	2039	2058	rBV	519513	887490	69.57%	8.945%
38	8.015	2074	2076	2086	rVB5	939	897	0.07%	0.009%
39	8.179	2115	2127	2147	rBV	101690	173309	13.59%	1.747%
40	8.369	2182	2186	2192	rVV3	491	537	0.04%	0.005%
41	8.398	2192	2195	2198	rVB2	394	251	0.02%	0.003%
42	8.459	2209	2214	2217	rBV2	566	492	0.04%	0.005%
43	8.475	2217	2219	2222	rVV2	639	438	0.03%	0.004%
44	8.552	2229	2243	2251	rVV6	2751	4110	0.32%	0.041%
45	8.636	2256	2269	2307	rBV2	350911	763093	59.82%	7.691%
46	8.903	2349	2352	2353	rBV2	565	289	0.02%	0.003%
47	8.935	2359	2362	2366	rVB3	449	346	0.03%	0.003%
48	9.002	2378	2383	2386	rVV2	310	306	0.02%	0.003%
49	9.157	2427	2431	2435	rBV2	235	275	0.02%	0.003%
50	9.337	2484	2487	2493	rBV2	287	225	0.02%	0.002%
51	9.369	2493	2497	2499	rBV	368	250	0.02%	0.003%
52	9.417	2499	2512	2536	rBV	509660	849764	66.61%	8.565%
53	9.568	2555	2559	2562	rVB2	688	549	0.04%	0.006%
54	9.610	2569	2572	2577	rVB3	237	222	0.02%	0.002%
55	9.690	2593	2597	2599	rBV3	441	309	0.02%	0.003%
56	10.099	2720	2724	2731	rVB3	768	848	0.07%	0.009%
57	10.192	2750	2753	2757	rBV2	275	272	0.02%	0.003%
58	10.488	2840	2845	2850	rVB4	1115	1161	0.09%	0.012%
59	10.655	2895	2897	2904	rVB2	445	363	0.03%	0.004%
60	10.755	2915	2928	2946	rBV	556086	899813	70.54%	9.069%
61	10.896	2969	2972	2975	rVB2	437	265	0.02%	0.003%
62	11.095	3031	3034	3036	rBV2	403	253	0.02%	0.003%
63	11.230	3072	3076	3078	rBV	313	271	0.02%	0.003%
64	11.285	3091	3093	3098	rBV3	353	263	0.02%	0.003%
65	11.359	3112	3116	3119	rBV2	289	255	0.02%	0.003%
66	11.472	3148	3151	3158	rBV2	648	587	0.05%	0.006%
67	11.520	3163	3166	3170	rBV	434	287	0.02%	0.003%
68	11.748	3233	3237	3240	rBV2	454	373	0.03%	0.004%
69	11.809	3242	3256	3272	rBV	469636	746992	58.56%	7.529%
70	12.066	3329	3336	3342	rBV5	2401	3669	0.29%	0.037%
71	12.115	3349	3351	3357	rVB2	700	545	0.04%	0.005%
72	12.144	3357	3360	3362	rBV	486	330	0.03%	0.003%
73	12.192	3362	3375	3402	rVV	541782	896561	70.28%	9.036%
74	12.311	3407	3412	3421	rVB3	5722	7994	0.63%	0.081%
75	12.613	3504	3506	3510	rVB3	505	390	0.03%	0.004%
76	12.681	3521	3527	3534	rBV4	1165	1351	0.11%	0.014%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
 Data File : VU051017.D
 Acq On : 30 Sep 2022 06:37
 Operator : JC/MD
 Sample : N4859-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E10017

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	12.893	3590	3593	3594	rBV2	485	289	0.02%	0.003%
78	12.922	3594	3602	3613	rVB2	18569	28259	2.22%	0.285%
79	13.025	3624	3634	3642	rBV5	5975	10106	0.79%	0.102%
80	13.073	3642	3649	3653	rVV4	2603	4515	0.35%	0.046%
81	13.108	3654	3660	3670	rVB3	6721	11498	0.90%	0.116%
82	13.311	3719	3723	3726	rBV2	382	416	0.03%	0.004%
83	13.356	3732	3737	3740	rBV3	289	296	0.02%	0.003%
84	13.378	3740	3744	3746	rBV2	286	244	0.02%	0.002%
85	13.452	3762	3767	3770	rBV4	601	477	0.04%	0.005%
86	13.484	3773	3777	3782	rBV3	494	549	0.04%	0.006%
87	13.517	3782	3787	3796	rBV3	2350	3283	0.26%	0.033%
88	13.626	3813	3821	3831	rVB6	3779	5625	0.44%	0.057%
89	13.787	3867	3871	3873	rBV2	634	452	0.04%	0.005%
90	13.838	3882	3887	3894	rBV3	1075	1185	0.09%	0.012%
91	14.060	3948	3956	3961	rBV3	5084	6724	0.53%	0.068%
92	14.240	4002	4012	4019	rBV4	3368	5642	0.44%	0.057%
93	14.320	4033	4037	4038	rBV3	470	337	0.03%	0.003%
94	14.336	4038	4042	4050	rVB6	1630	1921	0.15%	0.019%
95	14.391	4056	4059	4061	rBV3	527	259	0.02%	0.003%
96	14.549	4103	4108	4110	rBV4	631	584	0.05%	0.006%
97	14.684	4148	4150	4152	rBV	431	254	0.02%	0.003%
98	14.809	4185	4189	4196	rVB4	1433	1277	0.10%	0.013%
99	14.886	4206	4213	4220	rVB5	1876	2841	0.22%	0.029%
100	15.423	4377	4380	4385	rBV4	1195	1000	0.08%	0.010%




Sum of corrected areas: 9921705

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
Data File : VU051017.D
Acq On : 30 Sep 2022 06:37
Operator : JC/MD
Sample : N4859-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E10017

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

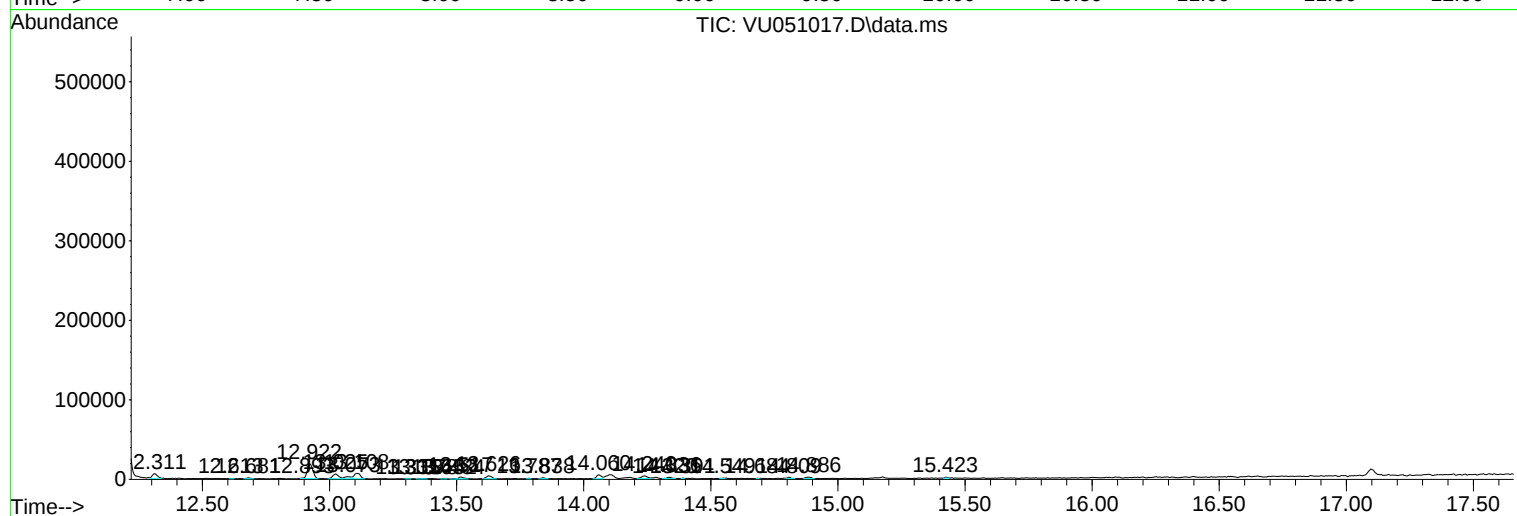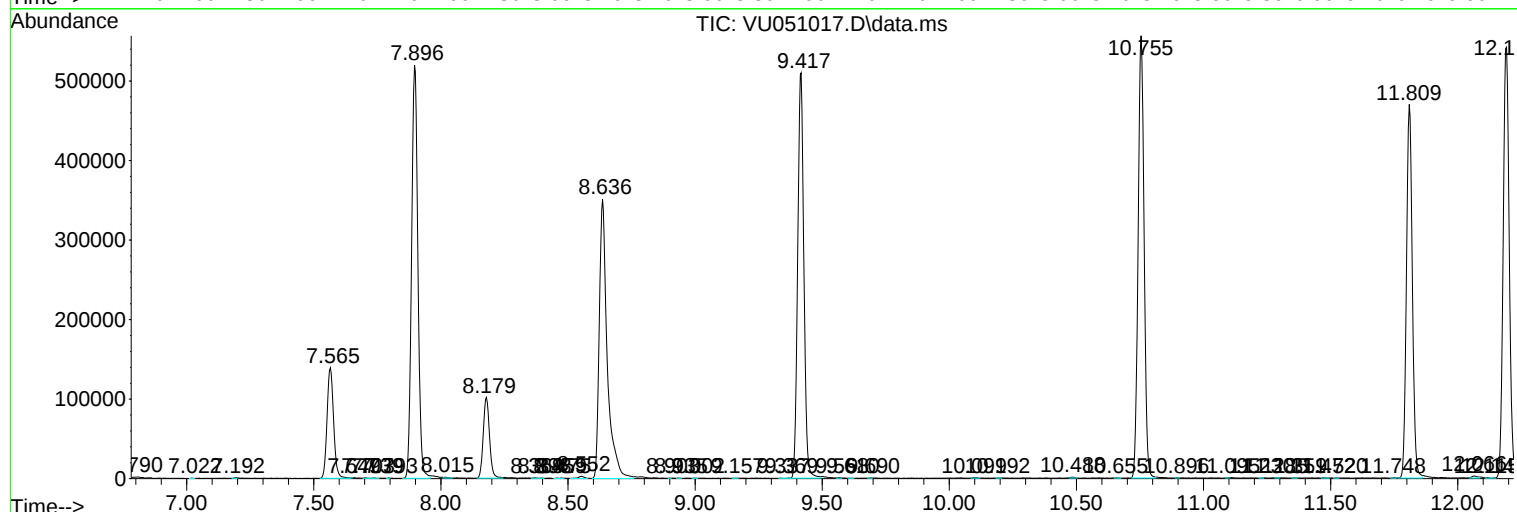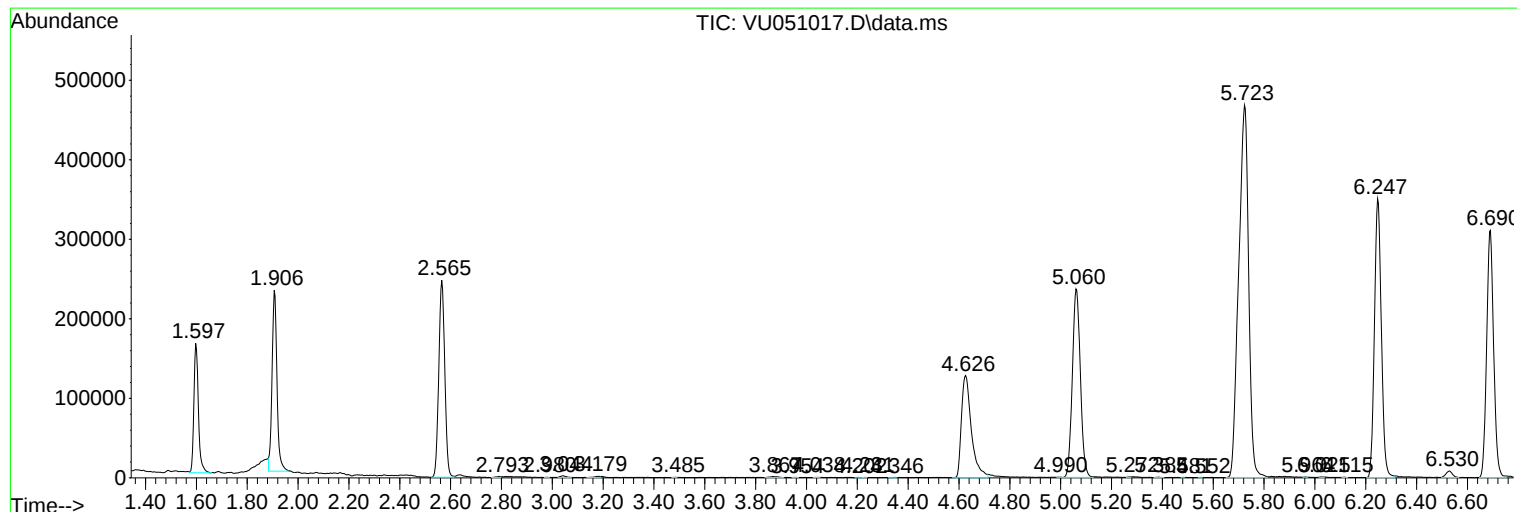

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
Data File : VU051017.D
Acq On : 30 Sep 2022 06:37
Operator : JC/MD
Sample : N4859-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E10017

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
Data File : VU051017.D
Acq On : 30 Sep 2022 06:37
Operator : JC/MD
Sample : N4859-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E10017

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------