

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
 Data File : VU051018.D
 Acq On : 30 Sep 2022 07:00
 Operator : JC/MD
 Sample : N4859-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E10018

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M

Title : VOC Analysis

Signal : TIC: VU051018.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	101	rBV	162780	199539	14.99%	1.994%
2	1.903	167	175	192	rVB	154936	209900	15.77%	2.097%
3	2.465	347	350	353	rBV3	353	238	0.02%	0.002%
4	2.507	361	363	367	rBV2	384	262	0.02%	0.003%
5	2.565	368	381	394	rBV	257342	415017	31.18%	4.147%
6	2.742	434	436	438	rBV	448	281	0.02%	0.003%
7	2.787	438	450	451	rBV6	2509	4050	0.30%	0.040%
8	2.871	474	476	480	rVB	475	259	0.02%	0.003%
9	2.893	480	483	489	rVB2	523	484	0.04%	0.005%
10	2.922	489	492	494	rBV3	512	267	0.02%	0.003%
11	2.973	503	508	513	rVB2	387	388	0.03%	0.004%
12	2.999	514	516	518	rBV	428	210	0.02%	0.002%
13	3.186	563	574	579	rBV4	1559	2841	0.21%	0.028%
14	3.379	629	634	636	rBV	265	229	0.02%	0.002%
15	3.465	657	661	664	rBV	257	209	0.02%	0.002%
16	3.597	695	702	707	rBV2	196	325	0.02%	0.003%
17	3.684	722	729	731	rBV	200	206	0.02%	0.002%
18	3.867	773	786	803	rVB4	1596	3612	0.27%	0.036%
19	4.514	981	987	990	rBV	253	258	0.02%	0.003%
20	4.620	1007	1020	1054	rBV	128192	327590	24.61%	3.273%
21	4.912	1109	1111	1114	rBV3	368	206	0.02%	0.002%
22	5.060	1141	1157	1182	rBV	243438	532871	40.04%	5.325%
23	5.215	1201	1205	1207	rBV3	517	346	0.03%	0.003%
24	5.288	1222	1228	1235	rVB2	1102	1650	0.12%	0.016%
25	5.443	1271	1276	1280	rBV	385	416	0.03%	0.004%
26	5.723	1341	1363	1399	rBV2	483419	1330917	100.00%	13.299%
27	5.906	1418	1420	1427	rVB4	846	824	0.06%	0.008%
28	5.948	1431	1433	1436	rVB3	506	281	0.02%	0.003%
29	5.970	1436	1440	1445	rVB3	528	376	0.03%	0.004%
30	6.102	1478	1481	1482	rBV2	327	199	0.01%	0.002%
31	6.157	1493	1498	1499	rBV2	348	252	0.02%	0.003%
32	6.247	1511	1526	1547	rBV	372157	702011	52.75%	7.015%
33	6.523	1603	1612	1627	rVB4	9071	18198	1.37%	0.182%
34	6.604	1631	1637	1640	rBV2	408	470	0.04%	0.005%
35	6.629	1640	1645	1648	rBV3	436	281	0.02%	0.003%
36	6.687	1650	1663	1687	rBV	311933	607744	45.66%	6.073%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
 Data File : VU051018.D
 Acq On : 30 Sep 2022 07:00
 Operator : JC/MD
 Sample : N4859-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E10018

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	6.967	1748	1750	1755	rVV2	183	199	0.01%	0.002%
38	7.005	1759	1762	1768	rVV2	240	214	0.02%	0.002%
39	7.105	1785	1793	1800	rBV3	506	729	0.05%	0.007%
40	7.189	1808	1819	1823	rBV5	765	1330	0.10%	0.013%
41	7.401	1881	1885	1891	rVB2	316	372	0.03%	0.004%
42	7.468	1901	1906	1912	rVB2	195	203	0.02%	0.002%
43	7.565	1921	1936	1955	rBV	146985	257757	19.37%	2.576%
44	7.790	2003	2006	2014	rVB3	406	359	0.03%	0.004%
45	7.845	2018	2023	2026	rBV	224	199	0.01%	0.002%
46	7.896	2026	2039	2063	rBV	555831	951911	71.52%	9.512%
47	8.179	2115	2127	2150	rBV2	106269	179097	13.46%	1.790%
48	8.311	2165	2168	2174	rBV3	662	565	0.04%	0.006%
49	8.346	2177	2179	2189	rVB3	499	586	0.04%	0.006%
50	8.452	2206	2212	2214	rBV2	371	433	0.03%	0.004%
51	8.552	2235	2243	2251	rVB4	3011	4573	0.34%	0.046%
52	8.632	2256	2268	2302	rBV3	335702	722755	54.31%	7.222%
53	8.851	2333	2336	2339	rBV3	385	287	0.02%	0.003%
54	8.867	2339	2341	2347	rVB3	342	291	0.02%	0.003%
55	8.915	2352	2356	2358	rBV	373	258	0.02%	0.003%
56	8.967	2369	2372	2375	rBV2	449	305	0.02%	0.003%
57	9.150	2425	2429	2435	rVB	404	383	0.03%	0.004%
58	9.240	2455	2457	2460	rBV	262	222	0.02%	0.002%
59	9.320	2479	2482	2488	rVB2	275	299	0.02%	0.003%
60	9.353	2489	2492	2496	rVB2	270	216	0.02%	0.002%
61	9.417	2498	2512	2533	rBV	542519	895354	67.27%	8.947%
62	9.562	2554	2557	2560	rBV3	404	327	0.02%	0.003%
63	9.693	2590	2598	2606	rBV4	1347	2028	0.15%	0.020%
64	9.761	2615	2619	2627	rVB2	204	298	0.02%	0.003%
65	9.845	2639	2645	2646	rBV	273	276	0.02%	0.003%
66	9.996	2689	2692	2694	rBV2	349	221	0.02%	0.002%
67	10.108	2721	2727	2731	rVB4	1115	1141	0.09%	0.011%
68	10.182	2744	2750	2753	rBV	293	287	0.02%	0.003%
69	10.382	2809	2812	2816	rVB	324	254	0.02%	0.003%
70	10.417	2820	2823	2826	rBV	320	211	0.02%	0.002%
71	10.755	2915	2928	2952	rBV	552651	888150	66.73%	8.875%
72	10.915	2976	2978	2983	rVB2	544	391	0.03%	0.004%
73	11.050	3015	3020	3025	rBV2	291	343	0.03%	0.003%
74	11.121	3038	3042	3047	rBV	533	331	0.02%	0.003%
75	11.176	3055	3059	3062	rVB2	384	305	0.02%	0.003%
76	11.378	3118	3122	3125	rBV2	418	384	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
 Data File : VU051018.D
 Acq On : 30 Sep 2022 07:00
 Operator : JC/MD
 Sample : N4859-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E10018

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	11.394	3125	3127	3132	rVB2	290	224	0.02%	0.002%
78	11.664	3208	3211	3214	rVB2	410	303	0.02%	0.003%
79	11.738	3226	3234	3237	rBV4	694	869	0.07%	0.009%
80	11.809	3243	3256	3280	rBV	486566	777221	58.40%	7.767%
81	11.947	3297	3299	3303	rVB2	567	319	0.02%	0.003%
82	12.070	3330	3337	3339	rBV5	1430	1580	0.12%	0.016%
83	12.192	3361	3375	3398	rBV	575917	943964	70.93%	9.433%
84	12.652	3515	3518	3520	rBV2	362	225	0.02%	0.002%
85	12.706	3532	3535	3538	rBV2	315	221	0.02%	0.002%
86	12.857	3579	3582	3586	rBV3	417	328	0.02%	0.003%
87	12.880	3586	3589	3590	rVV	405	222	0.02%	0.002%
88	12.896	3592	3594	3597	rVB2	638	360	0.03%	0.004%
89	13.002	3624	3627	3630	rVV3	407	297	0.02%	0.003%
90	13.073	3646	3649	3651	rBV	545	304	0.02%	0.003%
91	13.224	3693	3696	3699	rVB4	559	387	0.03%	0.004%
92	13.433	3758	3761	3763	rVB2	445	227	0.02%	0.002%
93	13.462	3767	3770	3774	rBV2	545	538	0.04%	0.005%
94	13.497	3779	3781	3784	rBV2	780	544	0.04%	0.005%
95	13.584	3805	3808	3814	rVB2	623	631	0.05%	0.006%
96	13.947	3919	3921	3926	rVB	585	358	0.03%	0.004%
97	14.037	3947	3949	3953	rBV2	462	275	0.02%	0.003%
98	14.243	4011	4013	4017	rVB2	658	339	0.03%	0.003%
99	14.439	4071	4074	4075	rBV	411	228	0.02%	0.002%
100	14.661	4141	4143	4145	rBV	581	333	0.03%	0.003%




Sum of corrected areas: 10007348

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
Data File : VU051018.D
Acq On : 30 Sep 2022 07:00
Operator : JC/MD
Sample : N4859-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E10018

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

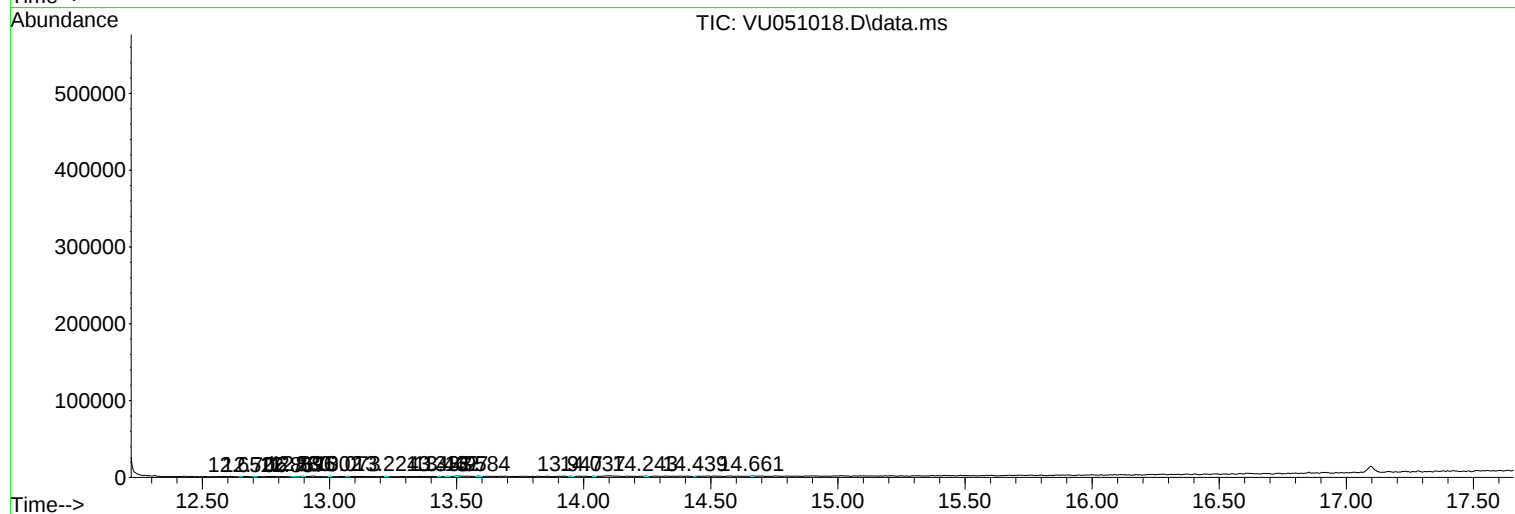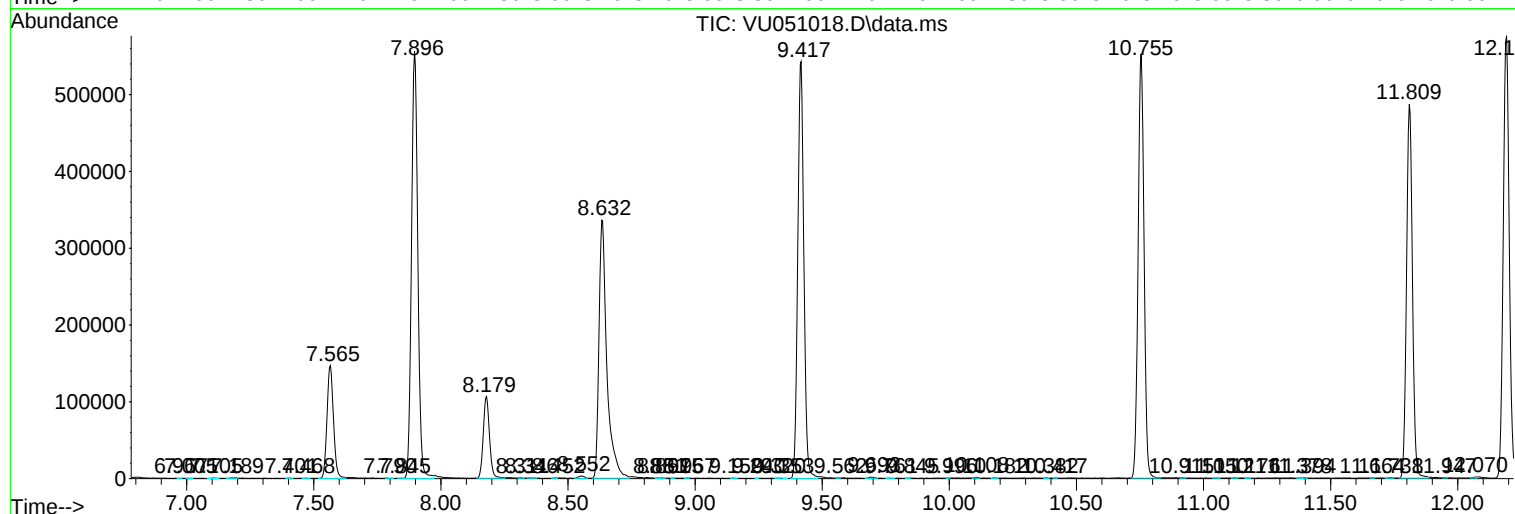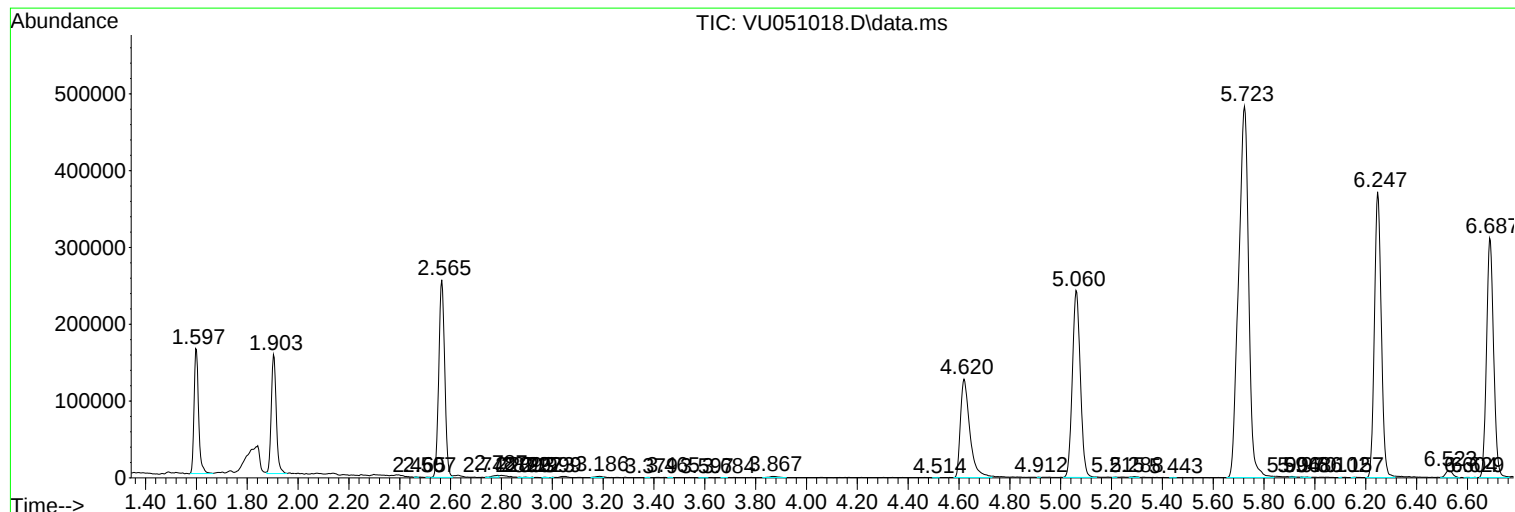

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
Data File : VU051018.D
Acq On : 30 Sep 2022 07:00
Operator : JC/MD
Sample : N4859-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E10018

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
Data File : VU051018.D
Acq On : 30 Sep 2022 07:00
Operator : JC/MD
Sample : N4859-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E10018

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------