

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
 Data File : VU051023.D
 Acq On : 30 Sep 2022 08:57
 Operator : JC/MD
 Sample : N4859-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E10051

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M

Title : VOC Analysis

Signal : TIC: VU051023.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	98	rVB	169764	206060	14.78%	2.032%
2	1.906	169	176	189	rVB	179825	240202	17.23%	2.369%
3	2.565	367	381	396	rBV	266901	434776	31.19%	4.287%
4	2.629	397	401	414	rVV4	3031	5325	0.38%	0.053%
5	2.681	414	417	420	rVB4	772	509	0.04%	0.005%
6	2.787	441	450	451	rBV5	1102	1207	0.09%	0.012%
7	2.944	494	499	508	rVB2	580	689	0.05%	0.007%
8	3.041	521	529	543	rVB6	1730	3235	0.23%	0.032%
9	3.173	563	570	571	rBV3	1156	1156	0.08%	0.011%
10	3.234	586	589	595	rVB3	272	252	0.02%	0.002%
11	3.324	610	617	621	rBV2	419	514	0.04%	0.005%
12	3.523	675	679	683	rVB2	269	244	0.02%	0.002%
13	3.542	683	685	688	rBV2	491	286	0.02%	0.003%
14	3.655	718	720	724	rVB	332	240	0.02%	0.002%
15	3.681	724	728	732	rBV	247	254	0.02%	0.003%
16	3.761	750	753	755	rBV	353	228	0.02%	0.002%
17	3.858	780	783	790	rVB2	287	243	0.02%	0.002%
18	3.944	806	810	816	rVB2	321	298	0.02%	0.003%
19	3.980	816	821	826	rBV2	418	523	0.04%	0.005%
20	4.054	841	844	849	rBV2	248	235	0.02%	0.002%
21	4.124	863	866	871	rVB2	258	221	0.02%	0.002%
22	4.385	940	947	951	rVV2	330	439	0.03%	0.004%
23	4.423	956	959	964	rVB2	309	295	0.02%	0.003%
24	4.497	979	982	985	rBV2	259	207	0.01%	0.002%
25	4.623	1007	1021	1048	rBV	132199	346916	24.89%	3.421%
26	4.890	1100	1104	1109	rVB2	479	446	0.03%	0.004%
27	5.060	1140	1157	1180	rBV	257761	567064	40.68%	5.592%
28	5.272	1221	1223	1226	rBV3	305	225	0.02%	0.002%
29	5.292	1226	1229	1231	rBV3	584	466	0.03%	0.005%
30	5.349	1243	1247	1251	rBV3	361	275	0.02%	0.003%
31	5.369	1251	1253	1260	rVB4	438	382	0.03%	0.004%
32	5.440	1272	1275	1282	rBV2	340	426	0.03%	0.004%
33	5.722	1341	1363	1396	rBV3	509908	1393948	100.00%	13.746%
34	5.899	1416	1418	1420	rBV3	428	217	0.02%	0.002%
35	6.038	1457	1461	1468	rVB4	410	478	0.03%	0.005%
36	6.112	1480	1484	1489	rBV2	363	406	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
 Data File : VU051023.D
 Acq On : 30 Sep 2022 08:57
 Operator : JC/MD
 Sample : N4859-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E10051

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	6.147	1492	1495	1499	rVB3	279	233	0.02%	0.002%
38	6.247	1512	1526	1545	rBV	399475	740008	53.09%	7.297%
39	6.468	1593	1595	1600	rVB3	424	300	0.02%	0.003%
40	6.526	1603	1613	1626	rVB4	10003	19953	1.43%	0.197%
41	6.603	1626	1637	1641	rBV2	390	503	0.04%	0.005%
42	6.690	1649	1664	1685	rBV	331552	644696	46.25%	6.357%
43	6.944	1740	1743	1748	rVB2	534	395	0.03%	0.004%
44	6.976	1748	1753	1758	rBV2	394	571	0.04%	0.006%
45	7.192	1809	1820	1827	rBV3	983	1846	0.13%	0.018%
46	7.247	1834	1837	1841	rBV2	237	225	0.02%	0.002%
47	7.353	1866	1870	1875	rVB2	210	237	0.02%	0.002%
48	7.391	1875	1882	1883	rBV	232	236	0.02%	0.002%
49	7.565	1923	1936	1952	rBV	153280	270134	19.38%	2.664%
50	7.751	1989	1994	1997	rBV2	194	215	0.02%	0.002%
51	7.896	2025	2039	2060	rBV	578292	1002621	71.93%	9.887%
52	8.179	2114	2127	2144	rBV2	107293	185789	13.33%	1.832%
53	8.401	2192	2196	2200	rBV3	410	429	0.03%	0.004%
54	8.462	2210	2215	2220	rBV4	533	645	0.05%	0.006%
55	8.555	2237	2244	2248	rBV3	1522	1918	0.14%	0.019%
56	8.636	2255	2269	2304	rBV3	349703	767027	55.03%	7.564%
57	8.822	2325	2327	2333	rVB	543	311	0.02%	0.003%
58	8.886	2343	2347	2350	rBV2	429	327	0.02%	0.003%
59	8.915	2353	2356	2363	rVB2	358	312	0.02%	0.003%
60	9.050	2394	2398	2402	rVB2	294	207	0.01%	0.002%
61	9.214	2446	2449	2453	rBV2	410	352	0.03%	0.003%
62	9.346	2485	2490	2496	rVB2	320	435	0.03%	0.004%
63	9.414	2496	2511	2539	rBV	558033	930228	66.73%	9.173%
64	9.562	2552	2557	2561	rBV2	587	499	0.04%	0.005%
65	9.851	2644	2647	2651	rBV	379	303	0.02%	0.003%
66	10.169	2742	2746	2750	rBV2	234	231	0.02%	0.002%
67	10.307	2785	2789	2792	rBV2	394	314	0.02%	0.003%
68	10.398	2814	2817	2820	rVB2	321	211	0.02%	0.002%
69	10.439	2820	2830	2833	rBV	293	449	0.03%	0.004%
70	10.635	2885	2891	2894	rBV2	362	333	0.02%	0.003%
71	10.754	2915	2928	2947	rBV	465759	751389	53.90%	7.410%
72	10.880	2964	2967	2971	rBV2	371	341	0.02%	0.003%
73	10.902	2972	2974	2978	rVB	558	326	0.02%	0.003%
74	11.050	3015	3020	3023	rBV2	305	243	0.02%	0.002%
75	11.082	3027	3030	3038	rVB2	313	338	0.02%	0.003%
76	11.275	3084	3090	3098	rVB2	298	549	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
 Data File : VU051023.D
 Acq On : 30 Sep 2022 08:57
 Operator : JC/MD
 Sample : N4859-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E10051

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	11.320	3098	3104	3110	rBV2	350	441	0.03%	0.004%
78	11.504	3159	3161	3166	rVB2	401	271	0.02%	0.003%
79	11.590	3185	3188	3196	rVB3	289	358	0.03%	0.004%
80	11.684	3207	3217	3220	rBV2	341	507	0.04%	0.005%
81	11.725	3226	3230	3233	rBV2	259	206	0.01%	0.002%
82	11.809	3243	3256	3280	rBV	408050	662643	47.54%	6.534%
83	12.008	3314	3318	3319	rBV	424	292	0.02%	0.003%
84	12.053	3328	3332	3335	rBV3	382	294	0.02%	0.003%
85	12.079	3335	3340	3346	rBV4	908	1069	0.08%	0.011%
86	12.131	3353	3356	3361	rVB2	258	221	0.02%	0.002%
87	12.192	3361	3375	3396	rBV	577446	924485	66.32%	9.116%
88	12.632	3509	3512	3517	rBV2	407	418	0.03%	0.004%
89	13.401	3749	3751	3754	rVB	453	247	0.02%	0.002%
90	13.478	3772	3775	3777	rBV2	451	378	0.03%	0.004%
91	14.066	3955	3958	3961	rBV3	616	454	0.03%	0.004%
92	15.018	4251	4254	4256	rVB2	471	254	0.02%	0.003%
93	15.108	4274	4282	4284	rBV2	585	834	0.06%	0.008%
94	15.153	4294	4296	4300	rBV3	451	379	0.03%	0.004%
95	15.346	4353	4356	4357	rBV	513	294	0.02%	0.003%
96	15.491	4398	4401	4402	rBV2	443	258	0.02%	0.003%
97	15.822	4499	4504	4507	rBV4	715	788	0.06%	0.008%
98	16.056	4576	4577	4580	rBV2	605	310	0.02%	0.003%
99	16.163	4608	4610	4612	rBV4	868	456	0.03%	0.004%
100	17.098	4894	4901	4909	rVB5	6662	10407	0.75%	0.103%




Sum of corrected areas: 10140830

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
Data File : VU051023.D
Acq On : 30 Sep 2022 08:57
Operator : JC/MD
Sample : N4859-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E10051

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

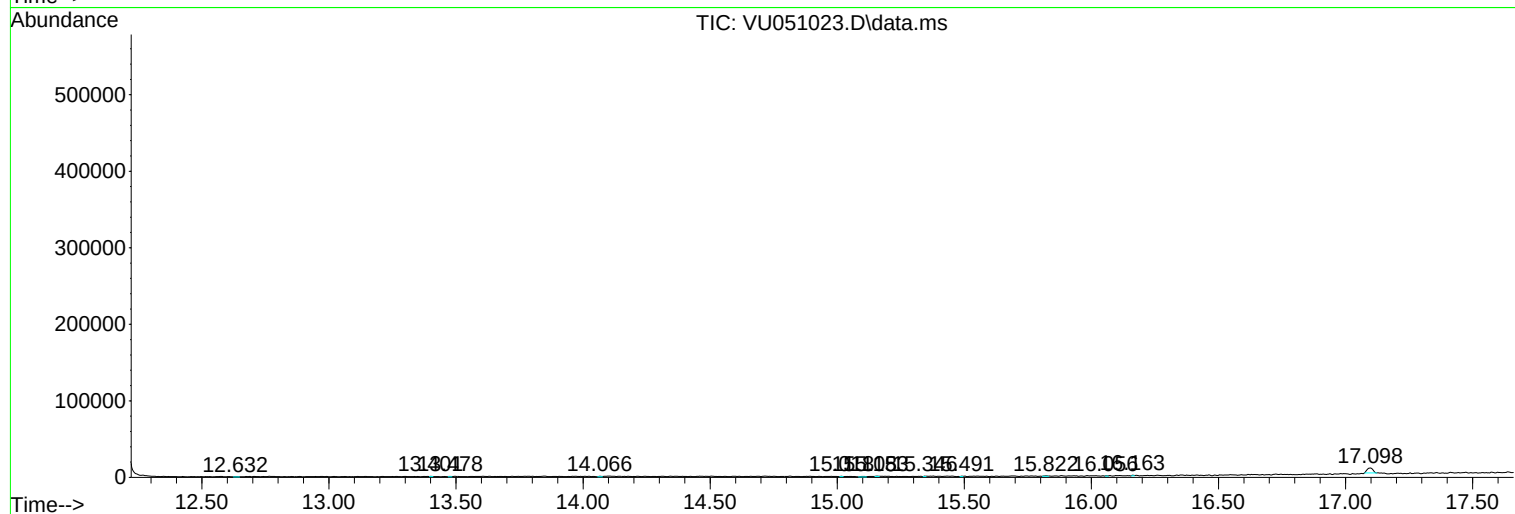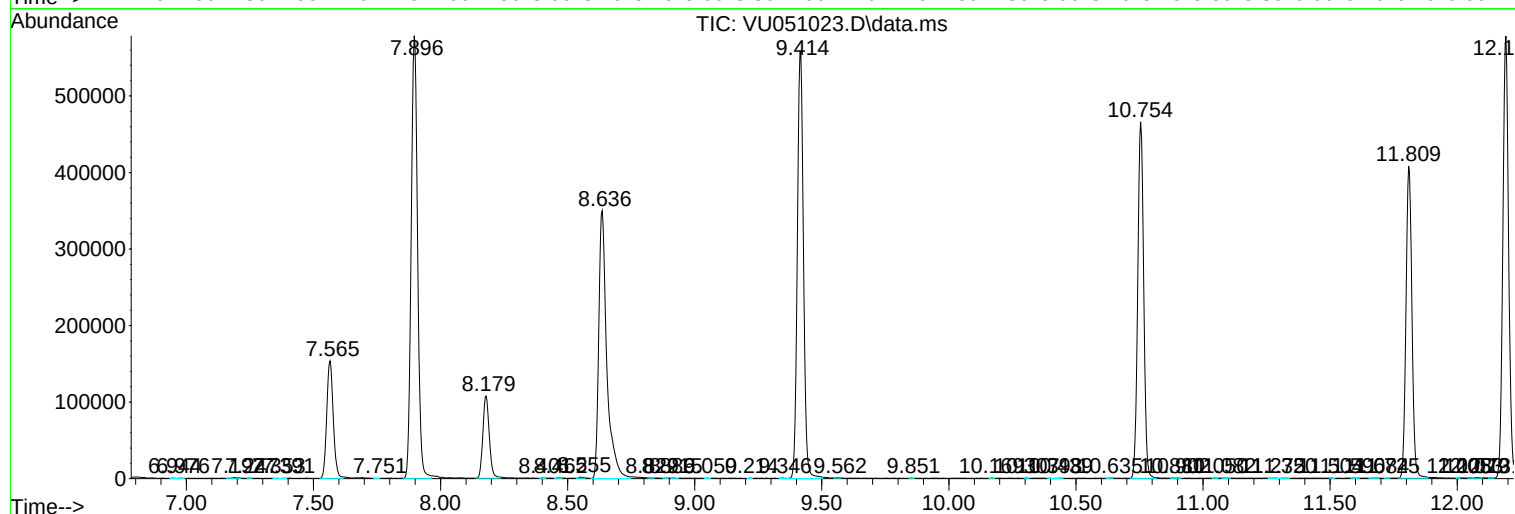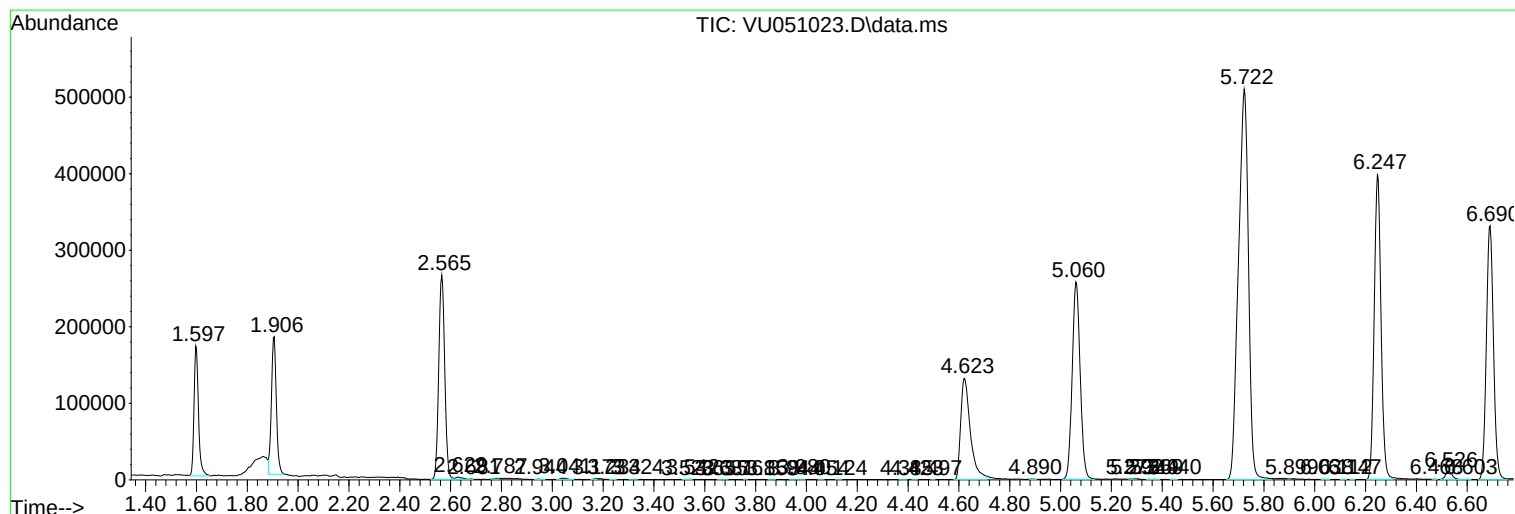

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
Data File : VU051023.D
Acq On : 30 Sep 2022 08:57
Operator : JC/MD
Sample : N4859-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E10051

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
Data File : VU051023.D
Acq On : 30 Sep 2022 08:57
Operator : JC/MD
Sample : N4859-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E10051

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------