


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU092922\
 Data File : VU050977.D
 Acq On : 29 Sep 2022 13:58
 Operator : JC/MD
 Sample : BFB133
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB133

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis
 Last Update : Sat Oct 01 03:04:59 2022

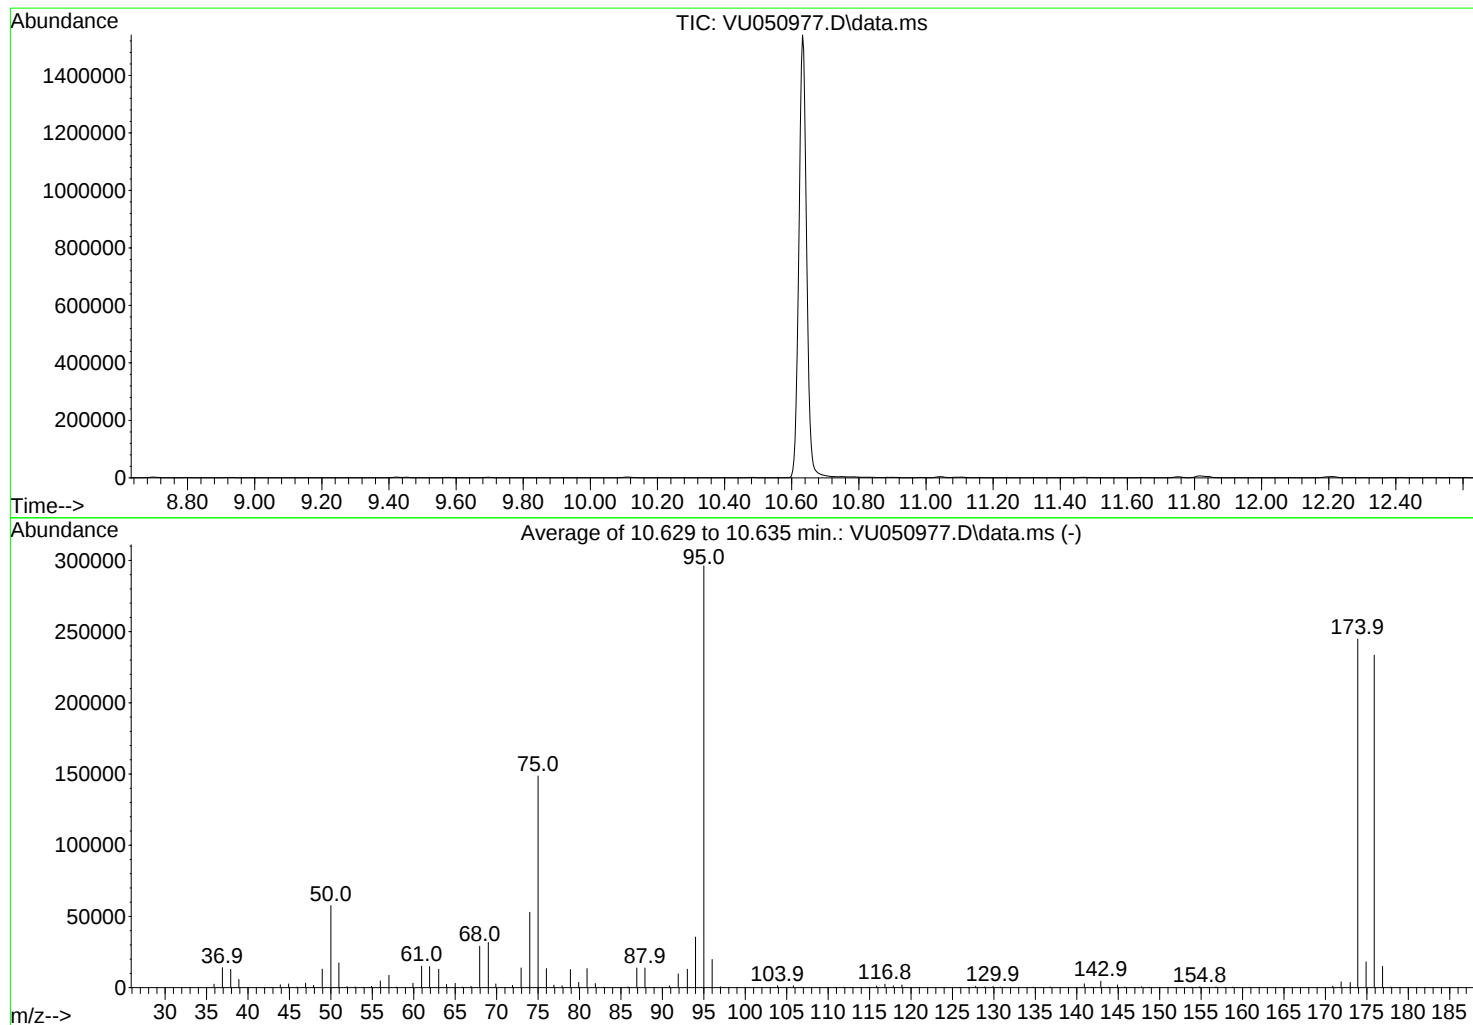

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.5	57645	PASS
75	95	30	80	50.2	148629	PASS
95	95	100	100	100.0	296256	PASS
96	95	5	9	6.7	19731	PASS
173	174	0.00	2	1.5	3553	PASS
174	95	50	120	82.7	244885	PASS
175	174	5	9	7.4	18099	PASS
176	174	95	101	95.4	233515	PASS
177	176	5	9	6.4	14955	PASS

m/z	Abundance
39.90	197.0
43.90	431.0

Instrument :
MSVOA_U
ClientSampleId :
BFB133

m/z	Abundance
35.90	2567.0
36.90	13681.0
37.90	12765.0
38.90	5558.0
40.10	287.0
41.00	154.0
41.90	107.0
42.80	266.0
43.90	2353.0
44.90	2532.0
45.90	379.0
46.90	3157.0
47.90	1453.0
48.90	13153.0
50.00	56760.0
51.00	16824.0
51.90	863.0
52.90	550.0
53.90	219.0
54.90	889.0
55.90	4687.0
57.00	8585.0
57.90	483.0
59.90	3082.0
60.90	14756.0
61.90	14833.0
63.00	12968.0
64.00	2314.0
65.00	3143.0
65.90	472.0
66.90	789.0
67.90	28224.0
69.00	30392.0
69.90	2560.0
71.90	1577.0
72.90	13272.0
74.00	52016.0
75.00	145408.0
76.00	13338.0
76.90	1713.0
77.90	1358.0
78.90	12643.0
79.90	3730.0
80.90	13195.0
81.90	2946.0
82.90	298.0
85.80	596.0
86.90	13326.0
87.90	13122.0
90.80	1174.0
91.90	9631.0
93.00	12529.0
94.00	35056.0
95.00	286656.0
96.00	19320.0
97.00	532.0
103.10	131.0
103.90	1181.0
105.00	332.0
105.80	1189.0
106.70	259.0
108.00	211.0
109.80	106.0
110.90	215.0
111.90	196.0
112.80	197.0
114.70	267.0
115.90	1034.0
116.80	2598.0
117.80	1238.0
118.90	1885.0
123.80	199.0
126.90	103.0
127.80	972.0
128.90	519.0
129.90	1017.0
130.80	462.0
134.80	465.0
135.70	166.0
136.80	589.0
139.80	134.0
140.90	2541.0
141.80	337.0
142.90	4594.0
143.80	331.0
144.90	2146.0
145.80	566.0
146.90	118.0
147.80	629.0
148.80	175.0
150.00	261.0
151.70	134.0

Instrument :
MSVOA_U
ClientSampleId :
BFB133

152.70	167.0
153.80	232.0
154.90	560.0
155.80	147.0
156.80	584.0
157.80	179.0
158.80	385.0
160.90	271.0
170.90	1064.0
171.90	3997.0
173.00	3354.0
173.90	231488.0
174.90	17704.0
175.90	220736.0
176.90	14533.0
177.90	425.0

Instrument :
MSVOA_U
ClientSampleId :
BFB133

m/z	Abundance
35.90	2583.0
36.90	14527.0
37.90	13290.0
38.90	5894.0
40.10	388.0
41.10	121.0
42.90	289.0
43.90	2594.0
44.90	2686.0
45.90	405.0
47.00	3244.0
47.90	1679.0
48.90	13529.0
50.00	59984.0
50.90	18040.0
51.90	838.0
52.90	521.0
53.90	326.0
54.90	897.0
56.00	4965.0
57.00	8995.0
57.90	441.0
59.90	3342.0
60.90	15520.0
61.90	15286.0
63.00	13401.0
64.00	2286.0
65.00	3195.0
65.90	422.0
66.90	909.0
68.00	30064.0
69.00	32768.0
69.90	2694.0
71.90	1635.0
73.00	14240.0
74.00	54736.0
75.00	153536.0
76.00	13884.0
76.90	1887.0
77.90	1423.0
78.90	13124.0
79.90	3943.0
80.90	13737.0
81.90	3041.0
82.90	355.0
85.90	591.0
86.90	14297.0
87.90	14512.0
90.80	1314.0
91.90	10076.0
93.00	13506.0
94.00	36832.0
95.00	306240.0
96.00	20360.0
97.00	569.0
103.00	139.0
103.90	1414.0
104.90	349.0
105.80	1330.0
106.80	348.0
108.00	247.0
109.90	172.0
110.90	261.0
111.80	220.0
112.70	189.0
114.80	298.0
115.80	1143.0
116.80	2528.0
117.80	1310.0
118.90	1950.0
122.80	101.0
123.80	195.0
125.80	125.0
127.80	1089.0
128.90	591.0
129.90	1096.0
130.80	446.0
134.70	529.0
135.80	122.0
136.80	601.0
139.90	155.0
140.90	2829.0
141.80	346.0
142.90	4553.0
143.90	359.0
144.90	1981.0
145.80	616.0
146.90	179.0
147.80	686.0
148.80	214.0
149.90	303.0
151.80	183.0

Instrument :
MSVOA_U
ClientSampleId :
BFB133

152.70	207.0
153.80	238.0
154.90	659.0
155.80	196.0
156.80	606.0
157.90	204.0
158.80	440.0
160.90	340.0
170.90	997.0
171.90	4237.0
173.00	3735.0
173.90	253312.0
174.90	18720.0
175.90	241536.0
176.90	15409.0
177.90	434.0

Instrument :
MSVOA_U
ClientSampleId :
BFB133

m/z	Abundance
35.90	2445.0
36.90	13930.0
37.90	12409.0
38.90	5766.0
40.00	448.0
42.90	259.0
43.90	2591.0
44.90	2512.0
45.90	464.0
47.00	3089.0
47.90	1810.0
49.00	12542.0
50.00	56192.0
51.00	17504.0
52.00	772.0
52.90	485.0
53.90	345.0
54.90	835.0
56.00	4686.0
57.00	8488.0
57.90	391.0
59.90	3063.0
61.00	15053.0
61.90	14386.0
63.00	12374.0
63.90	2067.0
65.00	2811.0
65.90	321.0
66.90	933.0
68.00	28952.0
69.00	31816.0
69.90	2546.0
71.90	1584.0
73.00	14085.0
74.00	52200.0
75.00	146944.0
76.00	12959.0
76.90	1961.0
77.90	1244.0
78.90	12241.0
79.90	3596.0
80.90	13112.0
81.90	2915.0
82.90	359.0
85.90	578.0
86.90	14034.0
87.90	14027.0
90.90	1277.0
91.90	9456.0
93.00	12720.0
94.00	34776.0
95.00	295872.0
96.00	19512.0
97.00	562.0
103.00	104.0
103.90	1493.0
104.90	334.0
105.80	1263.0
106.80	416.0
108.00	204.0
109.90	198.0
110.90	244.0
111.80	221.0
112.70	206.0
114.80	286.0
115.80	1089.0
116.90	2279.0
117.90	1235.0
118.90	1899.0
122.80	105.0
123.80	176.0
125.80	146.0
127.80	1013.0
128.90	582.0
129.90	1000.0
130.80	377.0
134.70	498.0
136.80	537.0
139.90	175.0
140.90	2865.0
141.80	338.0
142.90	4198.0
143.90	385.0
144.90	1610.0
145.80	540.0
146.90	201.0
147.80	614.0
148.80	204.0
149.90	304.0
151.80	201.0
152.70	209.0
153.80	250.0

Instrument :
MSVOA_U
ClientSampleId :
BFB133

154.80	743.0
155.80	209.0
156.80	629.0
157.90	197.0
158.80	424.0
160.90	385.0
170.90	826.0
171.90	4085.0
173.00	3570.0
173.90	249856.0
174.90	17872.0
175.90	238272.0
176.90	14924.0
177.90	405.0

Instrument :
MSVOA_U
ClientSampleId :
BFB133