

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100422\
 Data File : VU051108.D
 Acq On : 04 Oct 2022 15:17
 Operator : JC/MD
 Sample : VU1004WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU1004WBL01

Quant Time: Oct 05 02:48:06 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U100422DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Wed Oct 05 02:45:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.115	96	52308	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.636	95	12888	0.750	ug/l	0.00
Spiked Amount 1.000			Recovery	=	75.000%	
68) 1,2-Dichlorobenzene-d4	12.195	152	14634	0.766	ug/l	0.00
Spiked Amount 1.000			Recovery	=	77.000%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100422\
Data File : VU051108.D
Acq On : 04 Oct 2022 15:17
Operator : JC/MD
Sample : VU1004WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU1004WBL01

Quant Time: Oct 05 02:48:06 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U100422DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Wed Oct 05 02:45:21 2022
Response via : Initial Calibration




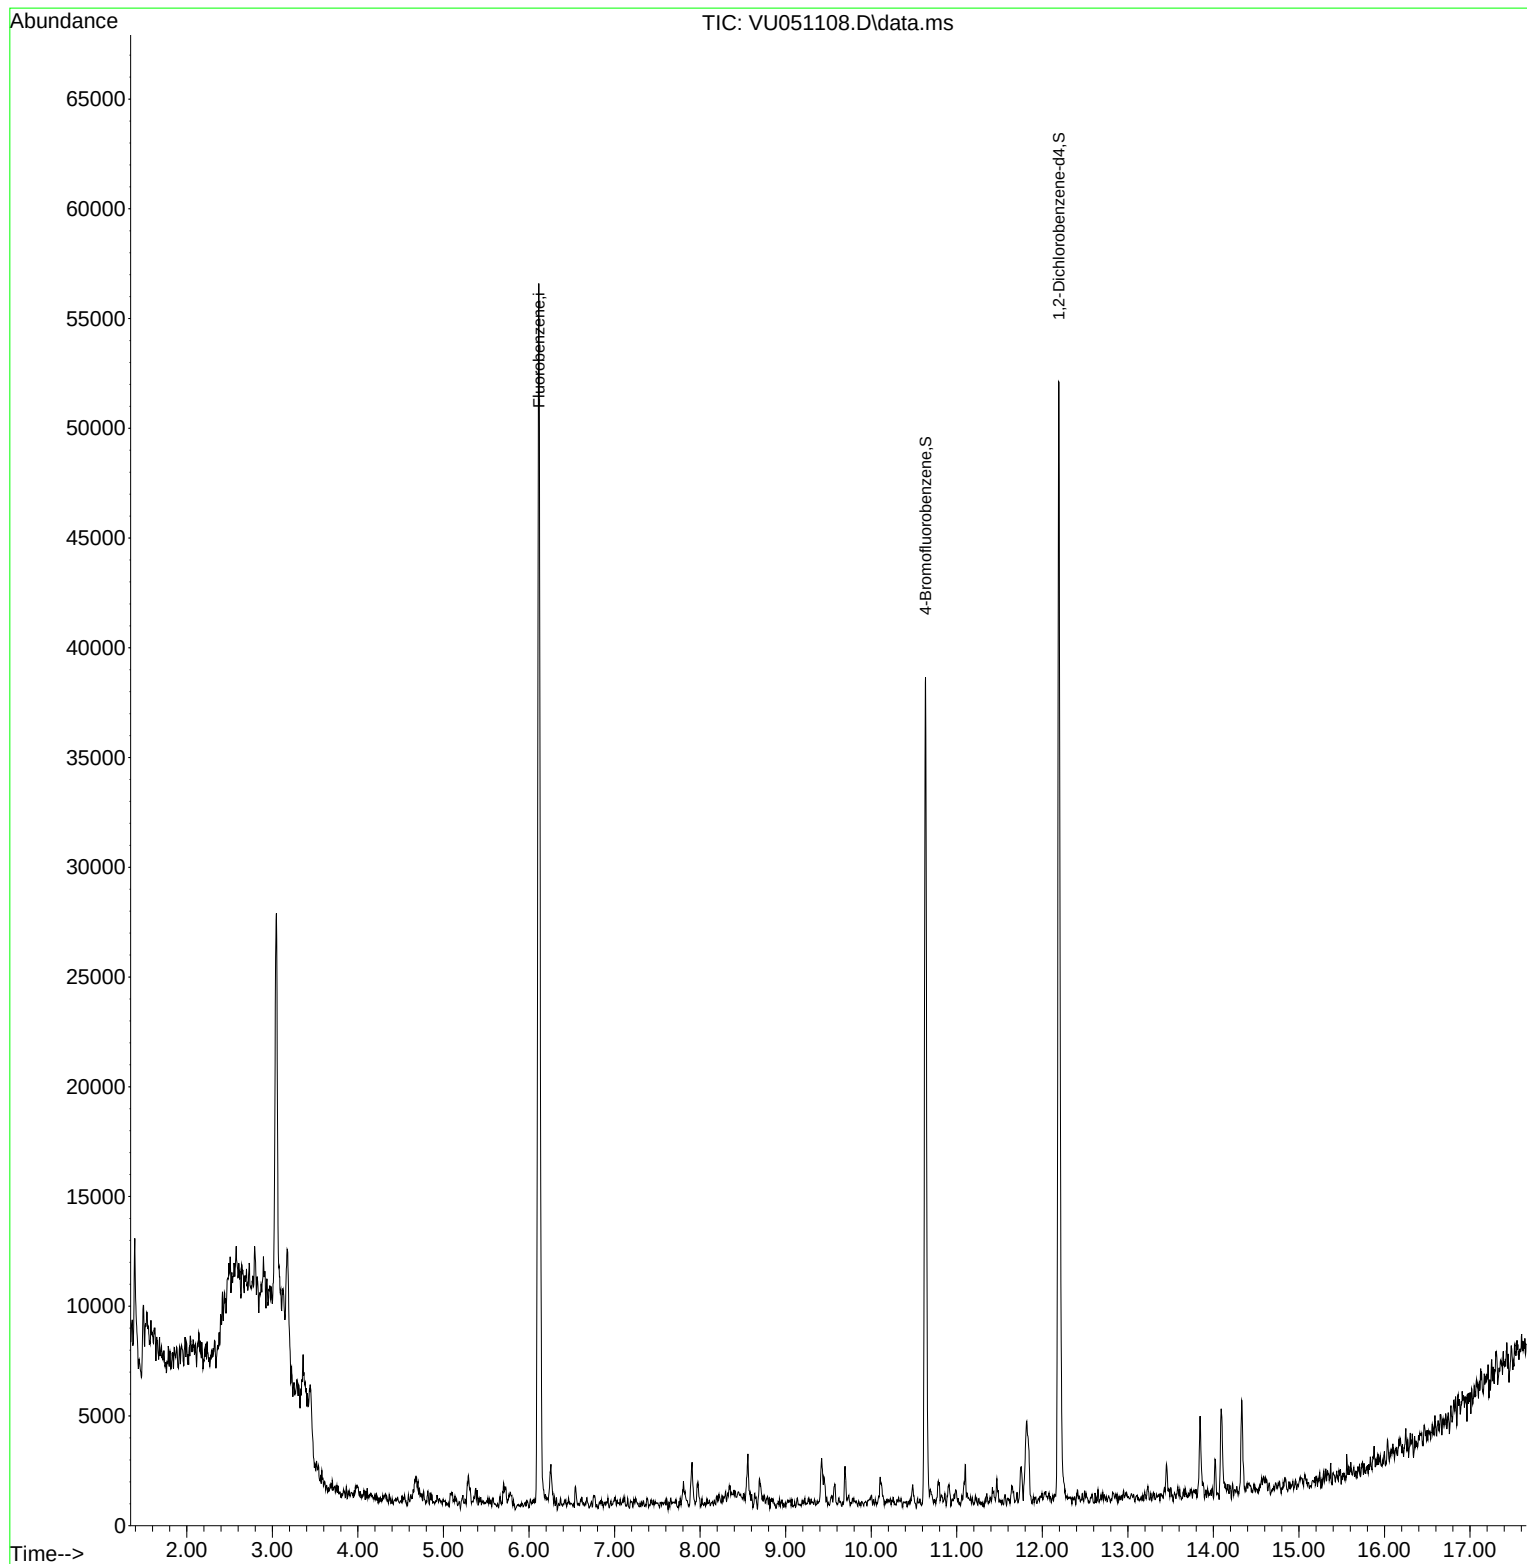


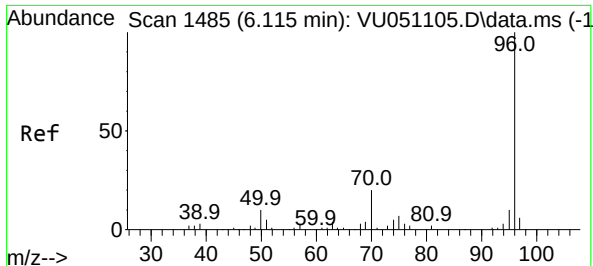

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.115 min Scan# 1485
Delta R.T. -0.000 min
Lab File: VU051108.D
Acq: 04 Oct 2022 15:17




Instrument :
MSVOA_U
ClientSampleId :
VU1004WBL01


Tgt Ion: 96	Resp: 52308
Ion Ratio	Lower Upper
96 100	
70 19.8	16.7 25.1
95 8.5	7.4 11.0
97 6.5	0.0 0.0#

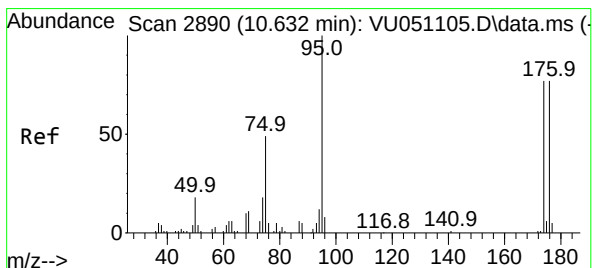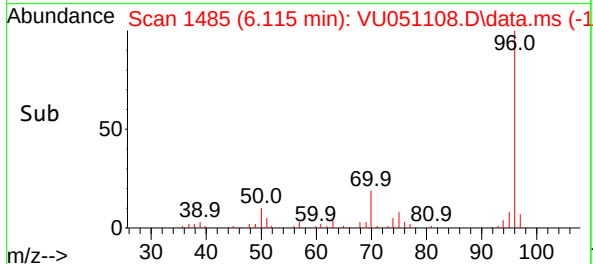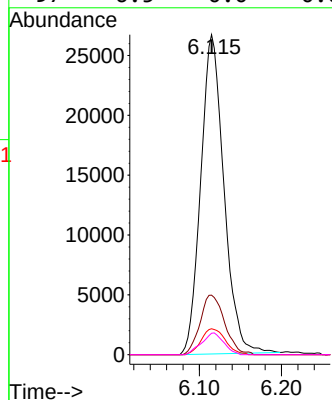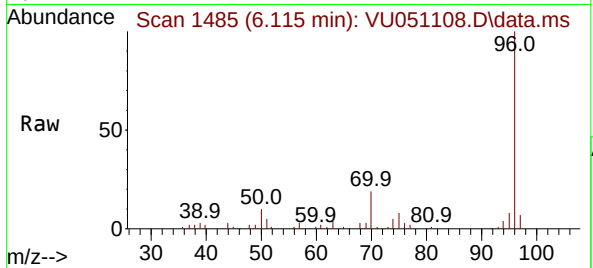

#57
4-Bromofluorobenzene
Concen: 0.750 ug/l
RT: 10.636 min Scan# 2891
Delta R.T. 0.003 min
Lab File: VU051108.D
Acq: 04 Oct 2022 15:17


Tgt Ion: 95	Resp: 12888
Ion Ratio	Lower Upper
95 100	
174 86.4	62.4 93.6
176 77.7	56.2 84.2

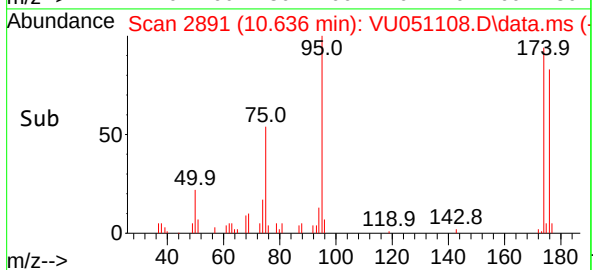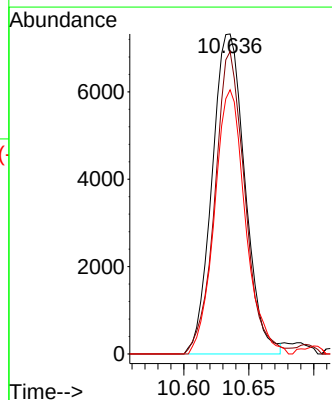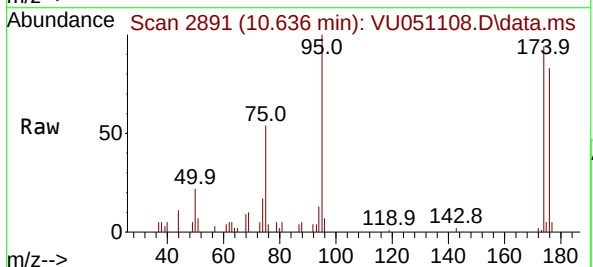

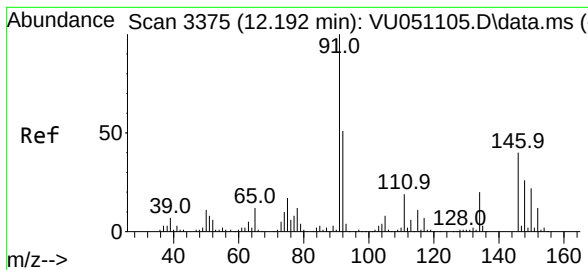

#68
 1,2-Dichlorobenzene-d4
 Concen: 0.766 ug/l
 RT: 12.195 min Scan# 31
 Delta R.T. 0.003 min
 Lab File: VU051108.D
 Acq: 04 Oct 2022 15:17

Instrument :
 MSVOA_U
 ClientSampleId :
 VU1004WBL01

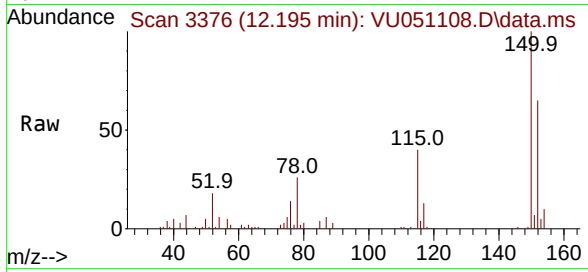

Tgt Ion:152	Resp:	14634
Ion	Ratio	Lower Upper
152	100	
115	63.0	0.0 254.6
150	163.4	0.0 623.6

