


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100422\
Data File : VU051100.D
Acq On : 04 Oct 2022 08:32
Operator : JC/MD
Sample : BFB
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U100422DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER
Last Update : Wed Oct 05 02:45:21 2022

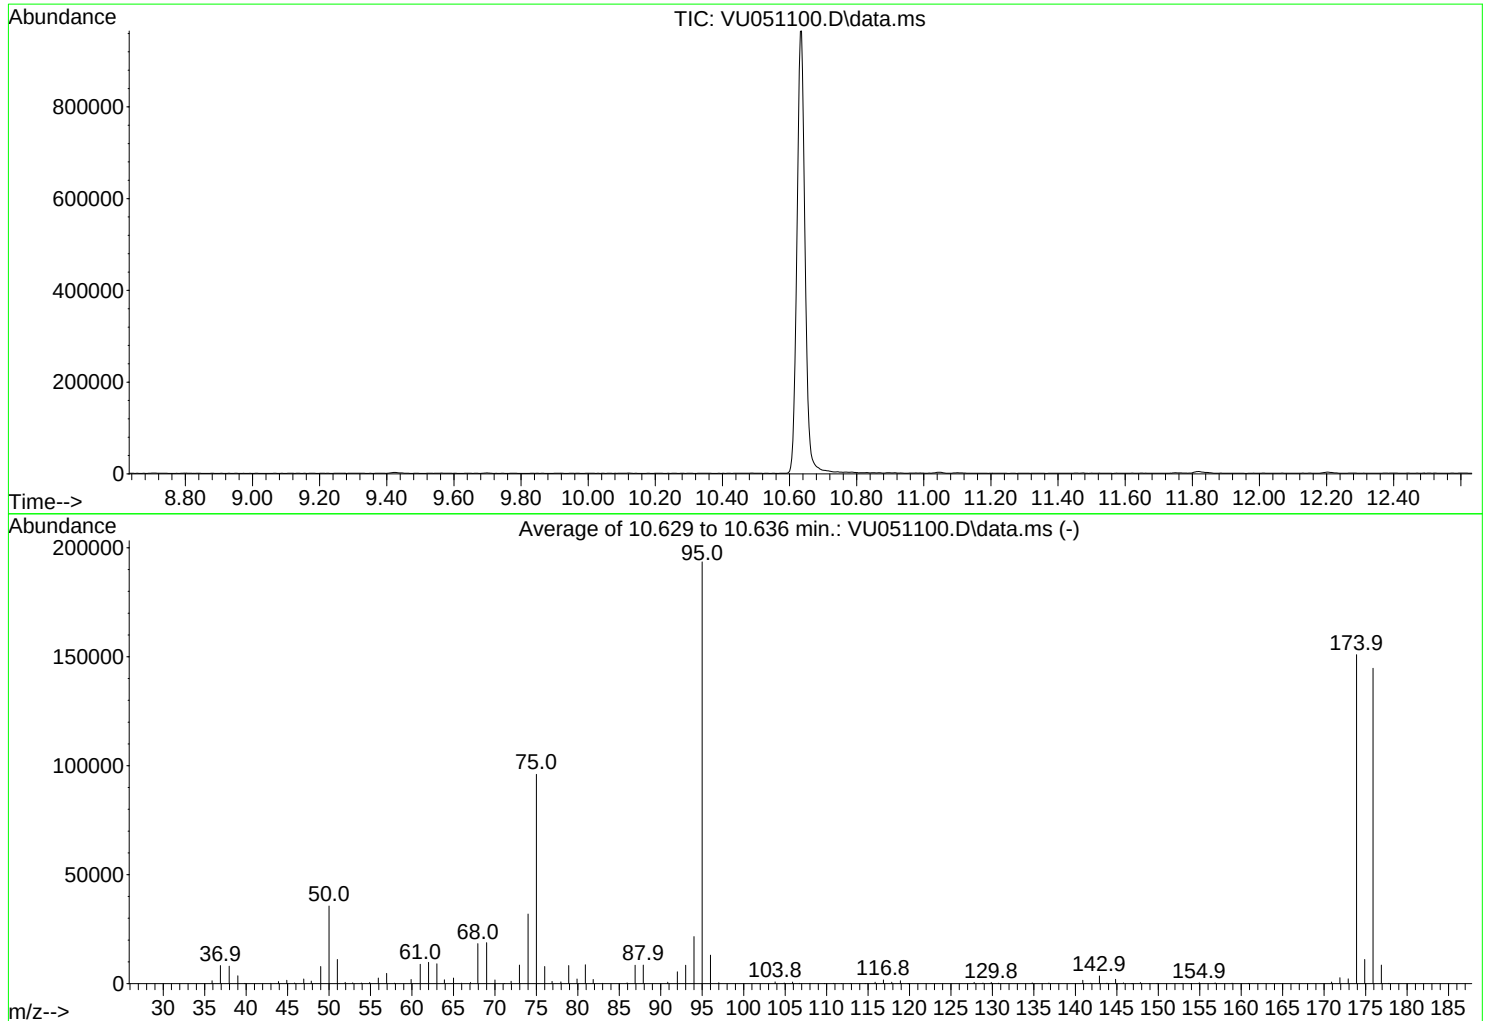

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2875

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.4	35621	PASS
75	95	30	60	49.6	96056	PASS
95	95	100	100	100.0	193557	PASS
96	95	5	9	6.7	13041	PASS
173	174	0.00	2	1.5	2201	PASS
174	95	50	100	78.0	150976	PASS
175	174	5	9	7.3	11089	PASS
176	174	95	101	95.8	144704	PASS
177	176	5	9	5.9	8524	PASS