




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
 Data File : VU051137.D
 Acq On : 05 Oct 2022 19:33
 Operator : JC/MD
 Sample : N4973-03ME
 Misc : 5.98g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY198ME

Manual IntegrationsAPPROVED

Quant Time: Oct 06 03:06:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Oct 06 02:55:50 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 10/06/2022
 Supervised By :Mahesh Dadoda 10/08/2022

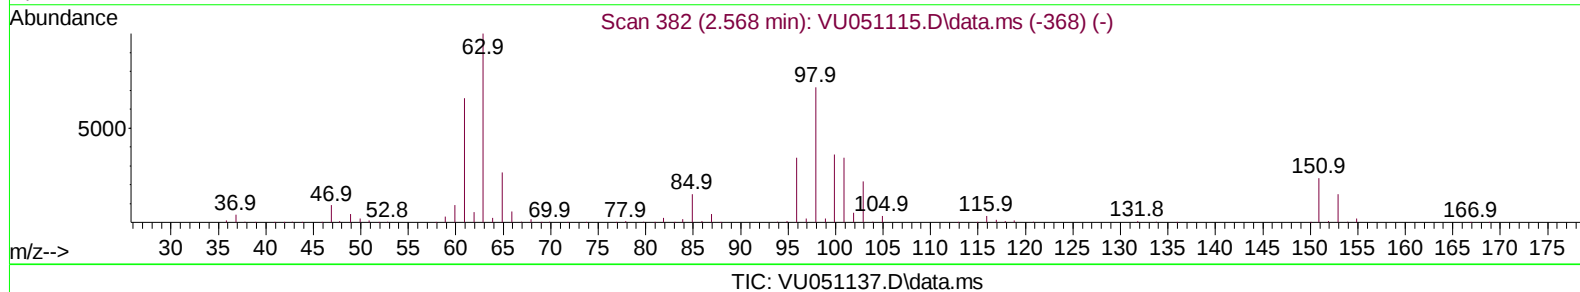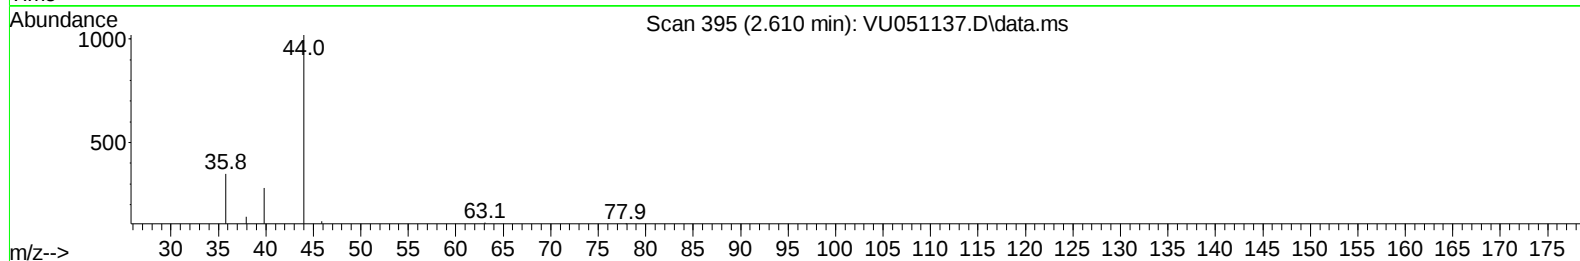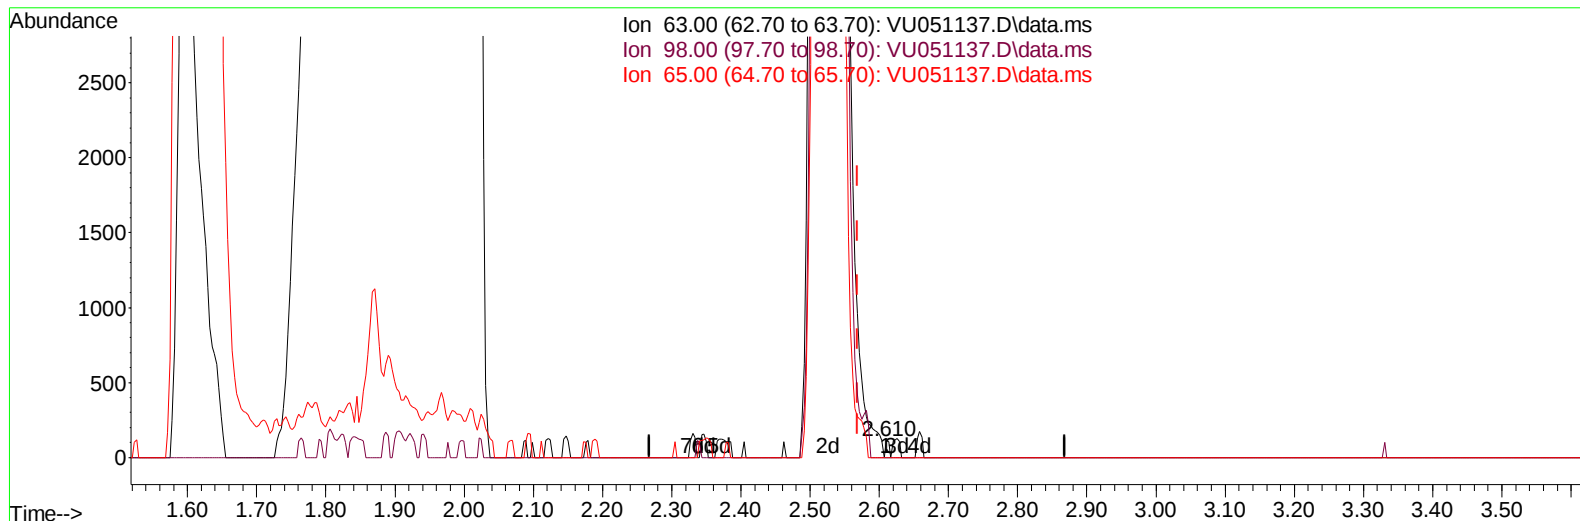

(11) 1,1-Dichloroethene-d2 (S)

2.610min (+ 0.042) 0.01 ug/L

response 42

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	75.40	380.95#
65.00	24.10	0.00#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
 Data File : VU051137.D
 Acq On : 05 Oct 2022 19:33
 Operator : JC/MD
 Sample : N4973-03ME
 Misc : 5.98g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY198ME

Manual IntegrationsAPPROVED

Quant Time: Oct 06 03:06:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Oct 06 02:55:50 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 10/06/2022
 Supervised By :Mahesh Dadoda 10/08/2022

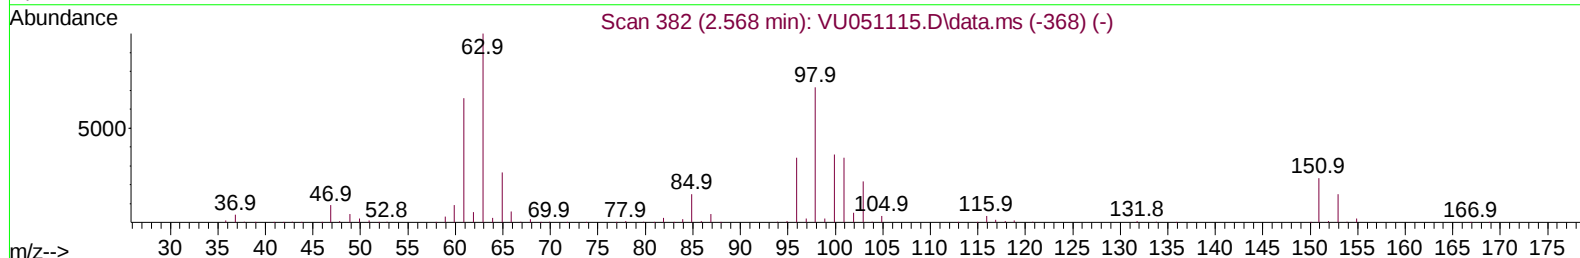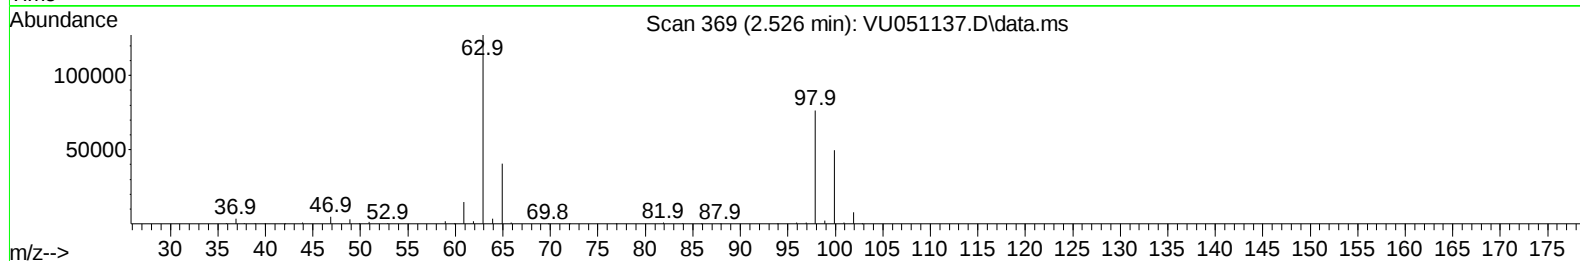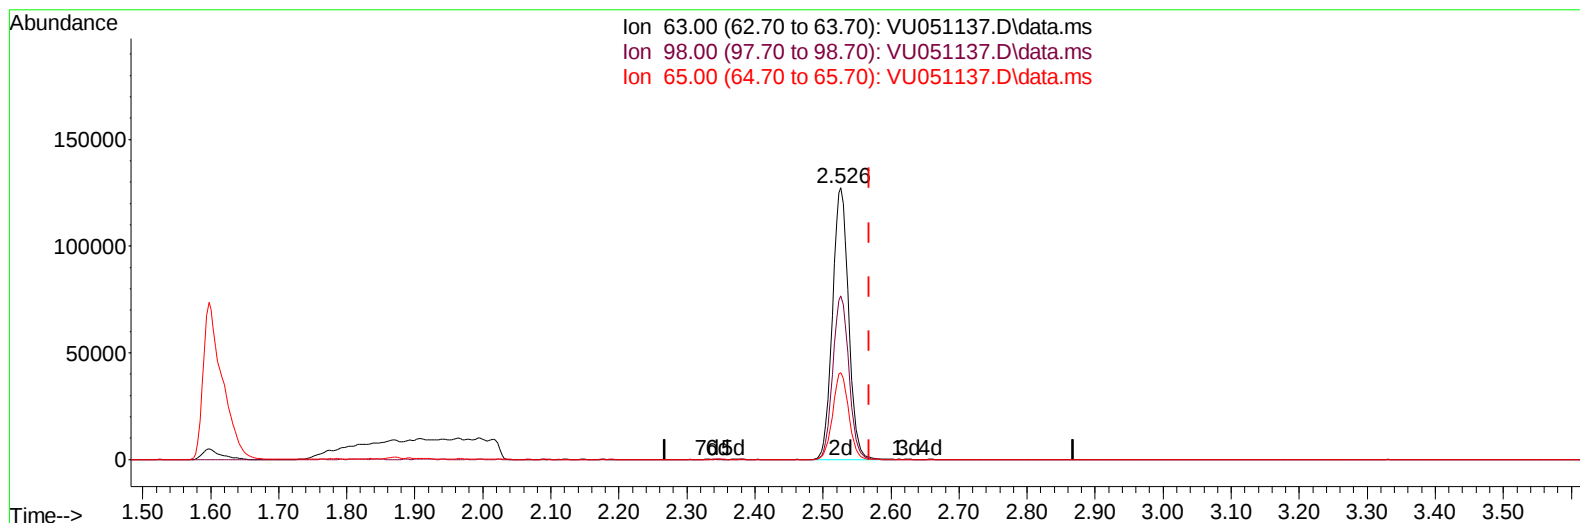

TIC: VU051137.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

2.526min (-0.042) 38.30 ug/L m

response 209047

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	75.40	0.08#
65.00	24.10	0.00#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
 Data File : VU051137.D
 Acq On : 05 Oct 2022 19:33
 Operator : JC/MD
 Sample : N4973-03ME
 Misc : 5.98g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY198ME

Manual IntegrationsAPPROVED

Quant Time: Oct 06 03:06:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Oct 06 02:55:50 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 10/06/2022
 Supervised By :Mahesh Dadoda 10/08/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.243	114	364573	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	374077	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	143664	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	143362	38.801	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	77.600%	
7) Chloroethane-d5	1.867	69	69730	20.317	ug/L	-0.04
Spiked Amount 50.000	Range 70	- 130	Recovery	=	40.640%#	
11) 1,1-Dichloroethene-d2	2.526	63	209047m	38.303	ug/L	-0.04
Spiked Amount 50.000	Range 60	- 125	Recovery	=	76.600%	
21) 2-Butanone-d5	4.632	46	264283	110.285	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	110.280%	
24) Chloroform-d	5.057	84	329582	55.367	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	110.740%	
26) 1,2-Dichloroethane-d4	5.697	65	219549	59.587	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	119.180%	
32) Benzene-d6	5.719	84	671587	61.308	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	122.620%	
36) 1,2-Dichloropropane-d6	6.687	67	231247	65.056	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	130.120%#	
41) Toluene-d8	7.896	98	553125	54.651	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	109.300%	
43) trans-1,3-Dichloroprop...	8.179	79	86399	50.960	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	101.920%	
47) 2-Hexanone-d5	8.648	63	160294	111.680	ug/L	0.02
Spiked Amount 100.000	Range 45	- 130	Recovery	=	111.680%	
56) 1,1,2,2-Tetrachloroeth...	10.761	84	371319	59.771	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	119.540%	
66) 1,2-Dichlorobenzene-d4	12.195	152	196520	64.033	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	128.060%#	
Target Compounds						
46) Tetrachloroethene	8.552	164	6611	2.953	ug/L	Qvalue 95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
Data File : VU051137.D
Acq On : 05 Oct 2022 19:33
Operator : JC/MD
Sample : N4973-03ME
Misc : 5.98g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY198ME

Manual IntegrationsAPPROVED

Quant Time: Oct 06 03:06:32 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Oct 06 02:55:50 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 10/06/2022
Supervised By :Mahesh Dadoda 10/08/2022

