

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
 Data File : VU051123.D
 Acq On : 05 Oct 2022 13:39
 Operator : JC/MD
 Sample : N4853-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY1B1

Quant Time: Oct 06 03:03:38 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Oct 06 02:55:50 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	331068	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	346124	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	116546	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	154621	46.084	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	92.160%
7) Chloroethane-d5	1.899	69	138448	44.421	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	88.840%
11) 1,1-Dichloroethene-d2	2.562	63	184488	37.224	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	74.440%
21) 2-Butanone-d5	4.620	46	220388	101.275	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	101.270%
24) Chloroform-d	5.060	84	289158	53.492	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	106.980%
26) 1,2-Dichloroethane-d4	5.700	65	185355	55.398	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	110.800%
32) Benzene-d6	5.726	84	552012	54.462	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	108.920%
36) 1,2-Dichloropropane-d6	6.690	67	192927	58.659	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	117.320%
41) Toluene-d8	7.896	98	425679	45.456	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	90.920%
43) trans-1,3-Dichloroprop...	8.179	79	63754	40.640	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	81.280%
47) 2-Hexanone-d5	8.632	63	98879	74.455	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	74.450%
56) 1,1,2,2-Tetrachloroeth...	10.754	84	292433	50.875	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	101.740%
66) 1,2-Dichlorobenzene-d4	12.192	152	144847	58.177	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	116.360%
Target Compounds						
16) Methylene chloride	3.044	84	4022	1.187	ug/L	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
Data File : VU051123.D
Acq On : 05 Oct 2022 13:39
Operator : JC/MD
Sample : N4853-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY1B1


Quant Time: Oct 06 03:03:38 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Oct 06 02:55:50 2022
Response via : Initial Calibration

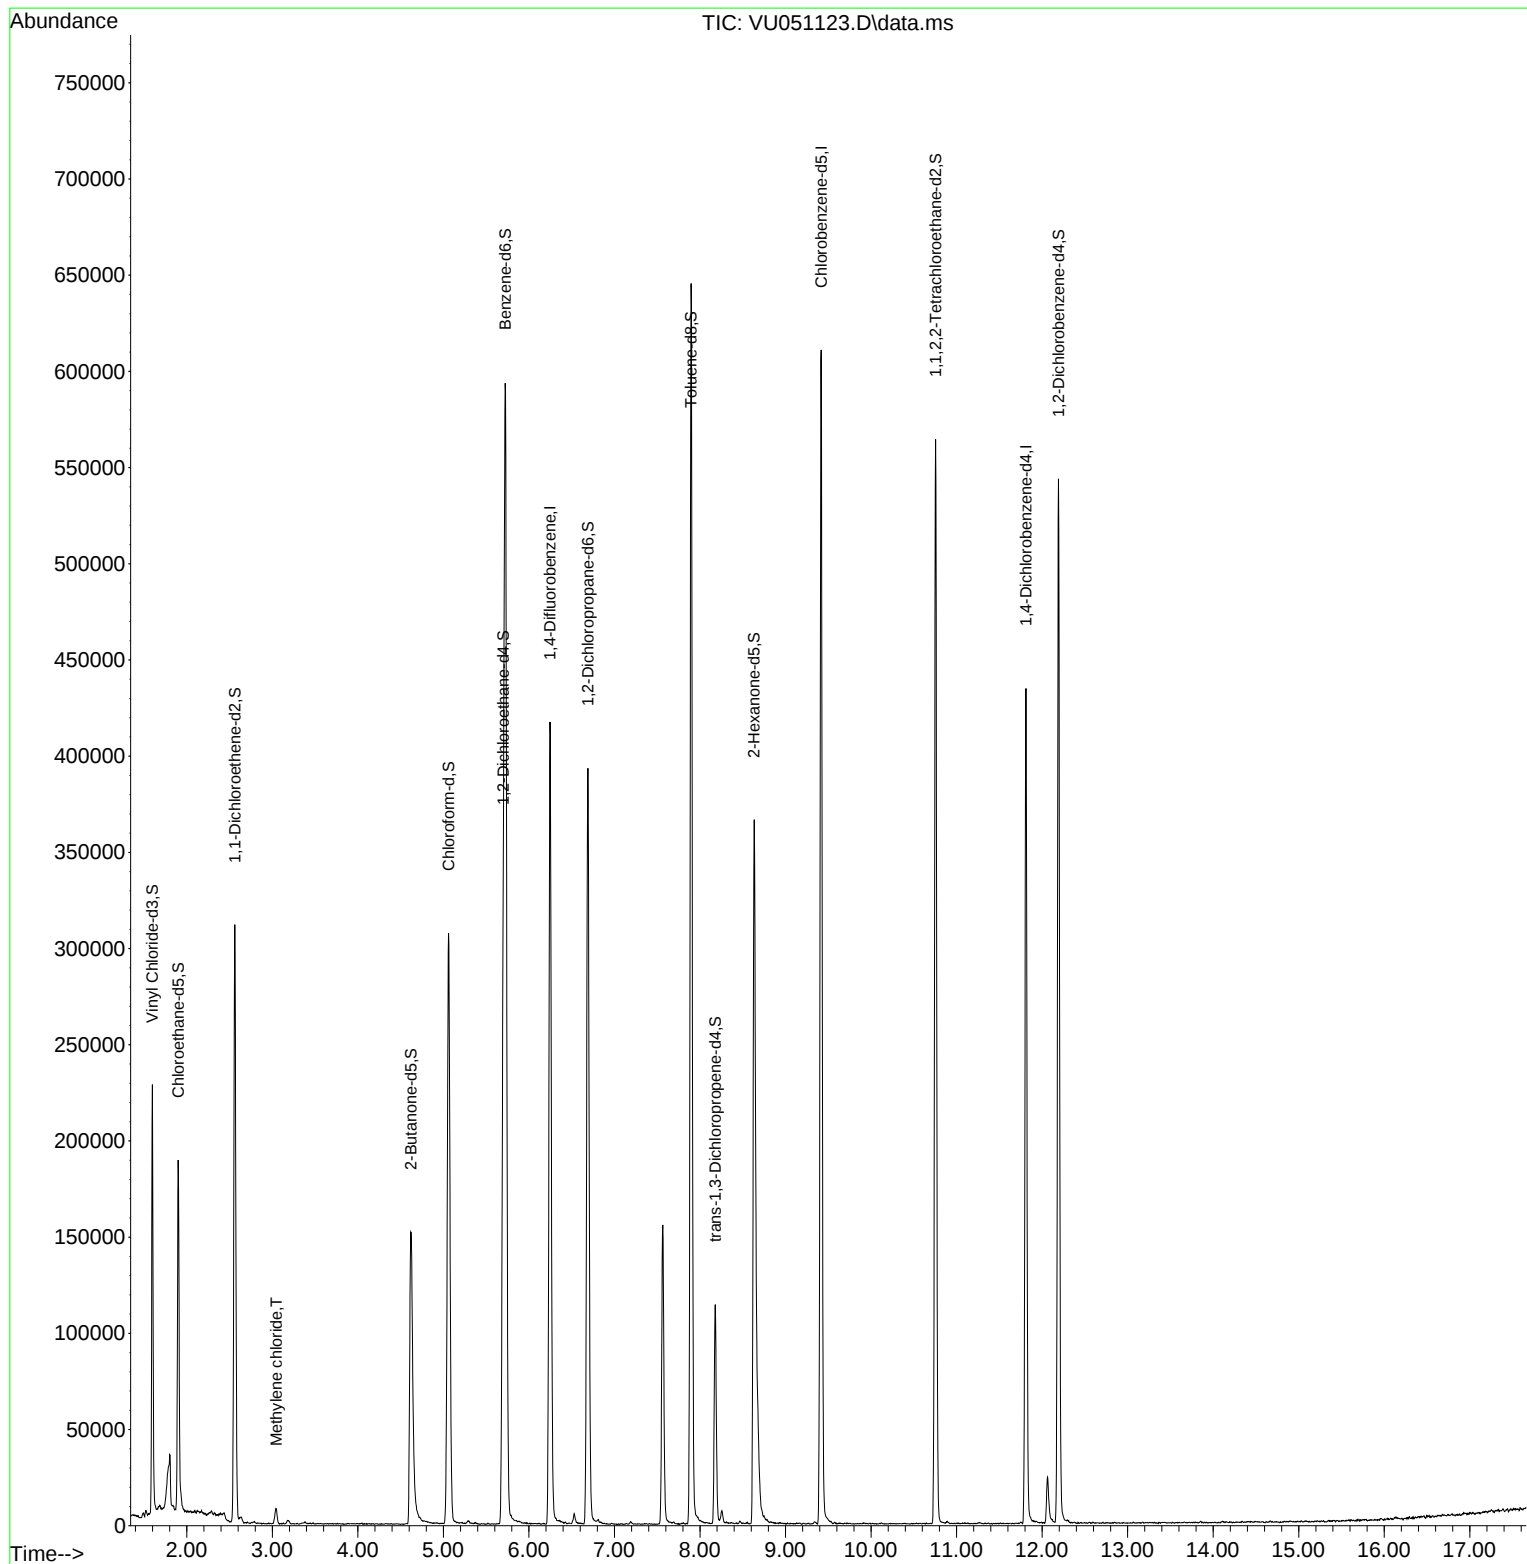

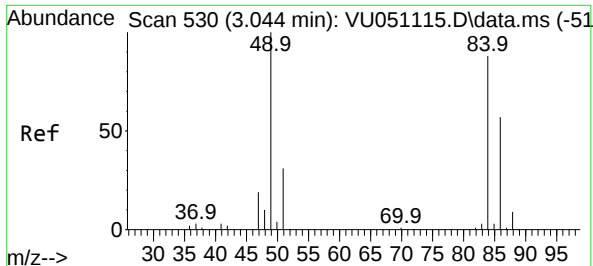

#16
Methylene chloride
Concen: 1.187 ug/L
RT: 3.044 min Scan# 51
Delta R.T. -0.000 min
Lab File: VU051123.D
Acq: 05 Oct 2022 13:39

Instrument :
MSVOA_U
ClientSampleId :
EY1B1

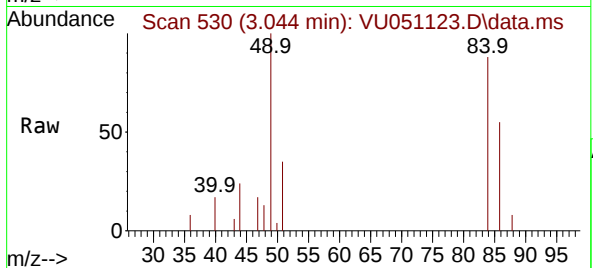

Tgt Ion:	84	Resp:	4022
Ion	Ratio	Lower	Upper
84	100		
86	62.2	45.4	84.4
49	113.8	78.3	145.3

