

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
 Data File : VU051139.D
 Acq On : 05 Oct 2022 20:20
 Operator : JC/MD
 Sample : N4858-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGSK3

Quant Time: Oct 06 03:06:55 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Oct 06 02:55:50 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	355642	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	371298	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	124636	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	143058	39.692	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	79.380%		
7) Chloroethane-d5	1.900	69	138694	41.425	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	82.860%		
11) 1,1-Dichloroethene-d2	2.562	63	183917	34.545	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	69.080%		
21) 2-Butanone-d5	4.620	46	236558	101.194	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	101.190%		
24) Chloroform-d	5.060	84	297940	51.308	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	102.620%		
26) 1,2-Dichloroethane-d4	5.700	65	195759	54.464	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	108.920%		
32) Benzene-d6	5.726	84	583779	53.691	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	107.380%		
36) 1,2-Dichloropropane-d6	6.687	67	203895	57.790	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	115.580%		
41) Toluene-d8	7.896	98	457655	45.557	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	91.120%		
43) trans-1,3-Dichloroprop...	8.176	79	72685	43.192	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	86.380%		
47) 2-Hexanone-d5	8.632	63	112220	78.771	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	78.770%		
56) 1,1,2,2-Tetrachloroeth...	10.755	84	307961	49.943	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	99.880%		
66) 1,2-Dichlorobenzene-d4	12.192	152	146916	55.178	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	110.360%		
Target Compounds					Qvalue	
13) Acetone	2.626	43	4843	2.594	ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
Data File : VU051139.D
Acq On : 05 Oct 2022 20:20
Operator : JC/MD
Sample : N4858-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGSK3

Quant Time: Oct 06 03:06:55 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Oct 06 02:55:50 2022
Response via : Initial Calibration

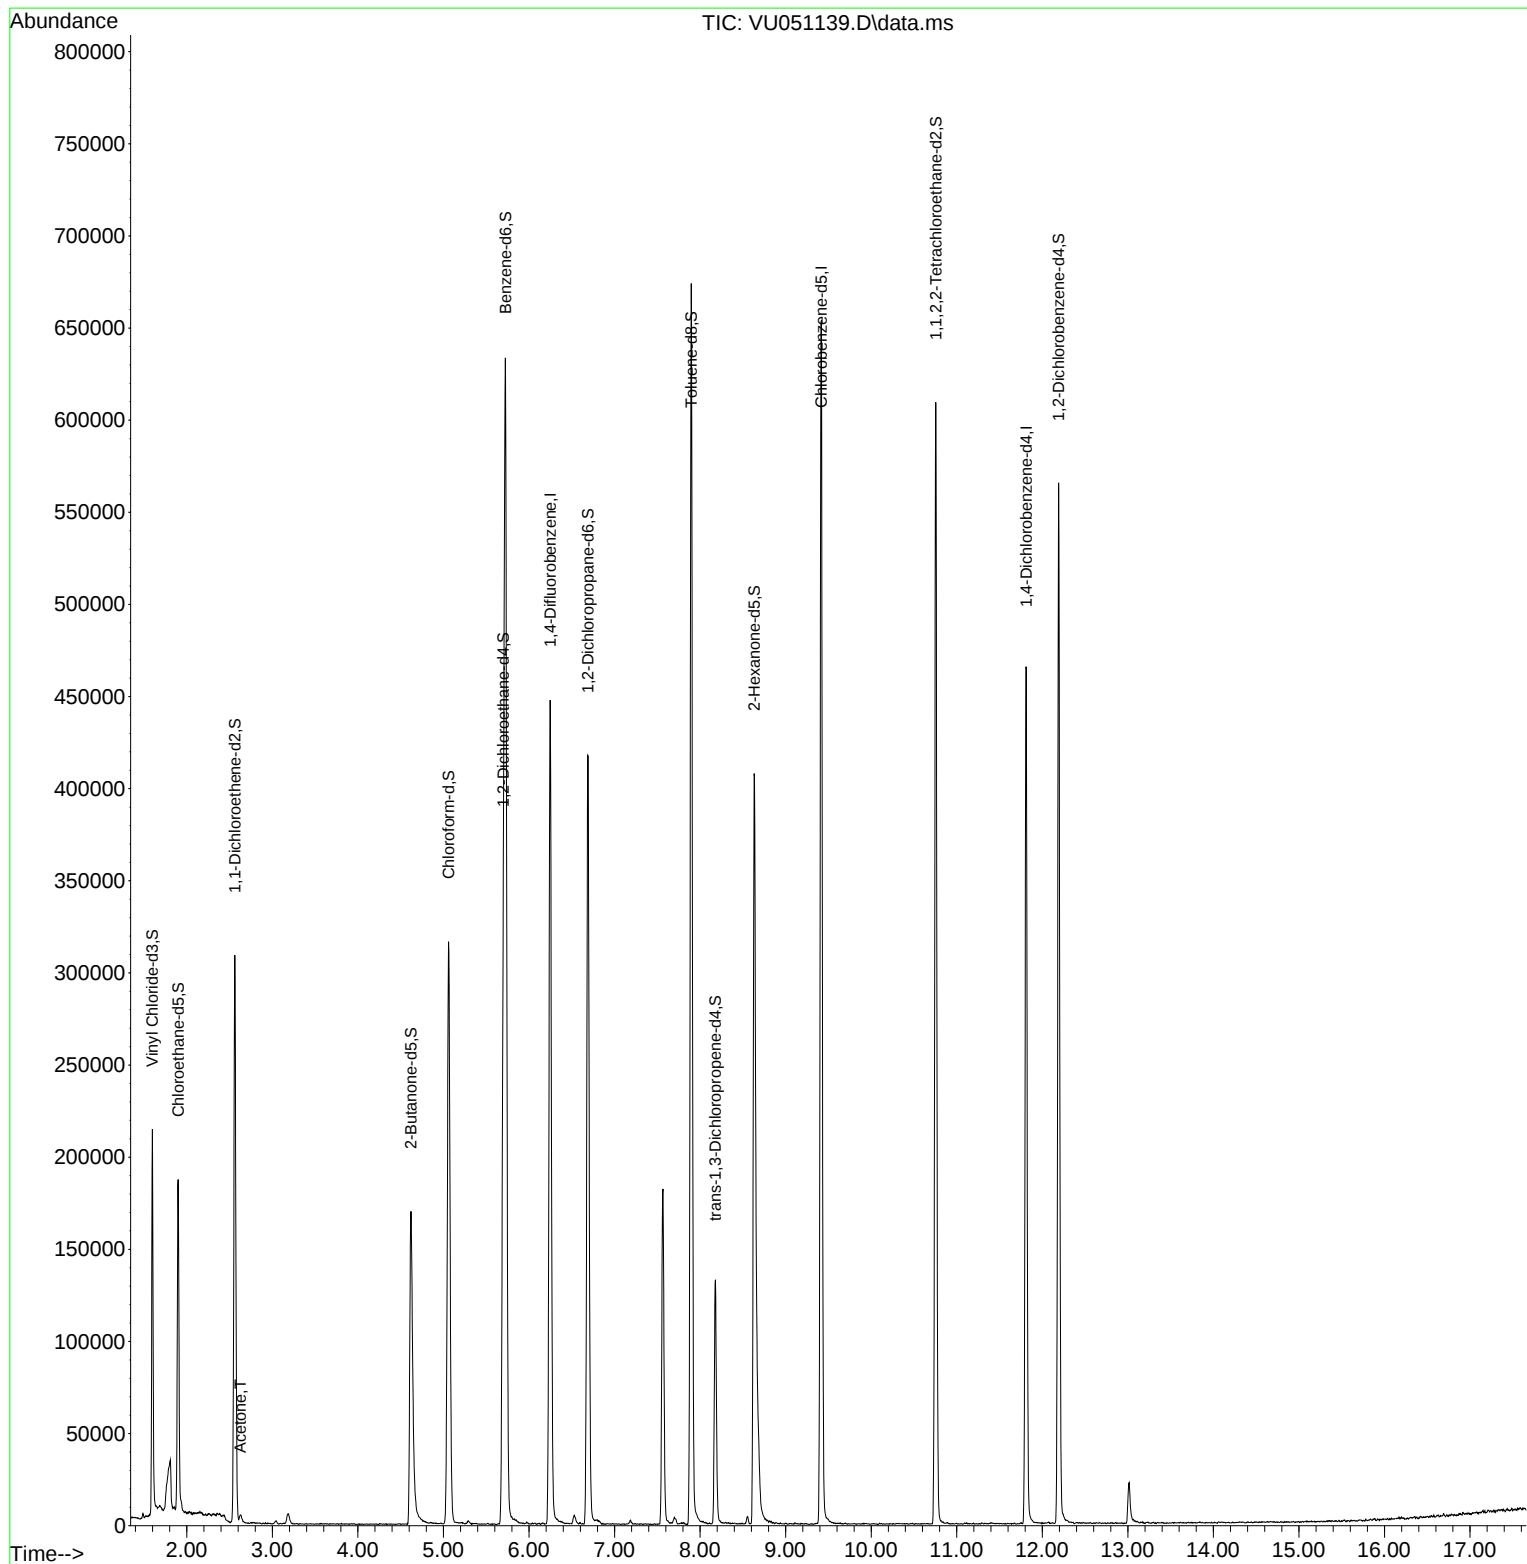

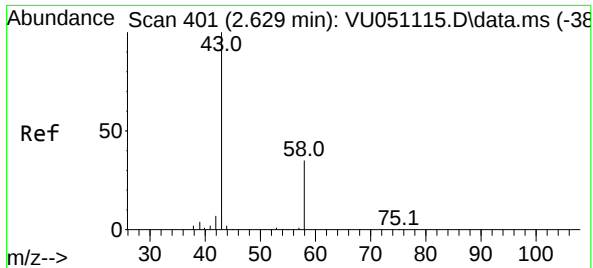

#13
 Acetone
 Concen: 2.594 ug/L
 RT: 2.626 min Scan# 40
 Delta R.T. -0.003 min
 Lab File: VU051139.D
 Acq: 05 Oct 2022 20:20

Instrument :
 MSVOA_U
 ClientSampleId :
 BGSK3

Tgt Ion: 43 Resp: 4843
 Ion Ratio Lower Upper
 43 100
 58 30.6 0.0 73.6

