

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
 Data File : VU051117.D
 Acq On : 05 Oct 2022 11:17
 Operator : JC/MD
 Sample : VU1005WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK197

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

Signal : TIC: VU051117.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	100	rBV	220531	264211	15.27%	2.073%
2	1.899	165	174	184	rBV	187420	250595	14.48%	1.966%
3	2.491	355	358	361	rVB2	754	422	0.02%	0.003%
4	2.562	368	380	396	rBV	339833	555864	32.12%	4.362%
5	2.768	433	444	448	rBV5	1803	3233	0.19%	0.025%
6	2.858	465	472	476	rBV3	614	910	0.05%	0.007%
7	2.880	476	479	484	rVV3	434	360	0.02%	0.003%
8	2.928	491	494	500	rBV3	400	551	0.03%	0.004%
9	3.009	516	519	521	rBV2	515	369	0.02%	0.003%
10	3.044	521	530	539	rVV2	4051	6900	0.40%	0.054%
11	3.079	539	541	548	rVB3	632	512	0.03%	0.004%
12	3.118	548	553	555	rBV2	472	434	0.03%	0.003%
13	3.182	558	573	590	rBV	51625	125467	7.25%	0.984%
14	3.327	614	618	622	rVB2	399	342	0.02%	0.003%
15	3.356	624	627	630	rVV3	493	352	0.02%	0.003%
16	3.430	645	650	652	rBV3	516	374	0.02%	0.003%
17	3.501	668	672	676	rVB2	355	328	0.02%	0.003%
18	3.726	738	742	748	rVB	579	510	0.03%	0.004%
19	3.858	779	783	787	rBV2	365	302	0.02%	0.002%
20	4.169	878	880	884	rVB	871	470	0.03%	0.004%
21	4.202	884	890	892	rBV	549	521	0.03%	0.004%
22	4.266	906	910	915	rVV	1101	869	0.05%	0.007%
23	4.314	919	925	927	rVV2	533	490	0.03%	0.004%
24	4.353	933	937	939	rBV2	493	301	0.02%	0.002%
25	4.491	976	980	984	rBV2	536	375	0.02%	0.003%
26	4.620	1004	1020	1049	rBV	193409	497443	28.74%	3.903%
27	4.989	1133	1135	1140	rVB4	425	330	0.02%	0.003%
28	5.060	1140	1157	1180	rBV	322921	708428	40.93%	5.559%
29	5.189	1192	1197	1199	rBV3	573	387	0.02%	0.003%
30	5.372	1251	1254	1262	rVB2	993	949	0.05%	0.007%
31	5.462	1278	1282	1285	rBV2	501	323	0.02%	0.003%
32	5.520	1296	1300	1302	rBV2	488	304	0.02%	0.002%
33	5.594	1318	1323	1327	rBV2	331	304	0.02%	0.002%
34	5.722	1341	1363	1386	rBV2	637980	1730622	100.00%	13.580%
35	6.247	1512	1526	1548	rBV	472945	904813	52.28%	7.100%
36	6.530	1604	1614	1624	rVB6	4973	9088	0.53%	0.071%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
 Data File : VU051117.D
 Acq On : 05 Oct 2022 11:17
 Operator : JC/MD
 Sample : VU1005WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK197

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	6.687	1648	1663	1684	rBV	418231	814740	47.08%	6.393%
38	6.857	1714	1716	1719	rVB3	686	358	0.02%	0.003%
39	6.922	1730	1736	1739	rBV3	492	518	0.03%	0.004%
40	7.179	1806	1816	1817	rBV2	1559	1298	0.08%	0.010%
41	7.285	1837	1849	1852	rBV2	258	531	0.03%	0.004%
42	7.385	1876	1880	1887	rVB2	375	410	0.02%	0.003%
43	7.565	1921	1936	1952	rBV2	168092	299531	17.31%	2.350%
44	7.793	1999	2007	2012	rBV4	1297	1660	0.10%	0.013%
45	7.896	2024	2039	2062	rBV	703690	1218517	70.41%	9.561%
46	8.179	2115	2127	2149	rBV	123681	210476	12.16%	1.652%
47	8.410	2194	2199	2205	rVV3	773	899	0.05%	0.007%
48	8.488	2219	2223	2227	rVB3	609	406	0.02%	0.003%
49	8.632	2255	2268	2307	rBV2	450102	989689	57.19%	7.766%
50	8.877	2340	2344	2351	rVB6	747	760	0.04%	0.006%
51	8.954	2364	2368	2370	rBV	440	312	0.02%	0.002%
52	8.986	2374	2378	2383	rVB2	500	488	0.03%	0.004%
53	9.092	2408	2411	2414	rBV2	482	317	0.02%	0.002%
54	9.324	2480	2483	2490	rVB2	325	321	0.02%	0.003%
55	9.353	2490	2492	2497	rBV3	454	357	0.02%	0.003%
56	9.417	2497	2512	2530	rBV	714452	1176915	68.01%	9.235%
57	9.645	2580	2583	2590	rVB3	700	661	0.04%	0.005%
58	9.690	2590	2597	2600	rBV2	498	679	0.04%	0.005%
59	9.838	2640	2643	2649	rVB2	559	477	0.03%	0.004%
60	9.880	2649	2656	2659	rBV2	370	510	0.03%	0.004%
61	10.105	2722	2726	2730	rBV3	661	572	0.03%	0.004%
62	10.214	2757	2760	2764	rVV3	487	454	0.03%	0.004%
63	10.288	2779	2783	2788	rBV	385	372	0.02%	0.003%
64	10.426	2822	2826	2829	rVB	564	323	0.02%	0.003%
65	10.462	2829	2837	2840	rBV2	349	454	0.03%	0.004%
66	10.481	2840	2843	2848	rBV2	403	384	0.02%	0.003%
67	10.639	2889	2892	2902	rBV5	589	838	0.05%	0.007%
68	10.684	2903	2906	2909	rBV	429	308	0.02%	0.002%
69	10.754	2915	2928	2949	rBV	635612	1027492	59.37%	8.062%
70	10.851	2955	2958	2961	rVB2	629	391	0.02%	0.003%
71	10.954	2987	2990	2993	rBV2	450	306	0.02%	0.002%
72	10.996	2998	3003	3004	rBV2	444	381	0.02%	0.003%
73	11.060	3019	3023	3026	rVB3	380	299	0.02%	0.002%
74	11.089	3027	3032	3038	rBV5	689	749	0.04%	0.006%
75	11.230	3073	3076	3087	rVB2	466	534	0.03%	0.004%
76	11.333	3105	3108	3115	rVB	408	386	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
 Data File : VU051117.D
 Acq On : 05 Oct 2022 11:17
 Operator : JC/MD
 Sample : VU1005WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK197

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	11.471	3147	3151	3157	rVV2	587	748	0.04%	0.006%
78	11.745	3231	3236	3243	rBV2	896	896	0.05%	0.007%
79	11.809	3244	3256	3276	rBV	541554	880053	50.85%	6.905%
80	12.192	3362	3375	3399	rBV	623427	1021517	59.03%	8.015%
81	12.539	3480	3483	3487	rVB2	537	382	0.02%	0.003%
82	12.571	3490	3493	3498	rBV3	298	425	0.02%	0.003%
83	12.651	3514	3518	3521	rVB3	549	399	0.02%	0.003%
84	12.671	3521	3524	3527	rBV2	351	317	0.02%	0.002%
85	12.732	3537	3543	3544	rBV	627	479	0.03%	0.004%
86	12.758	3548	3551	3555	rVV2	693	586	0.03%	0.005%
87	12.806	3561	3566	3567	rBV2	362	320	0.02%	0.003%
88	13.147	3668	3672	3677	rBV	505	497	0.03%	0.004%
89	13.217	3691	3694	3696	rBV	584	440	0.03%	0.003%
90	13.301	3717	3720	3724	rVB2	620	417	0.02%	0.003%
91	13.468	3768	3772	3776	rBV3	435	397	0.02%	0.003%
92	13.549	3793	3797	3801	rBV	434	556	0.03%	0.004%
93	13.844	3884	3889	3898	rVB6	1737	2601	0.15%	0.020%
94	14.076	3958	3961	3962	rBV	758	445	0.03%	0.003%
95	14.095	3962	3967	3976	rVB4	2424	3755	0.22%	0.029%
96	14.333	4035	4041	4049	rBV6	2127	3229	0.19%	0.025%
97	14.413	4063	4066	4071	rBV3	559	607	0.04%	0.005%
98	14.561	4107	4112	4115	rBV2	1054	1201	0.07%	0.009%
99	14.989	4242	4245	4250	rBV4	708	510	0.03%	0.004%
100	15.089	4274	4276	4280	rBV2	575	404	0.02%	0.003%




Sum of corrected areas: 12744307

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
Data File : VU051117.D
Acq On : 05 Oct 2022 11:17
Operator : JC/MD
Sample : VU1005WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK197

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

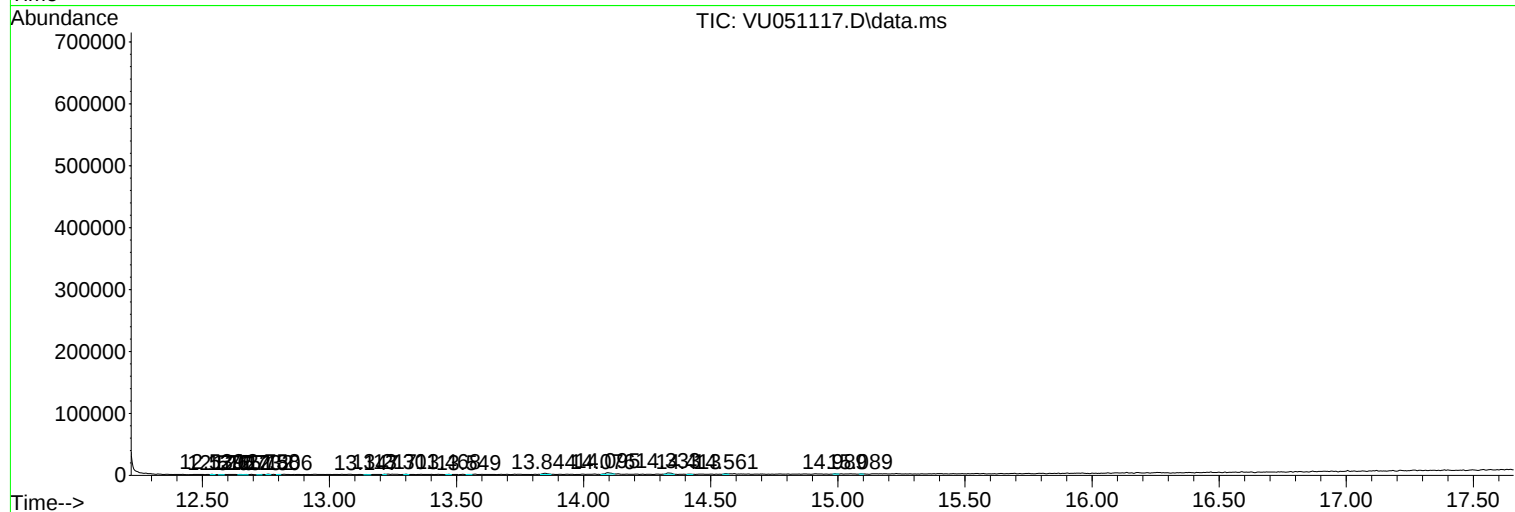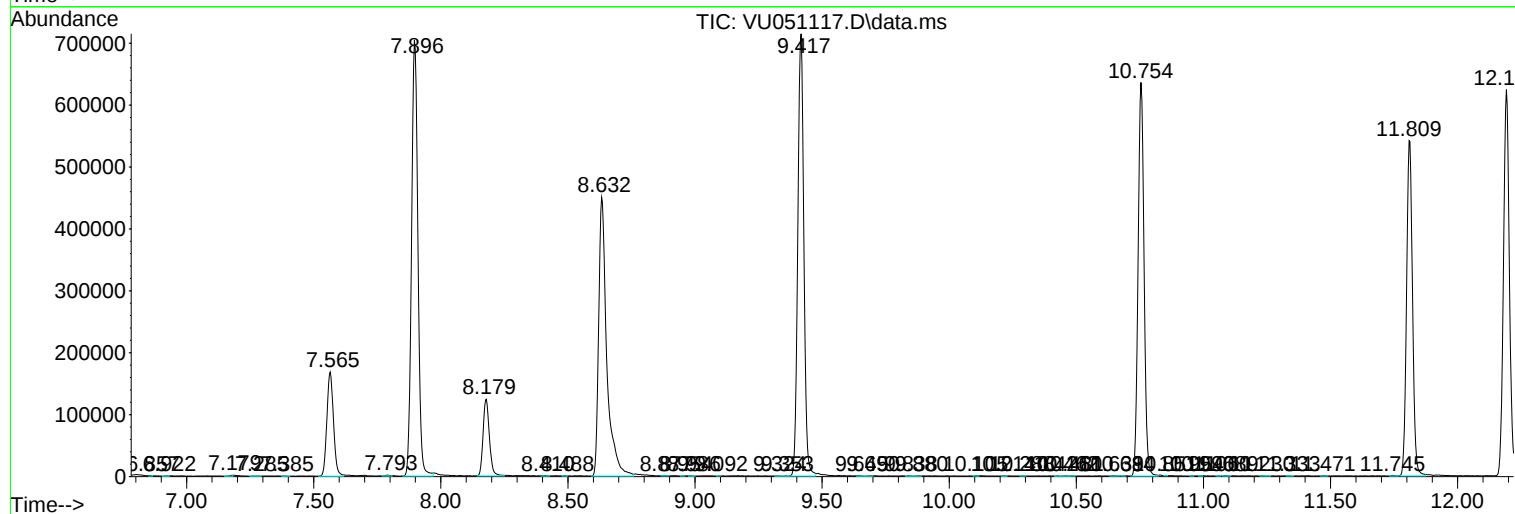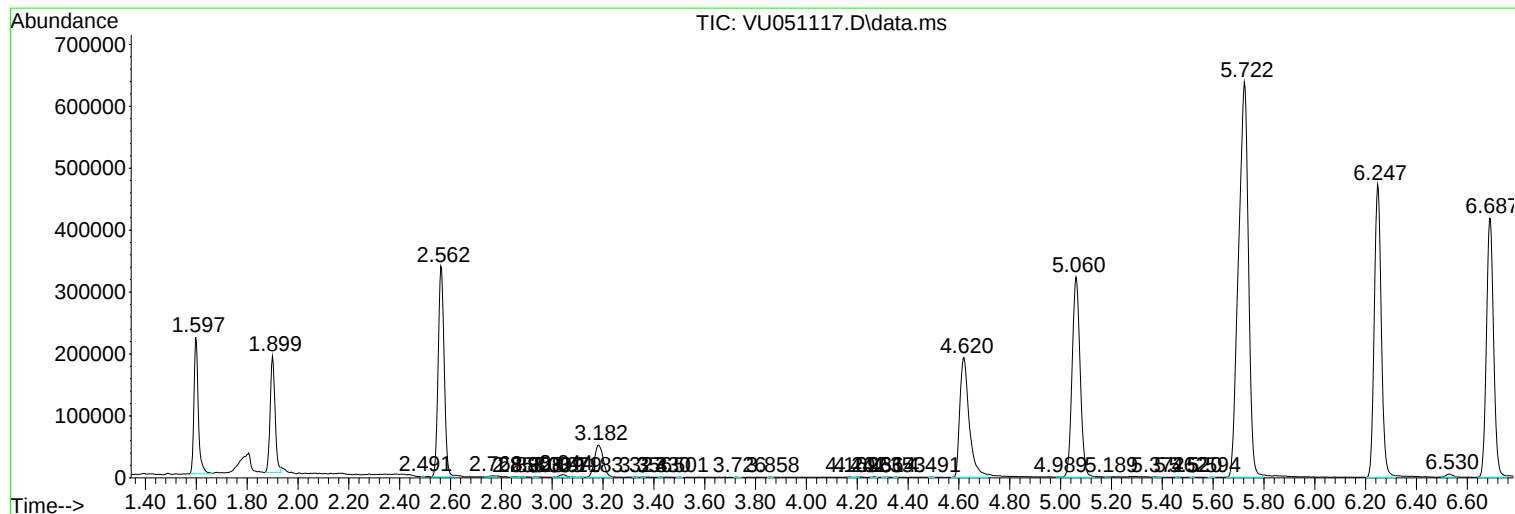

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
Data File : VU051117.D
Acq On : 05 Oct 2022 11:17
Operator : JC/MD
Sample : VU1005WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK197

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
Data File : VU051117.D
Acq On : 05 Oct 2022 11:17
Operator : JC/MD
Sample : VU1005WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK197

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc