

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
 Data File : VU051118.D
 Acq On : 05 Oct 2022 11:41
 Operator : JC/MD
 Sample : N4880-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

Signal : TIC: VU051118.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	96	rBV	234880	263468	15.15%	2.091%
2	1.900	166	174	197	rVB	191248	264641	15.21%	2.101%
3	2.562	368	380	395	rBV	338132	549027	31.56%	4.358%
4	2.684	413	418	420	rBV2	344	285	0.02%	0.002%
5	2.758	432	441	442	rBV2	1485	1750	0.10%	0.014%
6	2.973	505	508	512	rBV2	363	334	0.02%	0.003%
7	3.044	522	530	541	rVB4	4695	8373	0.48%	0.066%
8	3.099	541	547	548	rBV2	486	400	0.02%	0.003%
9	3.182	557	573	594	rVV	49312	112660	6.48%	0.894%
10	3.256	594	596	599	rVV2	537	302	0.02%	0.002%
11	3.359	626	628	634	rVB3	612	438	0.03%	0.003%
12	3.401	638	641	645	rVB2	482	349	0.02%	0.003%
13	3.536	676	683	687	rBV2	275	273	0.02%	0.002%
14	3.732	740	744	748	rBV2	586	435	0.03%	0.003%
15	3.925	802	804	810	rVB	372	285	0.02%	0.002%
16	4.076	845	851	856	rBV2	286	400	0.02%	0.003%
17	4.157	872	876	878	rBV2	389	286	0.02%	0.002%
18	4.198	885	889	892	rBV2	350	285	0.02%	0.002%
19	4.378	939	945	950	rBV2	350	461	0.03%	0.004%
20	4.488	975	979	981	rBV	440	288	0.02%	0.002%
21	4.620	1006	1020	1051	rBV	195004	495916	28.51%	3.937%
22	5.060	1140	1157	1182	rBV	318891	705220	40.54%	5.598%
23	5.218	1203	1206	1208	rBV3	501	429	0.02%	0.003%
24	5.292	1221	1229	1233	rBV5	1493	2369	0.14%	0.019%
25	5.378	1252	1256	1263	rVB4	943	1371	0.08%	0.011%
26	5.723	1340	1363	1392	rBV2	638068	1739478	100.00%	13.808%
27	5.973	1438	1441	1444	rVB3	794	492	0.03%	0.004%
28	6.005	1450	1451	1457	rVB3	408	303	0.02%	0.002%
29	6.063	1466	1469	1474	rVB2	363	355	0.02%	0.003%
30	6.115	1480	1485	1487	rBV	520	398	0.02%	0.003%
31	6.247	1508	1526	1551	rBV	467824	892100	51.29%	7.081%
32	6.417	1576	1579	1581	rVB	554	291	0.02%	0.002%
33	6.533	1605	1615	1628	rVB4	4693	9221	0.53%	0.073%
34	6.600	1633	1636	1639	rBV3	488	334	0.02%	0.003%
35	6.690	1649	1664	1685	rVV	415313	816518	46.94%	6.481%
36	6.919	1732	1735	1741	rVB3	308	286	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
 Data File : VU051118.D
 Acq On : 05 Oct 2022 11:41
 Operator : JC/MD
 Sample : N4880-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	6.973	1748	1752	1759	rBV2	1174	1269	0.07%	0.010%
38	7.108	1792	1794	1800	rVB3	645	534	0.03%	0.004%
39	7.144	1800	1805	1807	rBV2	454	357	0.02%	0.003%
40	7.166	1807	1812	1813	rVV2	644	565	0.03%	0.004%
41	7.182	1813	1817	1825	rVV5	1240	1884	0.11%	0.015%
42	7.327	1856	1862	1865	rBV3	484	498	0.03%	0.004%
43	7.565	1919	1936	1959	rBV	168062	302141	17.37%	2.398%
44	7.693	1973	1976	1979	rBV2	693	560	0.03%	0.004%
45	7.790	2001	2006	2008	rBV2	827	721	0.04%	0.006%
46	7.896	2026	2039	2057	rBV	696770	1199353	68.95%	9.520%
47	8.028	2078	2080	2084	rVB4	1195	758	0.04%	0.006%
48	8.050	2084	2087	2090	rVB4	432	308	0.02%	0.002%
49	8.089	2095	2099	2103	rVB3	768	805	0.05%	0.006%
50	8.115	2103	2107	2112	rBV3	409	385	0.02%	0.003%
51	8.179	2112	2127	2143	rBV	121583	206273	11.86%	1.637%
52	8.388	2188	2192	2194	rBV2	394	293	0.02%	0.002%
53	8.420	2199	2202	2206	rVB2	647	398	0.02%	0.003%
54	8.459	2209	2214	2217	rBV3	339	323	0.02%	0.003%
55	8.555	2236	2244	2249	rBV3	975	1192	0.07%	0.009%
56	8.632	2255	2268	2301	rBV3	434906	969047	55.71%	7.692%
57	8.841	2331	2333	2336	rVB3	897	375	0.02%	0.003%
58	8.857	2336	2338	2341	rBV3	649	402	0.02%	0.003%
59	8.906	2349	2353	2358	rBV3	407	419	0.02%	0.003%
60	9.124	2417	2421	2423	rBV3	532	374	0.02%	0.003%
61	9.169	2433	2435	2438	rVB3	634	332	0.02%	0.003%
62	9.237	2450	2456	2460	rVB2	351	327	0.02%	0.003%
63	9.417	2498	2512	2545	rBV	703611	1170718	67.30%	9.293%
64	9.597	2566	2568	2571	rVB3	697	379	0.02%	0.003%
65	9.648	2579	2584	2587	rBV3	547	523	0.03%	0.004%
66	9.700	2595	2600	2601	rBV	658	571	0.03%	0.005%
67	9.819	2633	2637	2641	rBV2	518	391	0.02%	0.003%
68	10.092	2716	2722	2725	rBV3	503	504	0.03%	0.004%
69	10.111	2725	2728	2731	rVV2	547	436	0.03%	0.003%
70	10.127	2731	2733	2738	rVB3	477	389	0.02%	0.003%
71	10.491	2840	2846	2851	rVB2	815	888	0.05%	0.007%
72	10.639	2889	2892	2898	rBV3	536	661	0.04%	0.005%
73	10.700	2907	2911	2915	rBV2	401	370	0.02%	0.003%
74	10.754	2915	2928	2948	rBV	640791	1018156	58.53%	8.082%
75	11.037	3013	3016	3019	rBV	663	476	0.03%	0.004%
76	11.111	3036	3039	3044	rVB3	578	613	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
 Data File : VU051118.D
 Acq On : 05 Oct 2022 11:41
 Operator : JC/MD
 Sample : N4880-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	11.211	3067	3070	3077	rVB2	321	308	0.02%	0.002%
78	11.471	3147	3151	3152	rBV	498	284	0.02%	0.002%
79	11.713	3220	3226	3230	rBV2	577	641	0.04%	0.005%
80	11.738	3230	3234	3239	rBV3	835	856	0.05%	0.007%
81	11.812	3244	3257	3284	rBV	522327	840450	48.32%	6.671%
82	11.928	3291	3293	3296	rBV2	470	324	0.02%	0.003%
83	11.999	3309	3315	3319	rVB5	557	559	0.03%	0.004%
84	12.079	3333	3340	3344	rBV3	368	466	0.03%	0.004%
85	12.192	3362	3375	3398	rBV	602129	990447	56.94%	7.862%
86	12.735	3541	3544	3546	rBV2	457	273	0.02%	0.002%
87	12.790	3557	3561	3565	rBV3	475	490	0.03%	0.004%
88	12.883	3588	3590	3594	rVB2	493	289	0.02%	0.002%
89	12.979	3617	3620	3625	rVV3	477	392	0.02%	0.003%
90	13.041	3637	3639	3646	rVB2	646	627	0.04%	0.005%
91	13.086	3650	3653	3657	rBV2	876	627	0.04%	0.005%
92	13.658	3828	3831	3834	rBV2	415	281	0.02%	0.002%
93	13.844	3885	3889	3890	rBV2	1211	766	0.04%	0.006%
94	14.336	4035	4042	4044	rBV3	1326	1511	0.09%	0.012%
95	14.915	4220	4222	4224	rBV	589	320	0.02%	0.003%
96	14.938	4227	4229	4231	rVB3	657	320	0.02%	0.003%
97	15.066	4266	4269	4271	rBV4	656	477	0.03%	0.004%
98	15.192	4305	4308	4312	rBV3	697	582	0.03%	0.005%
99	15.298	4338	4341	4346	rBV4	843	724	0.04%	0.006%
100	15.471	4391	4395	4401	rBV7	832	971	0.06%	0.008%




Sum of corrected areas: 12597774

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
Data File : VU051118.D
Acq On : 05 Oct 2022 11:41
Operator : JC/MD
Sample : N4880-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

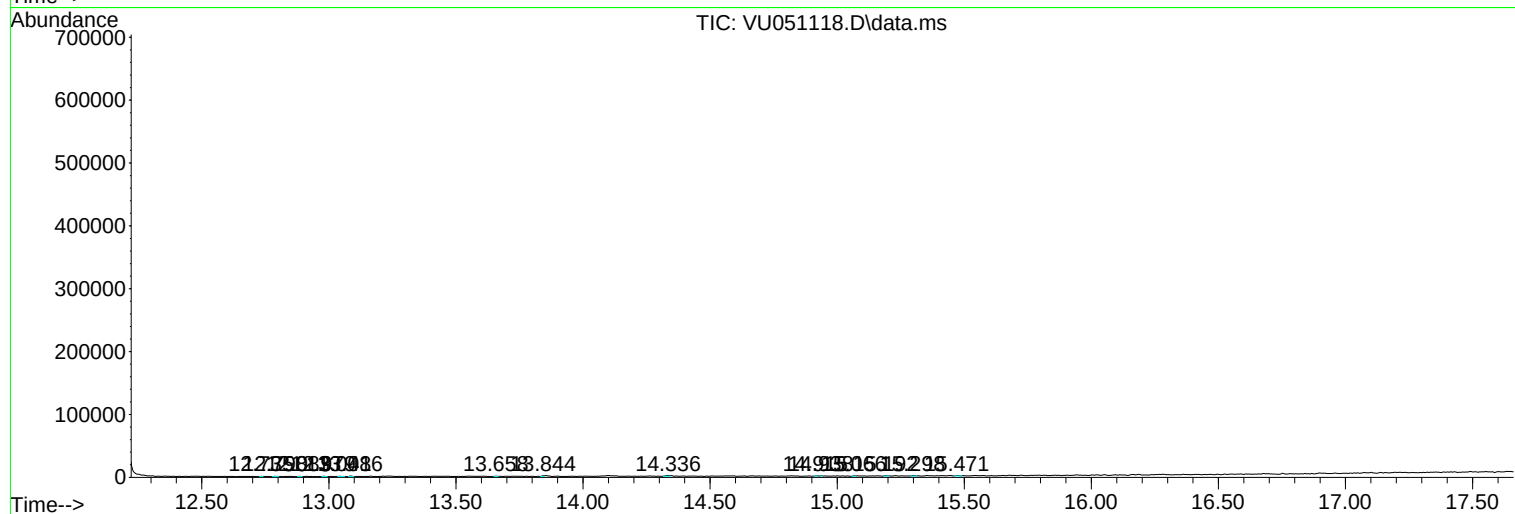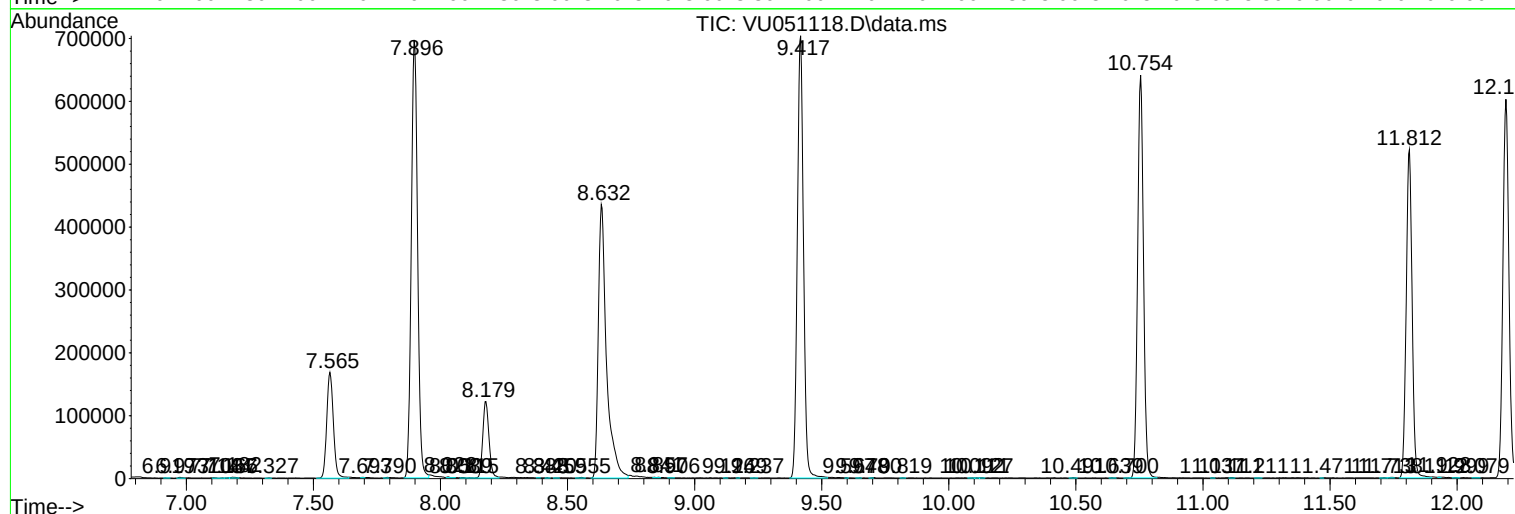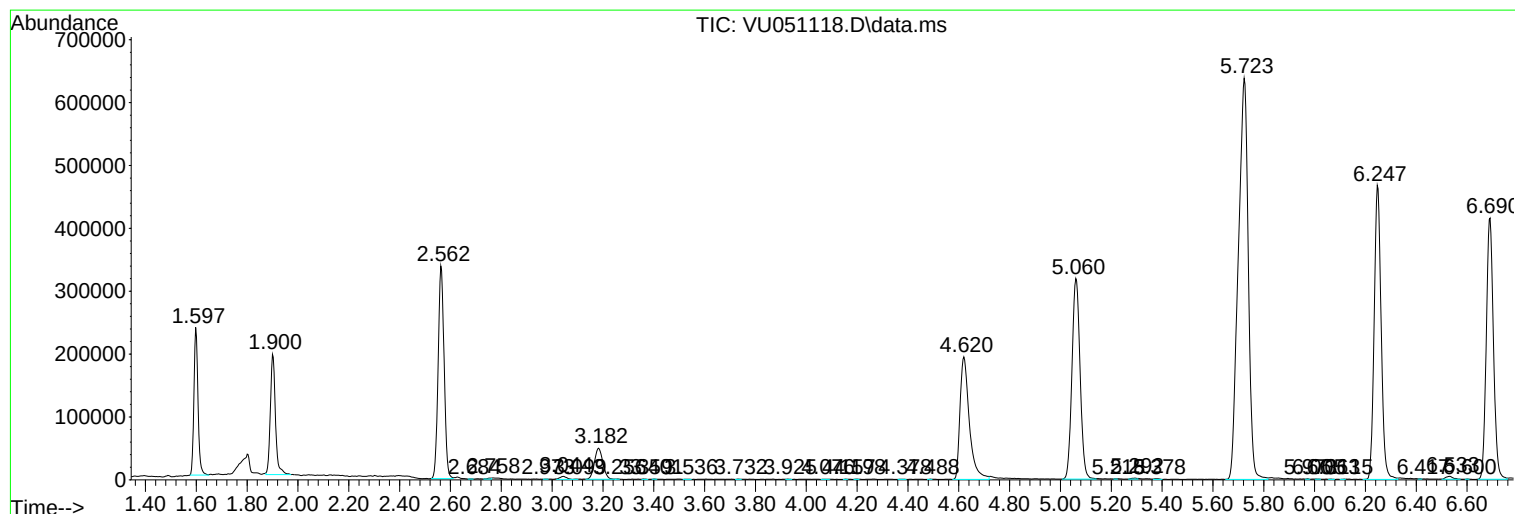

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
Data File : VU051118.D
Acq On : 05 Oct 2022 11:41
Operator : JC/MD
Sample : N4880-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
Data File : VU051118.D
Acq On : 05 Oct 2022 11:41
Operator : JC/MD
Sample : N4880-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc