

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
 Data File : VU051119.D
 Acq On : 05 Oct 2022 12:04
 Operator : JC/MD
 Sample : N4854-15
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

Signal : TIC: VU051119.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	94	rBV	237777	266324	15.37%	2.187%
2	1.899	166	174	193	rVB	194076	260068	15.01%	2.135%
3	2.562	368	380	399	rBV	335018	547705	31.61%	4.497%
4	3.041	521	529	540	rVB3	4450	7775	0.45%	0.064%
5	3.446	652	655	661	rVB2	429	458	0.03%	0.004%
6	3.517	676	677	678	rBV2	268	94	0.01%	0.001%
7	3.568	689	693	697	rBV3	272	273	0.02%	0.002%
8	3.597	697	702	706	rBV2	425	483	0.03%	0.004%
9	3.703	733	735	738	rVB2	371	146	0.01%	0.001%
10	3.745	745	748	749	rBV	171	73	0.00%	0.001%
11	3.758	749	752	757	rVB3	208	190	0.01%	0.002%
12	3.935	804	807	810	rBV	199	139	0.01%	0.001%
13	3.970	816	818	822	rVB2	305	173	0.01%	0.001%
14	3.993	822	825	828	rBV	276	169	0.01%	0.001%
15	4.015	828	832	836	rBV3	435	490	0.03%	0.004%
16	4.054	841	844	847	rVB	328	167	0.01%	0.001%
17	4.089	851	855	861	rBV2	388	434	0.03%	0.004%
18	4.118	861	864	866	rBV2	253	166	0.01%	0.001%
19	4.150	871	874	879	rBV2	248	215	0.01%	0.002%
20	4.195	885	888	890	rBV2	279	173	0.01%	0.001%
21	4.250	902	905	907	rVB	150	66	0.00%	0.001%
22	4.308	920	923	924	rBV	126	79	0.00%	0.001%
23	4.321	924	927	931	rVV3	410	344	0.02%	0.003%
24	4.378	943	945	951	rVB	260	186	0.01%	0.002%
25	4.433	960	962	964	rBV	252	124	0.01%	0.001%
26	4.449	964	967	969	rBV	204	131	0.01%	0.001%
27	4.491	977	980	985	rVB2	136	85	0.00%	0.001%
28	4.523	985	990	993	rBV2	319	321	0.02%	0.003%
29	4.571	1002	1005	1007	rBV2	227	154	0.01%	0.001%
30	4.620	1007	1020	1059	rBV	176772	454051	26.20%	3.728%
31	5.060	1141	1157	1179	rBV	323623	704484	40.65%	5.785%
32	5.372	1248	1254	1263	rBV5	836	1464	0.08%	0.012%
33	5.423	1268	1270	1276	rVB2	158	134	0.01%	0.001%
34	5.485	1286	1289	1291	rBV	308	168	0.01%	0.001%
35	5.523	1300	1301	1303	rBV	183	50	0.00%	0.000%
36	5.549	1306	1309	1311	rBV	309	205	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
 Data File : VU051119.D
 Acq On : 05 Oct 2022 12:04
 Operator : JC/MD
 Sample : N4854-15
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	5.565	1311	1314	1320	rVB2	346	335	0.02%	0.003%
38	5.604	1324	1326	1331	rVB3	183	120	0.01%	0.001%
39	5.629	1331	1334	1339	rBV2	360	233	0.01%	0.002%
40	5.722	1339	1363	1384	rBV2	639987	1732868	100.00%	14.229%
41	6.044	1460	1463	1472	rBV3	442	524	0.03%	0.004%
42	6.095	1476	1479	1483	rBV2	587	447	0.03%	0.004%
43	6.121	1484	1487	1493	rVB4	467	384	0.02%	0.003%
44	6.157	1496	1498	1501	rVB	264	109	0.01%	0.001%
45	6.173	1501	1503	1504	rBV	65	26	0.00%	0.000%
46	6.185	1505	1507	1511	rVB2	327	188	0.01%	0.002%
47	6.247	1511	1526	1545	rBV	451695	856369	49.42%	7.032%
48	6.526	1605	1613	1625	rVB7	4511	8447	0.49%	0.069%
49	6.594	1631	1634	1637	rVV3	662	419	0.02%	0.003%
50	6.610	1637	1639	1641	rVB	271	94	0.01%	0.001%
51	6.687	1646	1663	1683	rBV	412004	812703	46.90%	6.673%
52	6.896	1725	1728	1731	rBV2	279	151	0.01%	0.001%
53	6.941	1736	1742	1744	rBV2	255	258	0.01%	0.002%
54	6.980	1750	1754	1757	rBV2	437	380	0.02%	0.003%
55	7.034	1769	1771	1774	rBV2	299	209	0.01%	0.002%
56	7.066	1779	1781	1782	rBV2	61	26	0.00%	0.000%
57	7.083	1782	1786	1789	rBV2	332	256	0.01%	0.002%
58	7.179	1812	1816	1818	rBV3	813	745	0.04%	0.006%
59	7.266	1840	1843	1846	rBV2	247	179	0.01%	0.001%
60	7.282	1846	1848	1851	rBV	190	112	0.01%	0.001%
61	7.324	1858	1861	1866	rVB2	297	228	0.01%	0.002%
62	7.365	1870	1874	1878	rBV	274	260	0.02%	0.002%
63	7.423	1890	1892	1893	rBV	282	126	0.01%	0.001%
64	7.468	1903	1906	1909	rBV2	148	123	0.01%	0.001%
65	7.565	1923	1936	1953	rBV	166998	294554	17.00%	2.419%
66	7.748	1987	1993	1999	rBV3	440	583	0.03%	0.005%
67	7.896	2025	2039	2058	rBV	697342	1199879	69.24%	9.852%
68	8.179	2115	2127	2144	rBV	122945	208190	12.01%	1.709%
69	8.359	2180	2183	2185	rBV2	470	346	0.02%	0.003%
70	8.507	2228	2229	2232	rBV2	232	109	0.01%	0.001%
71	8.523	2232	2234	2235	rBV	313	118	0.01%	0.001%
72	8.549	2239	2242	2247	rBV4	734	747	0.04%	0.006%
73	8.632	2256	2268	2313	rBV3	413616	942830	54.41%	7.742%
74	8.931	2359	2361	2364	rBV	507	252	0.01%	0.002%
75	8.996	2379	2381	2384	rBV	316	231	0.01%	0.002%
76	9.095	2409	2412	2414	rBV2	381	262	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
 Data File : VU051119.D
 Acq On : 05 Oct 2022 12:04
 Operator : JC/MD
 Sample : N4854-15
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	9.144	2424	2427	2430	rBV2	398	232	0.01%	0.002%
78	9.192	2440	2442	2445	rVB	224	114	0.01%	0.001%
79	9.234	2453	2455	2456	rBV	237	108	0.01%	0.001%
80	9.349	2488	2491	2498	rVB	383	423	0.02%	0.003%
81	9.417	2498	2512	2533	rBV	678879	1112746	64.21%	9.137%
82	9.562	2555	2557	2558	rBV	445	142	0.01%	0.001%
83	9.681	2591	2594	2595	rBV2	470	248	0.01%	0.002%
84	10.234	2762	2766	2768	rBV2	278	224	0.01%	0.002%
85	10.291	2781	2784	2787	rBV2	372	290	0.02%	0.002%
86	10.529	2852	2858	2862	rBV2	294	366	0.02%	0.003%
87	10.555	2862	2866	2869	rBV	372	315	0.02%	0.003%
88	10.754	2915	2928	2948	rBV	617897	992249	57.26%	8.148%
89	10.909	2974	2976	2980	rVB3	683	444	0.03%	0.004%
90	10.931	2980	2983	2985	rBV	347	230	0.01%	0.002%
91	11.169	3054	3057	3062	rBV	548	404	0.02%	0.003%
92	11.809	3244	3256	3275	rBV	495973	789602	45.57%	6.484%
93	12.192	3362	3375	3403	rBV	588174	967531	55.83%	7.945%
94	12.590	3496	3499	3502	rBV2	453	274	0.02%	0.002%
95	12.606	3502	3504	3505	rBV	426	211	0.01%	0.002%
96	12.696	3530	3532	3535	rBV	491	205	0.01%	0.002%




Sum of corrected areas: 12178539

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
Data File : VU051119.D
Acq On : 05 Oct 2022 12:04
Operator : JC/MD
Sample : N4854-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

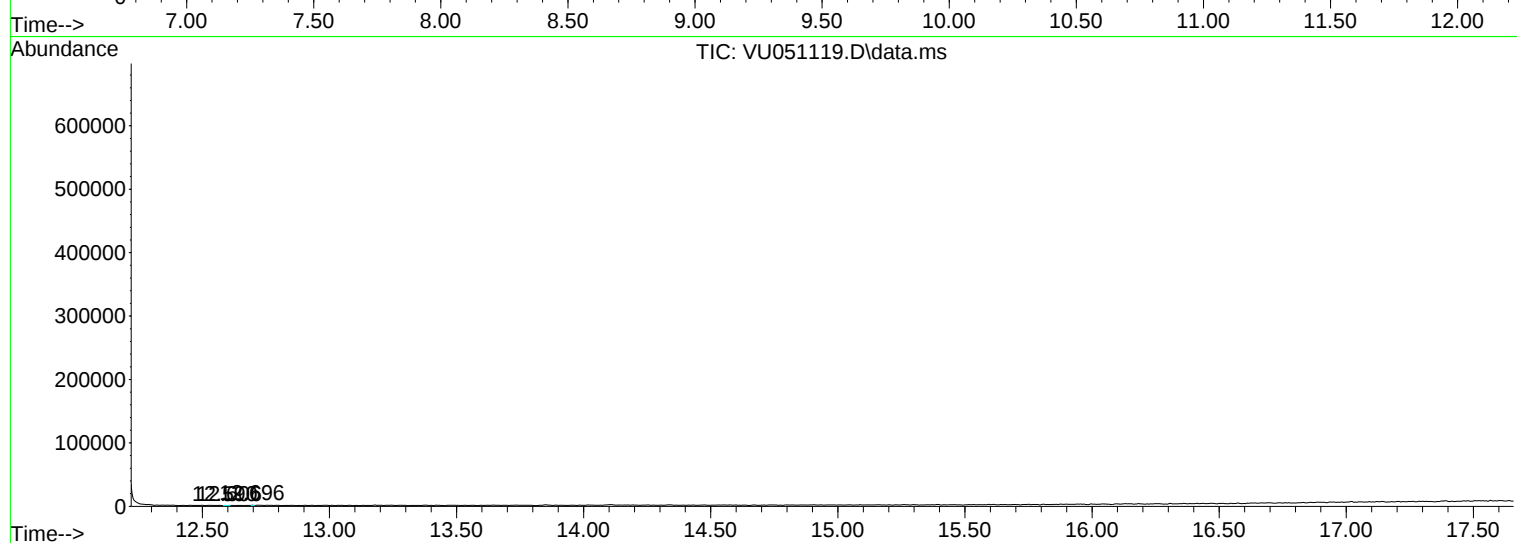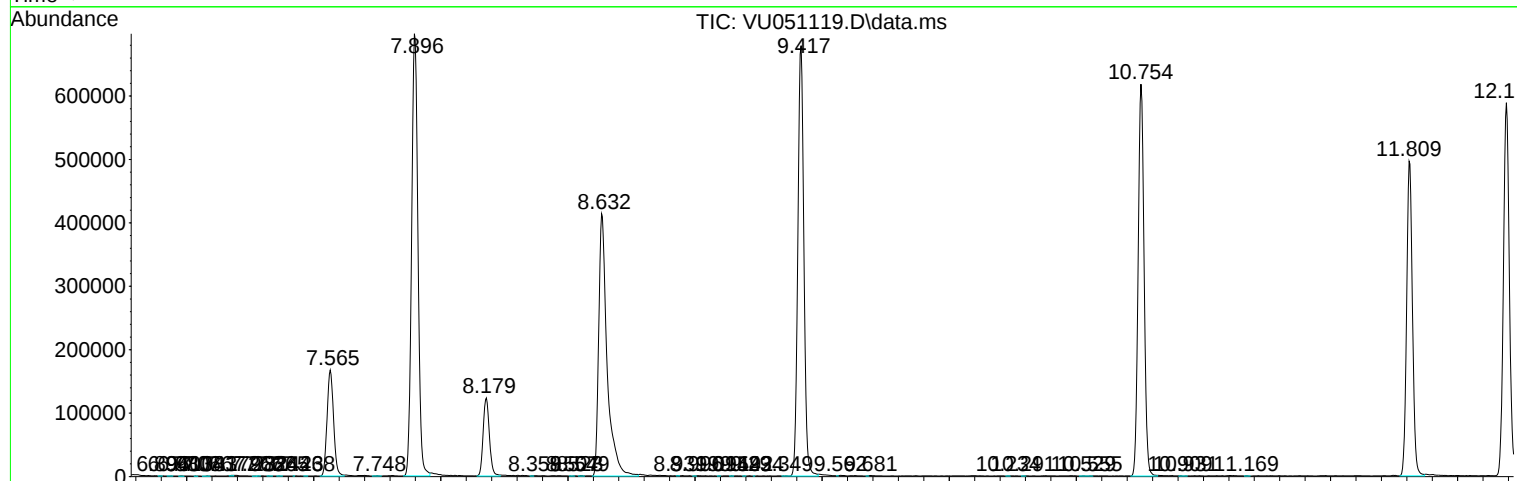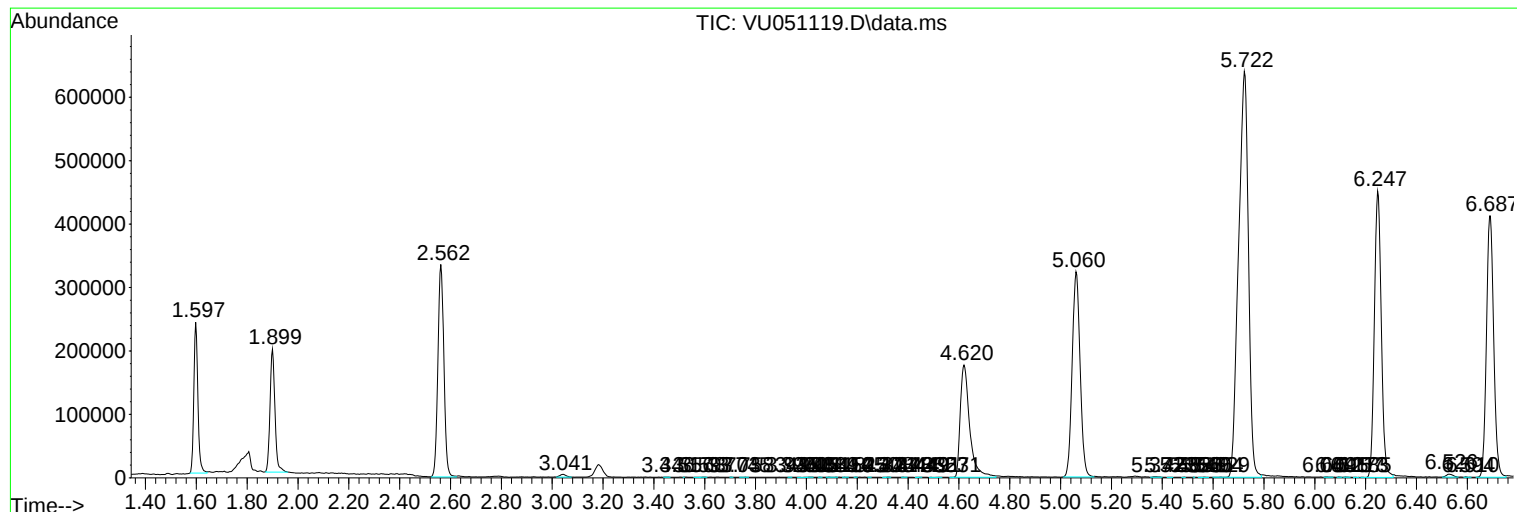

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
Data File : VU051119.D
Acq On : 05 Oct 2022 12:04
Operator : JC/MD
Sample : N4854-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
Data File : VU051119.D
Acq On : 05 Oct 2022 12:04
Operator : JC/MD
Sample : N4854-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc