

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
 Data File : VU051120.D
 Acq On : 05 Oct 2022 12:28
 Operator : JC/MD
 Sample : N4853-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW825

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

Signal : TIC: VU051120.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	93	rBV	224099	246344	14.82%	2.102%
2	1.900	166	174	192	rVB	184417	247580	14.90%	2.112%
3	2.562	368	380	397	rBV	312208	507129	30.51%	4.327%
4	2.713	424	427	429	rBV2	594	340	0.02%	0.003%
5	2.784	446	449	461	rVB4	1395	1998	0.12%	0.017%
6	2.838	461	466	469	rBV3	396	366	0.02%	0.003%
7	2.954	497	502	507	rBV2	472	608	0.04%	0.005%
8	3.044	518	530	541	rBV3	9944	18219	1.10%	0.155%
9	3.102	545	548	551	rVB	469	270	0.02%	0.002%
10	3.186	564	574	578	rBV3	1603	2654	0.16%	0.023%
11	3.279	599	603	608	rVB2	398	426	0.03%	0.004%
12	3.305	608	611	615	rBV2	350	311	0.02%	0.003%
13	3.411	639	644	650	rBV3	271	310	0.02%	0.003%
14	3.459	653	659	663	rBV2	464	440	0.03%	0.004%
15	3.726	733	742	746	rBV	326	562	0.03%	0.005%
16	3.941	807	809	816	rVB2	455	400	0.02%	0.003%
17	3.983	816	822	825	rBV2	278	294	0.02%	0.003%
18	4.224	895	897	903	rVB2	385	280	0.02%	0.002%
19	4.504	978	984	988	rBV3	251	312	0.02%	0.003%
20	4.620	1004	1020	1051	rBV	160862	409823	24.66%	3.497%
21	4.967	1126	1128	1133	rVB2	534	261	0.02%	0.002%
22	5.060	1139	1157	1179	rBV	309202	676084	40.68%	5.769%
23	5.211	1202	1204	1209	rVB3	613	468	0.03%	0.004%
24	5.272	1218	1223	1225	rBV3	788	747	0.04%	0.006%
25	5.292	1225	1229	1237	rVV4	1859	2123	0.13%	0.018%
26	5.327	1237	1240	1245	rVB4	455	474	0.03%	0.004%
27	5.369	1248	1253	1258	rBV4	727	1080	0.06%	0.009%
28	5.395	1258	1261	1266	rVV4	495	394	0.02%	0.003%
29	5.520	1298	1300	1305	rVB2	513	362	0.02%	0.003%
30	5.549	1305	1309	1312	rBV	406	258	0.02%	0.002%
31	5.723	1341	1363	1396	rBV2	606600	1662146	100.00%	14.182%
32	5.973	1439	1441	1450	rVB4	798	899	0.05%	0.008%
33	6.044	1460	1463	1464	rBV	436	261	0.02%	0.002%
34	6.115	1481	1485	1489	rBV2	557	537	0.03%	0.005%
35	6.150	1494	1496	1499	rBV2	388	274	0.02%	0.002%
36	6.247	1512	1526	1548	rBV	454908	858056	51.62%	7.321%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
 Data File : VU051120.D
 Acq On : 05 Oct 2022 12:28
 Operator : JC/MD
 Sample : N4853-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW825

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	6.469	1592	1595	1601	rVB2	375	258	0.02%	0.002%
38	6.523	1605	1612	1614	rBV6	3273	3846	0.23%	0.033%
39	6.607	1635	1638	1644	rVB4	652	624	0.04%	0.005%
40	6.687	1644	1663	1685	rBV	397476	784234	47.18%	6.692%
41	6.845	1710	1712	1717	rVB3	519	401	0.02%	0.003%
42	7.112	1793	1795	1798	rBV3	511	338	0.02%	0.003%
43	7.182	1812	1817	1818	rBV3	921	678	0.04%	0.006%
44	7.398	1877	1884	1889	rBV2	375	569	0.03%	0.005%
45	7.443	1894	1898	1901	rBV	304	269	0.02%	0.002%
46	7.510	1911	1919	1922	rBV	366	417	0.03%	0.004%
47	7.565	1923	1936	1954	rBV	161010	284339	17.11%	2.426%
48	7.655	1960	1964	1968	rBV3	552	438	0.03%	0.004%
49	7.694	1971	1976	1979	rBV4	1208	1111	0.07%	0.009%
50	7.793	2005	2007	2013	rVB2	734	547	0.03%	0.005%
51	7.896	2022	2039	2061	rBV	655627	1134253	68.24%	9.678%
52	8.118	2105	2108	2112	rVB3	471	344	0.02%	0.003%
53	8.179	2112	2127	2147	rBV	115878	196915	11.85%	1.680%
54	8.475	2217	2219	2225	rBV2	403	329	0.02%	0.003%
55	8.549	2238	2242	2243	rBV2	1027	706	0.04%	0.006%
56	8.636	2256	2269	2308	rBV2	380215	877184	52.77%	7.485%
57	8.848	2331	2335	2340	rBV4	890	852	0.05%	0.007%
58	8.931	2357	2361	2364	rBV2	521	320	0.02%	0.003%
59	8.986	2374	2378	2381	rBV3	361	279	0.02%	0.002%
60	9.018	2386	2388	2391	rVB	589	311	0.02%	0.003%
61	9.182	2435	2439	2442	rBV	477	411	0.02%	0.004%
62	9.240	2454	2457	2465	rVB2	407	438	0.03%	0.004%
63	9.276	2465	2468	2470	rBV	397	288	0.02%	0.002%
64	9.417	2498	2512	2535	rBV	669094	1112844	66.95%	9.495%
65	9.642	2577	2582	2585	rBV2	538	406	0.02%	0.003%
66	9.693	2593	2598	2602	rVB4	793	924	0.06%	0.008%
67	9.729	2602	2609	2612	rBV2	467	393	0.02%	0.003%
68	9.812	2631	2635	2637	rBV	370	313	0.02%	0.003%
69	9.890	2654	2659	2661	rBV2	304	260	0.02%	0.002%
70	10.028	2699	2702	2707	rVB2	403	321	0.02%	0.003%
71	10.054	2707	2710	2720	rVB2	303	475	0.03%	0.004%
72	10.095	2720	2723	2726	rBV2	488	389	0.02%	0.003%
73	10.157	2738	2742	2745	rBV2	516	344	0.02%	0.003%
74	10.269	2774	2777	2785	rVB2	332	362	0.02%	0.003%
75	10.600	2876	2880	2883	rBV2	357	332	0.02%	0.003%
76	10.648	2889	2895	2902	rVB2	701	750	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
 Data File : VU051120.D
 Acq On : 05 Oct 2022 12:28
 Operator : JC/MD
 Sample : N4853-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW825

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	10.755	2914	2928	2951	rBV	580565	937774	56.42%	8.002%
78	10.893	2965	2971	2979	rVB4	561	739	0.04%	0.006%
79	11.025	3008	3012	3018	rVB3	328	352	0.02%	0.003%
80	11.086	3027	3031	3034	rBV3	611	507	0.03%	0.004%
81	11.407	3123	3131	3136	rBV4	815	1070	0.06%	0.009%
82	11.529	3166	3169	3172	rBV	501	277	0.02%	0.002%
83	11.751	3234	3238	3244	rVB3	674	728	0.04%	0.006%
84	11.809	3244	3256	3279	rBV	484030	774258	46.58%	6.606%
85	11.980	3306	3309	3312	rBV2	353	276	0.02%	0.002%
86	12.063	3326	3335	3356	rBV4	16473	34643	2.08%	0.296%
87	12.192	3362	3375	3396	rBV	565068	911353	54.83%	7.776%
88	12.703	3528	3534	3537	rVB4	744	797	0.05%	0.007%
89	12.729	3537	3542	3544	rBV3	575	463	0.03%	0.004%
90	12.947	3606	3610	3613	rBV	640	531	0.03%	0.005%
91	12.999	3623	3626	3628	rBV2	554	367	0.02%	0.003%
92	13.140	3667	3670	3675	rBV3	352	381	0.02%	0.003%
93	13.221	3691	3695	3700	rVB2	1043	881	0.05%	0.008%
94	13.266	3707	3709	3712	rVB3	527	278	0.02%	0.002%
95	13.359	3735	3738	3740	rBV	557	343	0.02%	0.003%
96	13.375	3740	3743	3746	rVB2	657	434	0.03%	0.004%
97	13.465	3767	3771	3773	rBV3	520	396	0.02%	0.003%
98	13.639	3822	3825	3827	rBV2	465	321	0.02%	0.003%
99	13.751	3857	3860	3861	rBV	509	306	0.02%	0.003%
100	14.307	4031	4033	4037	rBV2	529	390	0.02%	0.003%




Sum of corrected areas: 11719767

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
Data File : VU051120.D
Acq On : 05 Oct 2022 12:28
Operator : JC/MD
Sample : N4853-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW825

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

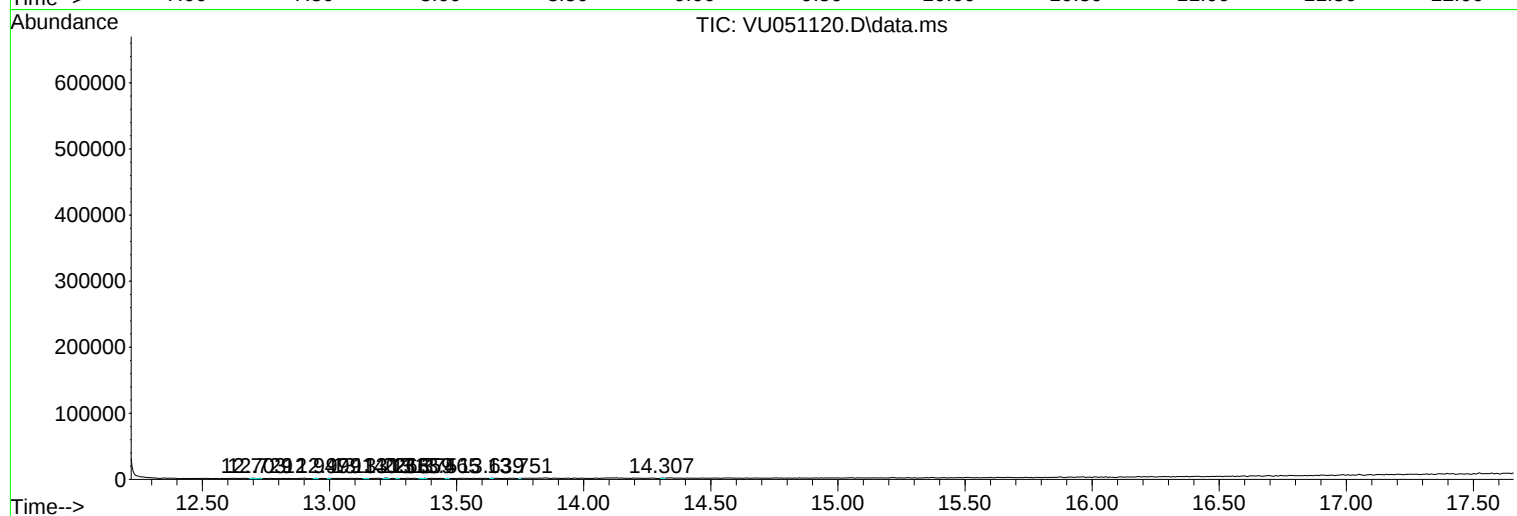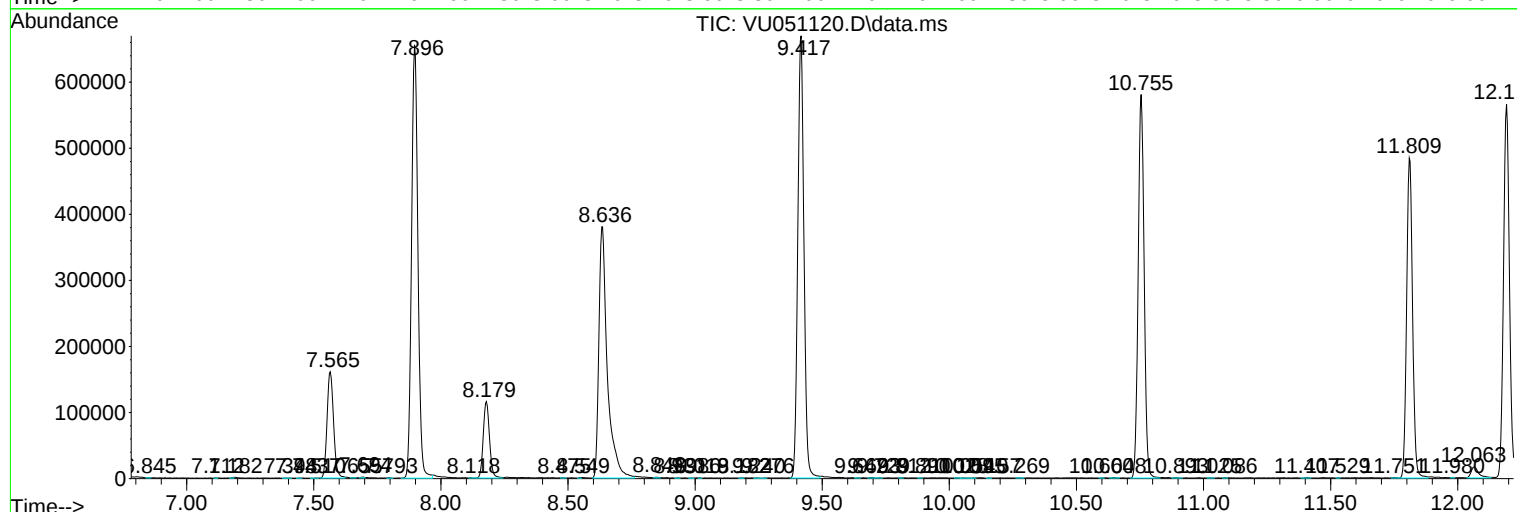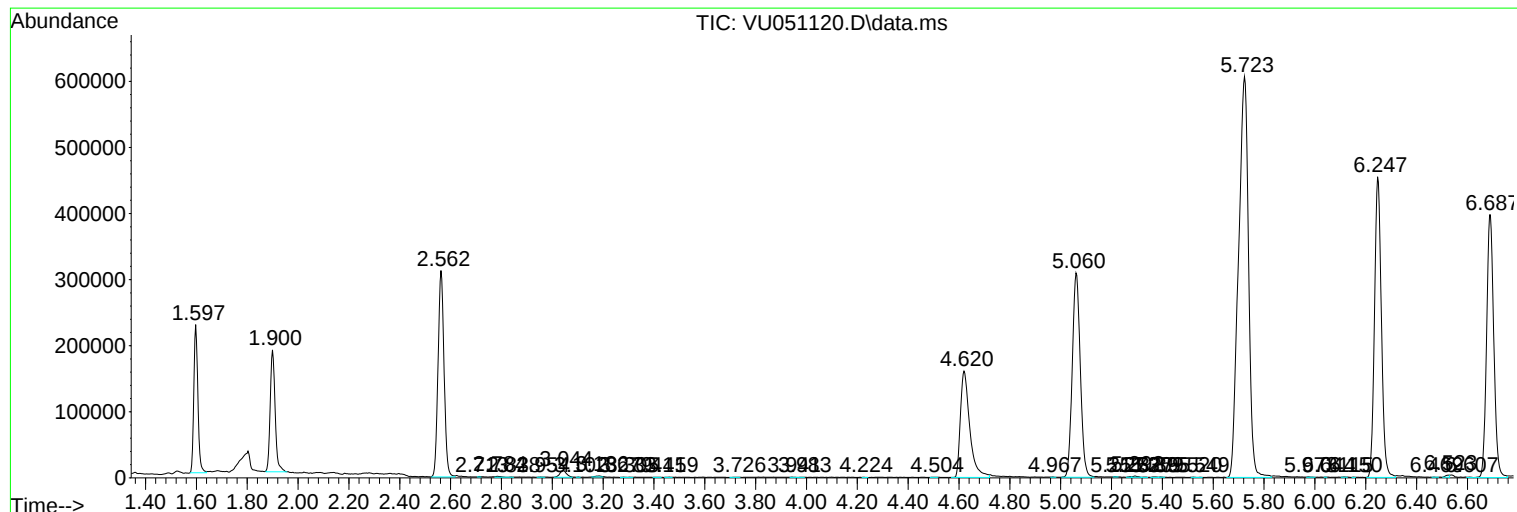

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
Data File : VU051120.D
Acq On : 05 Oct 2022 12:28
Operator : JC/MD
Sample : N4853-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW825

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
Data File : VU051120.D
Acq On : 05 Oct 2022 12:28
Operator : JC/MD
Sample : N4853-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW825

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc