

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
 Data File : VU051122.D
 Acq On : 05 Oct 2022 13:15
 Operator : JC/MD
 Sample : N4853-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW840

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

Signal : TIC: VU051122.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	99	rBV	220893	257139	15.67%	2.200%
2	1.896	165	173	195	rVB	182574	250088	15.24%	2.139%
3	2.559	367	379	395	rBV	308544	508002	30.95%	4.345%
4	2.777	445	447	451	rBV2	472	400	0.02%	0.003%
5	2.961	501	504	507	rBV3	374	269	0.02%	0.002%
6	2.986	507	512	515	rVV3	424	411	0.03%	0.004%
7	3.038	518	528	541	rVV4	9606	18411	1.12%	0.157%
8	3.273	597	601	605	rVB2	330	319	0.02%	0.003%
9	3.295	605	608	611	rBV2	467	287	0.02%	0.002%
10	3.324	613	617	621	rVB4	548	471	0.03%	0.004%
11	3.356	621	627	629	rBV2	351	349	0.02%	0.003%
12	3.465	658	661	666	rBV2	335	277	0.02%	0.002%
13	3.646	714	717	722	rBV2	428	380	0.02%	0.003%
14	3.816	764	770	774	rBV2	348	430	0.03%	0.004%
15	3.935	803	807	811	rBV	354	308	0.02%	0.003%
16	4.099	852	858	864	rBV2	443	474	0.03%	0.004%
17	4.192	883	887	893	rBV2	302	312	0.02%	0.003%
18	4.369	938	942	947	rVB2	258	296	0.02%	0.003%
19	4.401	947	952	956	rBV2	298	327	0.02%	0.003%
20	4.620	1008	1020	1057	rBV	160656	413016	25.16%	3.533%
21	4.813	1076	1080	1085	rVB4	503	529	0.03%	0.005%
22	5.060	1140	1157	1182	rBV	307937	677678	41.29%	5.797%
23	5.289	1224	1228	1233	rBV6	1047	1093	0.07%	0.009%
24	5.388	1257	1259	1263	rVB3	946	614	0.04%	0.005%
25	5.417	1263	1268	1270	rBV2	354	382	0.02%	0.003%
26	5.436	1271	1274	1279	rVB2	450	412	0.03%	0.004%
27	5.588	1319	1321	1326	rVB2	336	288	0.02%	0.002%
28	5.723	1342	1363	1386	rBV2	605361	1641247	100.00%	14.039%
29	6.041	1459	1462	1466	rBV2	522	405	0.02%	0.003%
30	6.115	1481	1485	1487	rBV2	507	454	0.03%	0.004%
31	6.247	1511	1526	1554	rBV	445673	851400	51.88%	7.283%
32	6.395	1570	1572	1574	rBV3	853	470	0.03%	0.004%
33	6.530	1603	1614	1625	rVB9	3532	8040	0.49%	0.069%
34	6.584	1628	1631	1632	rBV	617	304	0.02%	0.003%
35	6.613	1637	1640	1642	rVB2	647	362	0.02%	0.003%
36	6.687	1647	1663	1688	rBV	398941	785437	47.86%	6.719%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
 Data File : VU051122.D
 Acq On : 05 Oct 2022 13:15
 Operator : JC/MD
 Sample : N4853-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW840

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	6.941	1739	1742	1745	rBV2	346	312	0.02%	0.003%
38	6.977	1751	1753	1757	rVB2	387	287	0.02%	0.002%
39	7.009	1757	1763	1769	rVB2	486	554	0.03%	0.005%
40	7.073	1779	1783	1786	rVB	467	288	0.02%	0.002%
41	7.105	1789	1793	1800	rVB3	489	610	0.04%	0.005%
42	7.144	1800	1805	1807	rBV2	319	274	0.02%	0.002%
43	7.308	1853	1856	1860	rBV3	276	262	0.02%	0.002%
44	7.411	1882	1888	1891	rBV2	296	358	0.02%	0.003%
45	7.485	1907	1911	1914	rBV2	367	305	0.02%	0.003%
46	7.565	1922	1936	1956	rBV	158277	283150	17.25%	2.422%
47	7.700	1976	1978	1984	rVB3	944	567	0.03%	0.005%
48	7.758	1993	1996	2000	rBV2	663	503	0.03%	0.004%
49	7.787	2000	2005	2006	rBV3	381	315	0.02%	0.003%
50	7.896	2025	2039	2060	rBV	653149	1130647	68.89%	9.672%
51	8.179	2115	2127	2145	rBV2	114211	195383	11.90%	1.671%
52	8.243	2145	2147	2154	rVB4	1083	941	0.06%	0.008%
53	8.346	2177	2179	2184	rVB3	644	473	0.03%	0.004%
54	8.385	2188	2191	2196	rVV2	372	371	0.02%	0.003%
55	8.510	2227	2230	2233	rVB2	440	341	0.02%	0.003%
56	8.549	2234	2242	2251	rBV7	4328	7252	0.44%	0.062%
57	8.632	2256	2268	2304	rBV2	389459	886092	53.99%	7.580%
58	8.935	2358	2362	2365	rBV2	534	397	0.02%	0.003%
59	9.076	2402	2406	2411	rBV2	505	499	0.03%	0.004%
60	9.166	2432	2434	2439	rBV2	559	453	0.03%	0.004%
61	9.340	2481	2488	2491	rBV2	479	397	0.02%	0.003%
62	9.417	2499	2512	2537	rBV	664528	1095667	66.76%	9.372%
63	9.607	2567	2571	2576	rVB3	667	668	0.04%	0.006%
64	9.639	2576	2581	2586	rBV3	822	777	0.05%	0.007%
65	9.684	2591	2595	2597	rBV	498	321	0.02%	0.003%
66	9.957	2678	2680	2686	rVV2	333	337	0.02%	0.003%
67	10.102	2721	2725	2729	rVB3	952	793	0.05%	0.007%
68	10.124	2729	2732	2734	rBV2	439	306	0.02%	0.003%
69	10.150	2737	2740	2745	rVV2	247	257	0.02%	0.002%
70	10.378	2807	2811	2814	rBV2	420	311	0.02%	0.003%
71	10.478	2840	2842	2849	rVB3	533	507	0.03%	0.004%
72	10.623	2883	2887	2890	rBV	355	317	0.02%	0.003%
73	10.645	2890	2894	2895	rBV2	932	612	0.04%	0.005%
74	10.755	2915	2928	2949	rBV	587228	949848	57.87%	8.125%
75	10.893	2968	2971	2977	rVB4	894	822	0.05%	0.007%
76	11.041	3015	3017	3022	rVB	429	283	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
 Data File : VU051122.D
 Acq On : 05 Oct 2022 13:15
 Operator : JC/MD
 Sample : N4853-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW840

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	11.092	3031	3033	3036	rBV2	394	268	0.02%	0.002%
78	11.295	3090	3096	3100	rVV2	407	461	0.03%	0.004%
79	11.337	3106	3109	3114	rVB	599	405	0.02%	0.003%
80	11.472	3148	3151	3155	rVV3	493	386	0.02%	0.003%
81	11.565	3176	3180	3184	rBV2	283	282	0.02%	0.002%
82	11.742	3231	3235	3239	rBV3	492	519	0.03%	0.004%
83	11.809	3244	3256	3281	rBV	484158	773537	47.13%	6.617%
84	11.919	3288	3290	3293	rBV2	570	301	0.02%	0.003%
85	12.018	3318	3321	3327	rBV4	372	401	0.02%	0.003%
86	12.066	3328	3336	3349	rBV4	6346	12182	0.74%	0.104%
87	12.192	3362	3375	3396	rBV	555273	912353	55.59%	7.804%
88	12.388	3433	3436	3439	rBV2	371	305	0.02%	0.003%
89	12.629	3507	3511	3515	rBV3	506	494	0.03%	0.004%
90	12.690	3528	3530	3535	rVB	527	300	0.02%	0.003%
91	12.812	3562	3568	3571	rBV3	693	735	0.04%	0.006%
92	13.086	3651	3653	3657	rBV2	425	307	0.02%	0.003%
93	13.127	3661	3666	3671	rBV2	621	677	0.04%	0.006%
94	13.324	3724	3727	3729	rBV2	491	328	0.02%	0.003%
95	13.555	3795	3799	3800	rBV	465	319	0.02%	0.003%
96	13.963	3923	3926	3928	rBV3	428	321	0.02%	0.003%
97	14.189	3992	3996	3997	rBV	523	411	0.03%	0.004%
98	14.253	4013	4016	4018	rBV	534	283	0.02%	0.002%
99	14.282	4023	4025	4029	rVB2	570	288	0.02%	0.002%
100	15.150	4292	4295	4299	rVB2	867	556	0.03%	0.005%




Sum of corrected areas: 11690357

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
Data File : VU051122.D
Acq On : 05 Oct 2022 13:15
Operator : JC/MD
Sample : N4853-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW840

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

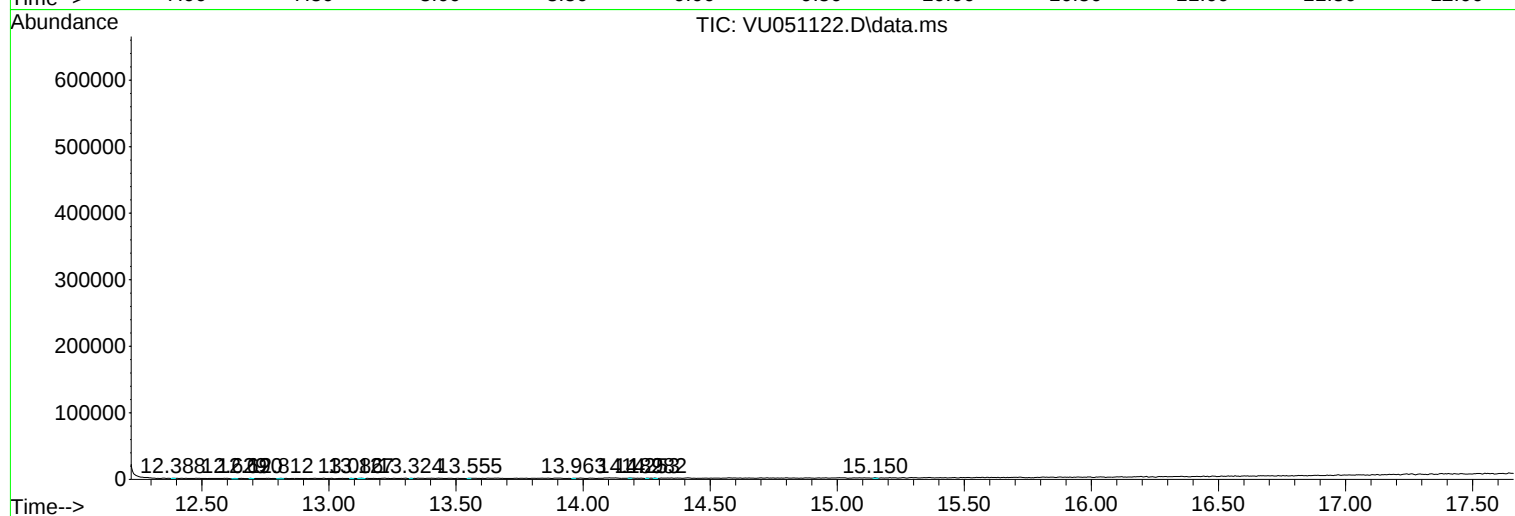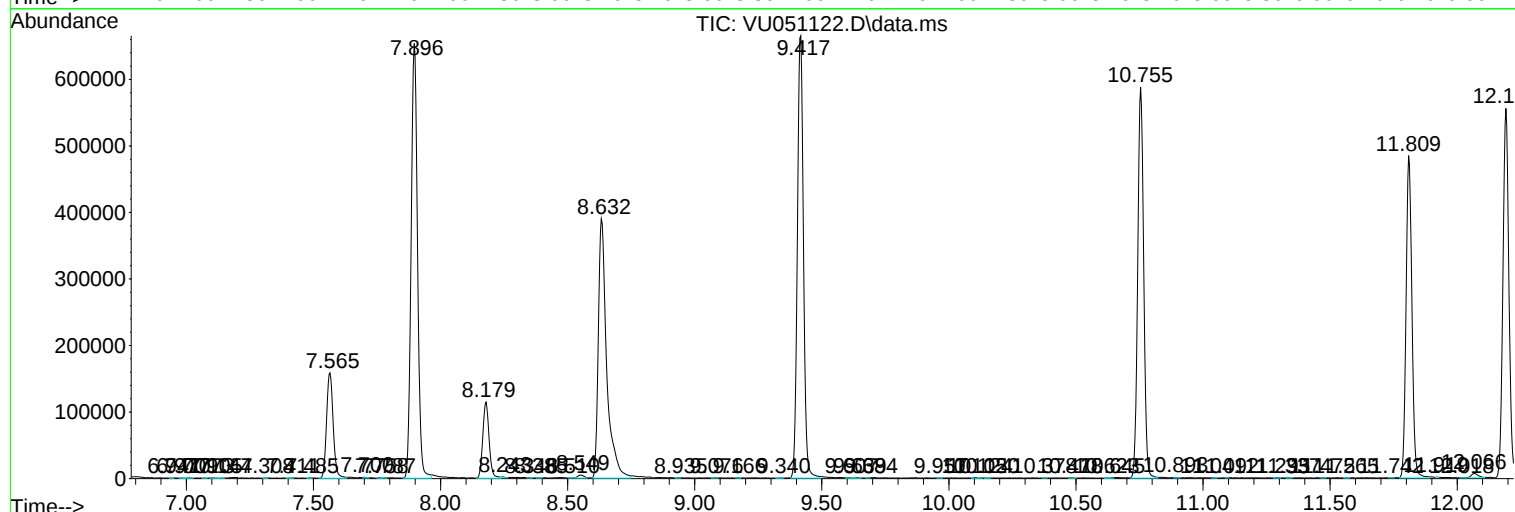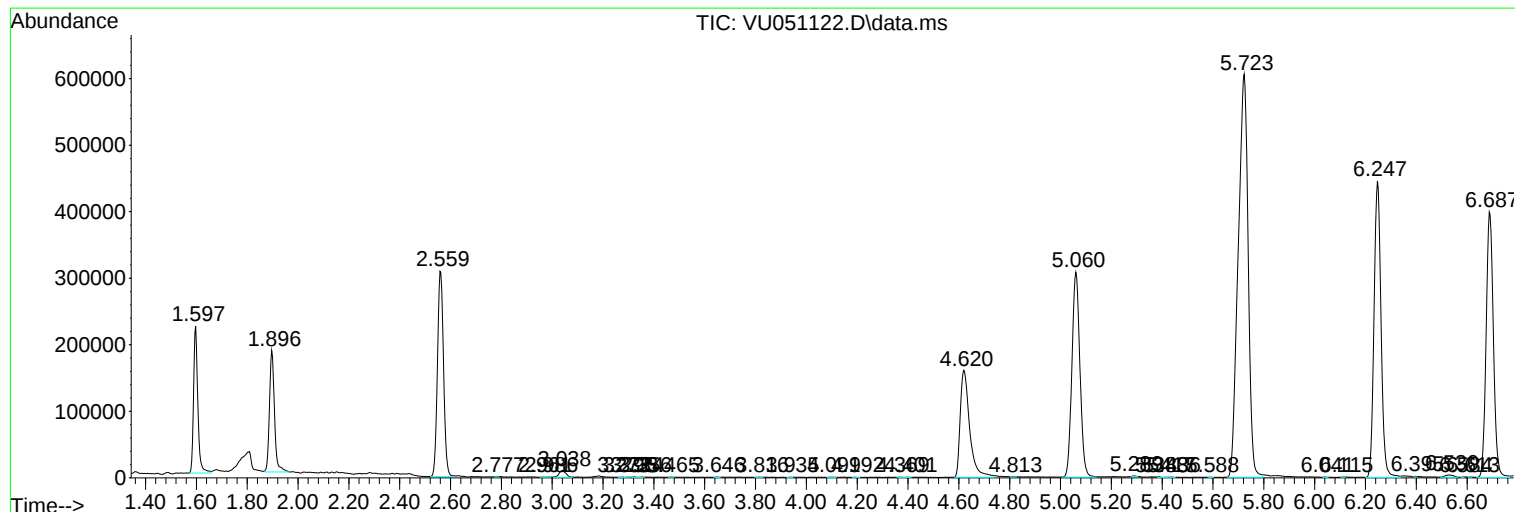

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
Data File : VU051122.D
Acq On : 05 Oct 2022 13:15
Operator : JC/MD
Sample : N4853-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW840

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
Data File : VU051122.D
Acq On : 05 Oct 2022 13:15
Operator : JC/MD
Sample : N4853-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW840

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc