

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
 Data File : VU051126.D
 Acq On : 05 Oct 2022 14:50
 Operator : JC/MD
 Sample : N4853-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW833

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

Signal : TIC: VU051126.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	93	rBV	225277	245636	15.20%	2.187%
2	1.896	166	173	194	rVB	181660	249724	15.45%	2.223%
3	2.562	368	380	395	rBV	301278	493432	30.53%	4.393%
4	3.041	519	529	543	rVB3	6439	12193	0.75%	0.109%
5	3.099	543	547	550	rBV2	477	475	0.03%	0.004%
6	3.260	594	597	602	rVB2	336	295	0.02%	0.003%
7	3.511	669	675	686	rVB2	405	719	0.04%	0.006%
8	3.556	687	689	690	rBV2	211	80	0.00%	0.001%
9	3.584	695	698	699	rBV	330	212	0.01%	0.002%
10	3.652	716	719	722	rBV2	310	177	0.01%	0.002%
11	3.668	722	724	725	rBV	341	162	0.01%	0.001%
12	3.748	747	749	752	rBV	370	168	0.01%	0.001%
13	3.867	784	786	791	rVB2	366	198	0.01%	0.002%
14	3.896	792	795	801	rVB	360	340	0.02%	0.003%
15	3.929	801	805	810	rBV3	283	320	0.02%	0.003%
16	3.954	810	813	816	rVB2	306	197	0.01%	0.002%
17	3.980	816	821	823	rBV2	268	223	0.01%	0.002%
18	4.022	830	834	837	rBV	286	315	0.02%	0.003%
19	4.073	847	850	852	rBV	271	133	0.01%	0.001%
20	4.099	852	858	860	rVV	375	349	0.02%	0.003%
21	4.134	864	869	875	rBV2	372	386	0.02%	0.003%
22	4.160	875	877	881	rVB	195	128	0.01%	0.001%
23	4.199	881	889	891	rBV	357	336	0.02%	0.003%
24	4.244	901	903	904	rBV	210	99	0.01%	0.001%
25	4.282	912	915	917	rBV	214	138	0.01%	0.001%
26	4.350	931	936	945	rVB2	437	549	0.03%	0.005%
27	4.401	945	952	959	rBV2	320	562	0.03%	0.005%
28	4.510	984	986	989	rBV	240	120	0.01%	0.001%
29	4.620	1008	1020	1047	rBV	149524	384181	23.77%	3.420%
30	5.060	1140	1157	1179	rBV	303387	663387	41.04%	5.906%
31	5.414	1263	1267	1270	rBV2	332	261	0.02%	0.002%
32	5.433	1270	1273	1277	rVV2	190	171	0.01%	0.002%
33	5.472	1283	1285	1286	rBV2	158	69	0.00%	0.001%
34	5.530	1301	1303	1309	rVB	545	400	0.02%	0.004%
35	5.568	1309	1315	1318	rVB2	431	340	0.02%	0.003%
36	5.584	1318	1320	1327	rBV2	287	350	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
 Data File : VU051126.D
 Acq On : 05 Oct 2022 14:50
 Operator : JC/MD
 Sample : N4853-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW833

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	5.652	1338	1341	1342	rBV2	151	80	0.00%	0.001%
38	5.723	1342	1363	1393	rBV2	590626	1616462	100.00%	14.391%
39	5.967	1437	1439	1440	rBV2	337	109	0.01%	0.001%
40	6.154	1494	1497	1502	rBV3	370	292	0.02%	0.003%
41	6.176	1502	1504	1507	rBV	302	171	0.01%	0.002%
42	6.247	1512	1526	1556	rBV	451533	866177	53.58%	7.712%
43	6.443	1584	1587	1590	rBV3	310	216	0.01%	0.002%
44	6.481	1596	1599	1602	rBV3	436	369	0.02%	0.003%
45	6.533	1606	1615	1621	rBV4	2781	4804	0.30%	0.043%
46	6.575	1627	1628	1630	rBV2	293	125	0.01%	0.001%
47	6.642	1646	1649	1650	rBV2	487	297	0.02%	0.003%
48	6.690	1650	1664	1696	rVV	396177	770966	47.69%	6.864%
49	6.880	1720	1723	1726	rBV	619	343	0.02%	0.003%
50	6.928	1735	1738	1741	rBV2	302	240	0.01%	0.002%
51	6.961	1746	1748	1750	rBV	222	94	0.01%	0.001%
52	7.115	1794	1796	1798	rBV	144	57	0.00%	0.001%
53	7.134	1798	1802	1805	rBV	461	357	0.02%	0.003%
54	7.166	1806	1812	1813	rBV3	644	536	0.03%	0.005%
55	7.247	1830	1837	1840	rBV2	526	555	0.03%	0.005%
56	7.295	1848	1852	1854	rBV2	264	180	0.01%	0.002%
57	7.308	1854	1856	1858	rBV2	297	153	0.01%	0.001%
58	7.350	1866	1869	1874	rBV2	375	417	0.03%	0.004%
59	7.407	1885	1887	1890	rBV2	465	275	0.02%	0.002%
60	7.501	1911	1916	1917	rBV	336	266	0.02%	0.002%
61	7.565	1924	1936	1954	rBV2	153626	268569	16.61%	2.391%
62	7.800	2007	2009	2011	rBV3	360	138	0.01%	0.001%
63	7.896	2025	2039	2060	rBV	615120	1064408	65.85%	9.476%
64	8.099	2101	2102	2105	rBV2	321	144	0.01%	0.001%
65	8.179	2113	2127	2144	rBV	111266	188511	11.66%	1.678%
66	8.446	2209	2210	2211	rBV	262	86	0.01%	0.001%
67	8.555	2237	2244	2251	rVB5	3074	4273	0.26%	0.038%
68	8.633	2255	2268	2302	rBV2	365426	833208	51.55%	7.418%
69	8.915	2352	2356	2358	rBV2	707	418	0.03%	0.004%
70	8.928	2358	2360	2364	rVB2	516	284	0.02%	0.003%
71	9.150	2427	2429	2433	rVB	382	184	0.01%	0.002%
72	9.166	2433	2434	2438	rVB	227	103	0.01%	0.001%
73	9.192	2439	2442	2445	rVV	578	385	0.02%	0.003%
74	9.208	2445	2447	2450	rVB2	387	197	0.01%	0.002%
75	9.353	2489	2492	2494	rBV	265	179	0.01%	0.002%
76	9.414	2498	2511	2538	rBV	654403	1094009	67.68%	9.740%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
 Data File : VU051126.D
 Acq On : 05 Oct 2022 14:50
 Operator : JC/MD
 Sample : N4853-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW833

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	9.571	2557	2560	2562	rBV	544	408	0.03%	0.004%
78	9.719	2604	2606	2608	rBV	488	313	0.02%	0.003%
79	9.790	2625	2628	2630	rBV	256	171	0.01%	0.002%
80	9.838	2639	2643	2645	rBV2	375	289	0.02%	0.003%
81	9.909	2663	2665	2668	rVB2	400	201	0.01%	0.002%
82	10.002	2691	2694	2696	rBV2	273	192	0.01%	0.002%
83	10.137	2734	2736	2738	rVB	267	109	0.01%	0.001%
84	10.153	2739	2741	2743	rBV	164	86	0.01%	0.001%
85	10.192	2750	2753	2756	rVB	370	220	0.01%	0.002%
86	10.346	2796	2801	2803	rBV2	247	249	0.02%	0.002%
87	10.485	2838	2844	2845	rBV	438	401	0.02%	0.004%
88	10.549	2861	2864	2866	rBV	417	298	0.02%	0.003%
89	10.755	2915	2928	2952	rBV	568327	903097	55.87%	8.040%
90	10.886	2966	2969	2979	rVB4	1285	1597	0.10%	0.014%
91	11.063	3021	3024	3026	rBV	457	189	0.01%	0.002%
92	11.166	3053	3056	3059	rBV	687	457	0.03%	0.004%
93	11.198	3062	3066	3069	rBV2	520	497	0.03%	0.004%
94	11.295	3094	3096	3099	rBV2	388	231	0.01%	0.002%
95	11.661	3208	3210	3213	rBV2	394	225	0.01%	0.002%
96	11.809	3244	3256	3281	rBV	456200	733796	45.40%	6.533%
97	12.063	3326	3335	3351	rBV4	14124	28554	1.77%	0.254%
98	12.192	3363	3375	3397	rBV	478957	785129	48.57%	6.990%




Sum of corrected areas: 11232171

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
Data File : VU051126.D
Acq On : 05 Oct 2022 14:50
Operator : JC/MD
Sample : N4853-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW833

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

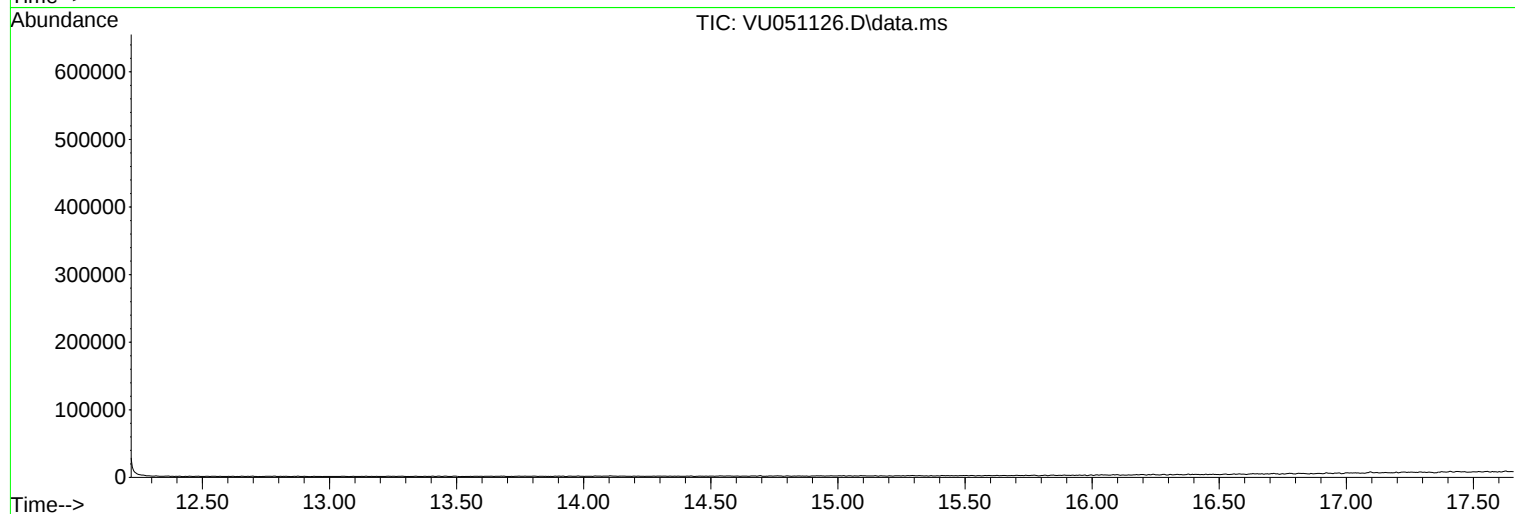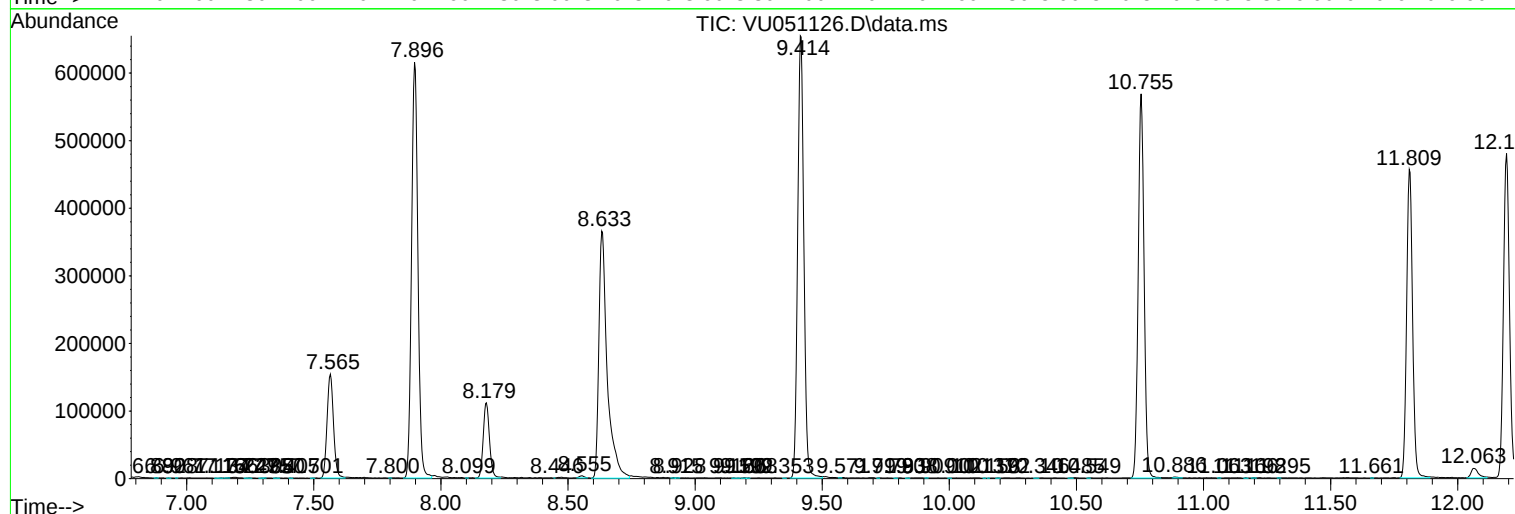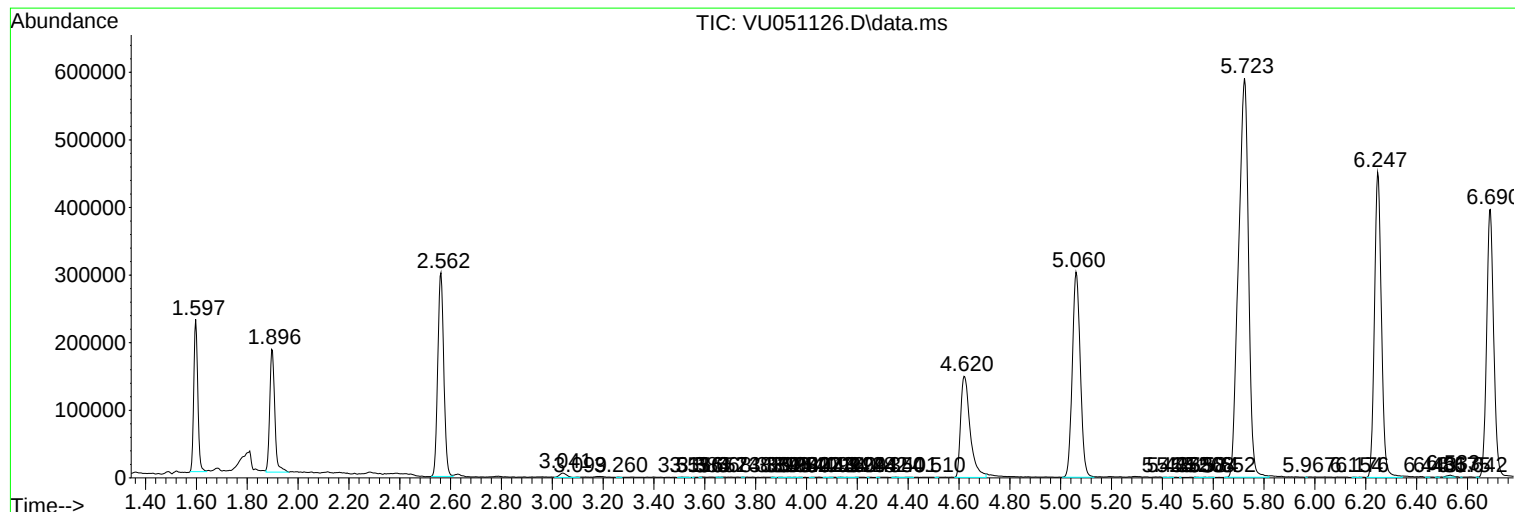

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
Data File : VU051126.D
Acq On : 05 Oct 2022 14:50
Operator : JC/MD
Sample : N4853-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW833

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
Data File : VU051126.D
Acq On : 05 Oct 2022 14:50
Operator : JC/MD
Sample : N4853-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW833

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc