

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
 Data File : VU051127.D
 Acq On : 05 Oct 2022 15:13
 Operator : JC/MD
 Sample : N4853-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW834

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

Signal : TIC: VU051127.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	103	rBV	209862	273840	18.12%	2.569%
2	1.900	167	174	193	rVB	161732	218705	14.47%	2.051%
3	2.562	368	380	394	rBV	269189	436589	28.89%	4.095%
4	2.787	442	450	461	rVB2	5541	9150	0.61%	0.086%
5	2.919	488	491	496	rVB3	667	435	0.03%	0.004%
6	2.944	496	499	501	rBV2	535	348	0.02%	0.003%
7	3.038	522	528	540	rVB4	5213	10332	0.68%	0.097%
8	3.176	564	571	575	rBV7	1145	1701	0.11%	0.016%
9	3.353	621	626	631	rBV4	1216	1274	0.08%	0.012%
10	3.629	710	712	717	rBV2	457	373	0.02%	0.003%
11	3.694	728	732	737	rBV3	529	592	0.04%	0.006%
12	3.874	781	788	791	rVV2	309	379	0.03%	0.004%
13	3.928	803	805	809	rBV2	412	286	0.02%	0.003%
14	3.993	823	825	830	rVB2	395	323	0.02%	0.003%
15	4.105	856	860	865	rBV2	248	290	0.02%	0.003%
16	4.198	884	889	895	rBV2	346	512	0.03%	0.005%
17	4.282	910	915	918	rBV3	309	331	0.02%	0.003%
18	4.375	939	944	949	rBV2	490	431	0.03%	0.004%
19	4.443	960	965	968	rVV2	355	348	0.02%	0.003%
20	4.459	968	970	978	rVB2	309	273	0.02%	0.003%
21	4.620	1008	1020	1059	rBV	145875	373561	24.72%	3.504%
22	5.060	1141	1157	1177	rVV	280207	617136	40.84%	5.789%
23	5.260	1215	1219	1220	rBV3	396	306	0.02%	0.003%
24	5.292	1223	1229	1235	rVV3	1507	2122	0.14%	0.020%
25	5.366	1249	1252	1253	rBV2	531	276	0.02%	0.003%
26	5.382	1255	1257	1261	rVB3	950	632	0.04%	0.006%
27	5.604	1322	1326	1332	rBV2	1003	860	0.06%	0.008%
28	5.636	1332	1336	1342	rBV2	478	421	0.03%	0.004%
29	5.723	1342	1363	1392	rBV2	548902	1511093	100.00%	14.174%
30	5.919	1421	1424	1427	rVV2	440	282	0.02%	0.003%
31	5.941	1427	1431	1434	rVV3	447	345	0.02%	0.003%
32	5.957	1434	1436	1441	rVV2	730	488	0.03%	0.005%
33	5.983	1441	1444	1449	rVB2	597	381	0.03%	0.004%
34	6.157	1496	1498	1504	rVB4	463	383	0.03%	0.004%
35	6.247	1512	1526	1549	rBV	415019	790186	52.29%	7.412%
36	6.526	1599	1613	1616	rBV7	2833	4069	0.27%	0.038%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
 Data File : VU051127.D
 Acq On : 05 Oct 2022 15:13
 Operator : JC/MD
 Sample : N4853-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW834

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	6.575	1625	1628	1630	rBV2	441	300	0.02%	0.003%
38	6.687	1648	1663	1681	rBV	365811	718123	47.52%	6.736%
39	6.960	1746	1748	1754	rVB2	485	357	0.02%	0.003%
40	7.118	1793	1797	1801	rBV2	279	281	0.02%	0.003%
41	7.182	1810	1817	1818	rBV3	1251	1169	0.08%	0.011%
42	7.247	1835	1837	1842	rVB2	556	401	0.03%	0.004%
43	7.452	1900	1901	1909	rVB	457	349	0.02%	0.003%
44	7.565	1924	1936	1951	rBV	152909	268710	17.78%	2.520%
45	7.645	1959	1961	1966	rVB2	693	573	0.04%	0.005%
46	7.697	1973	1977	1980	rBV4	594	542	0.04%	0.005%
47	7.790	2000	2006	2007	rBV3	587	614	0.04%	0.006%
48	7.896	2025	2039	2056	rBV	581055	998618	66.09%	9.367%
49	8.070	2091	2093	2097	rVB4	684	431	0.03%	0.004%
50	8.102	2101	2103	2110	rVB2	819	593	0.04%	0.006%
51	8.179	2113	2127	2145	rBV	108967	185893	12.30%	1.744%
52	8.552	2236	2243	2253	rVB7	2254	3618	0.24%	0.034%
53	8.632	2256	2268	2302	rBV2	364352	803029	53.14%	7.532%
54	8.848	2332	2335	2339	rBV4	1094	786	0.05%	0.007%
55	8.915	2353	2356	2359	rVB4	514	369	0.02%	0.003%
56	8.941	2359	2364	2368	rBV3	676	645	0.04%	0.006%
57	9.047	2391	2397	2400	rBV2	523	508	0.03%	0.005%
58	9.246	2457	2459	2462	rVV	450	276	0.02%	0.003%
59	9.414	2499	2511	2535	rBV	611867	1015104	67.18%	9.522%
60	9.690	2588	2597	2600	rBV3	1078	1505	0.10%	0.014%
61	9.928	2668	2671	2675	rBV	504	385	0.03%	0.004%
62	10.105	2720	2726	2735	rVB5	728	1380	0.09%	0.013%
63	10.362	2802	2806	2809	rBV	286	302	0.02%	0.003%
64	10.404	2817	2819	2822	rVV2	578	345	0.02%	0.003%
65	10.754	2913	2928	2947	rBV	541501	864769	57.23%	8.111%
66	10.883	2963	2968	2974	rVB4	782	848	0.06%	0.008%
67	10.941	2981	2986	2990	rBV2	463	483	0.03%	0.005%
68	11.005	3000	3006	3008	rBV	251	295	0.02%	0.003%
69	11.099	3030	3035	3040	rBV4	486	496	0.03%	0.005%
70	11.237	3076	3078	3080	rVV	494	278	0.02%	0.003%
71	11.369	3115	3119	3124	rVB3	348	331	0.02%	0.003%
72	11.398	3124	3128	3131	rBV	401	367	0.02%	0.003%
73	11.414	3131	3133	3139	rVB2	603	467	0.03%	0.004%
74	11.446	3139	3143	3147	rBV2	378	367	0.02%	0.003%
75	11.471	3148	3151	3153	rBV3	496	313	0.02%	0.003%
76	11.584	3183	3186	3191	rBV2	446	468	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
 Data File : VU051127.D
 Acq On : 05 Oct 2022 15:13
 Operator : JC/MD
 Sample : N4853-13
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW834

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	11.610	3192	3194	3199	rBV	350	323	0.02%	0.003%
78	11.745	3232	3236	3240	rBV4	605	488	0.03%	0.005%
79	11.809	3244	3256	3281	rBV	433771	699251	46.27%	6.559%
80	12.066	3327	3336	3351	rBV6	12046	23967	1.59%	0.225%
81	12.192	3362	3375	3390	rBV	481517	794233	52.56%	7.450%
82	12.375	3427	3432	3435	rVB3	677	446	0.03%	0.004%
83	12.455	3454	3457	3462	rBV3	510	439	0.03%	0.004%
84	12.536	3480	3482	3486	rBV2	318	279	0.02%	0.003%
85	12.613	3503	3506	3508	rBV2	365	279	0.02%	0.003%
86	12.661	3515	3521	3522	rBV2	481	452	0.03%	0.004%
87	12.700	3528	3533	3538	rBV2	453	512	0.03%	0.005%
88	12.770	3552	3555	3561	rVV3	532	550	0.04%	0.005%
89	12.860	3579	3583	3590	rVB3	592	619	0.04%	0.006%
90	12.951	3608	3611	3614	rBV2	416	286	0.02%	0.003%
91	12.970	3614	3617	3622	rBV2	408	423	0.03%	0.004%
92	13.594	3808	3811	3814	rBV3	501	331	0.02%	0.003%
93	13.899	3904	3906	3909	rBV2	433	296	0.02%	0.003%
94	14.063	3953	3957	3961	rBV2	433	449	0.03%	0.004%
95	14.806	4186	4188	4190	rBV2	610	286	0.02%	0.003%
96	15.156	4294	4297	4299	rBV	826	479	0.03%	0.004%
97	15.426	4379	4381	4384	rBV	638	399	0.03%	0.004%
98	15.597	4431	4434	4436	rBV2	860	533	0.04%	0.005%
99	16.105	4589	4592	4595	rBV4	1283	1176	0.08%	0.011%
100	16.243	4633	4635	4638	rBV3	1258	908	0.06%	0.009%




Sum of corrected areas: 10661145

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
Data File : VU051127.D
Acq On : 05 Oct 2022 15:13
Operator : JC/MD
Sample : N4853-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW834

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

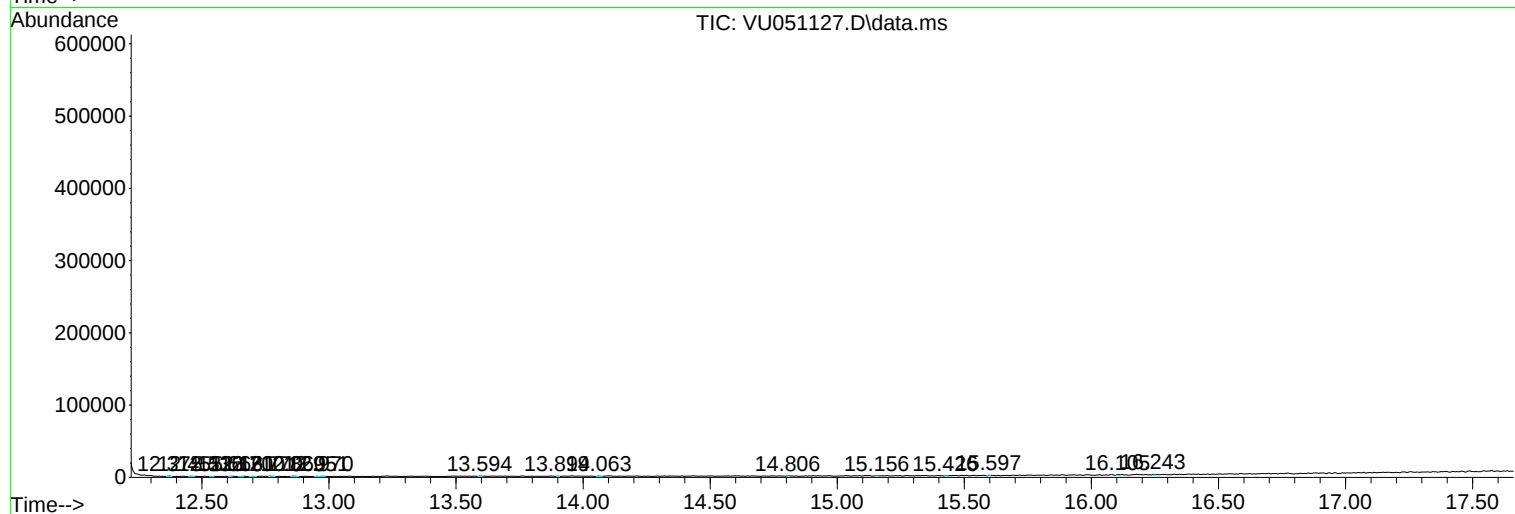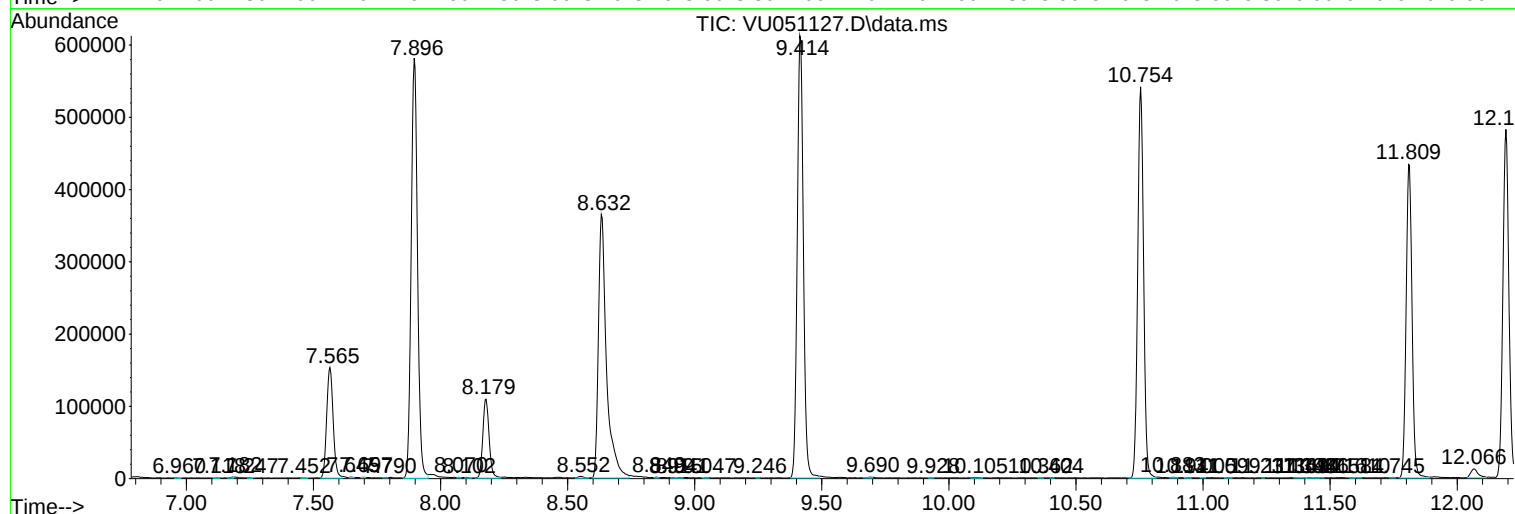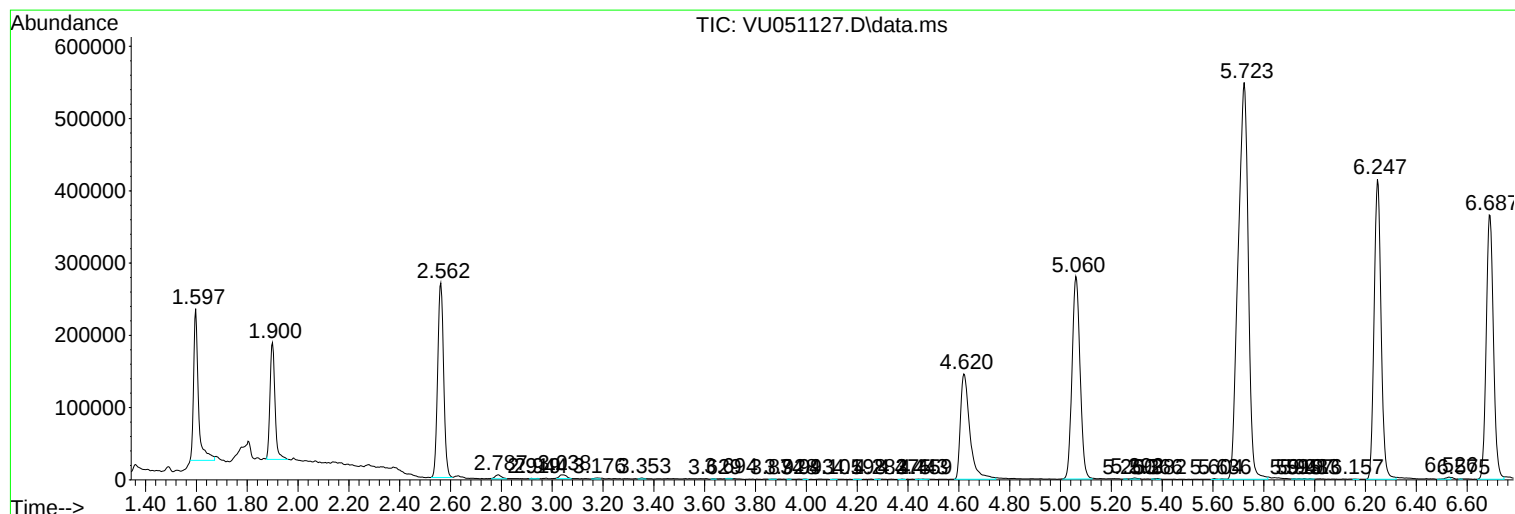

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
Data File : VU051127.D
Acq On : 05 Oct 2022 15:13
Operator : JC/MD
Sample : N4853-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW834

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
Data File : VU051127.D
Acq On : 05 Oct 2022 15:13
Operator : JC/MD
Sample : N4853-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW834

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc