

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
 Data File : VU051132.D
 Acq On : 05 Oct 2022 17:34
 Operator : JC/MD
 Sample : N4853-16
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW838

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

Signal : TIC: VU051132.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	93	rBV	201483	226831	14.73%	2.110%
2	1.899	167	174	194	rVB	166049	224608	14.59%	2.090%
3	2.562	368	380	394	rBV	271178	442008	28.71%	4.112%
4	2.825	460	462	464	rBV2	481	254	0.02%	0.002%
5	3.041	520	529	540	rVB2	9889	16242	1.05%	0.151%
6	3.176	564	571	574	rBV2	919	1268	0.08%	0.012%
7	3.301	608	610	611	rBV2	162	72	0.00%	0.001%
8	3.317	611	615	618	rVB2	476	323	0.02%	0.003%
9	3.337	618	621	623	rBV2	481	307	0.02%	0.003%
10	3.350	623	625	626	rBV	495	190	0.01%	0.002%
11	3.433	649	651	657	rVB	400	320	0.02%	0.003%
12	3.472	657	663	666	rBV3	642	696	0.05%	0.006%
13	3.623	707	710	714	rBV	288	209	0.01%	0.002%
14	3.713	735	738	740	rBV	199	131	0.01%	0.001%
15	3.835	772	776	784	rBV2	280	408	0.03%	0.004%
16	3.938	806	808	810	rBV	136	52	0.00%	0.000%
17	3.967	815	817	819	rBV2	133	75	0.00%	0.001%
18	4.015	827	832	838	rVB3	276	294	0.02%	0.003%
19	4.050	840	843	848	rBV	438	327	0.02%	0.003%
20	4.102	854	859	865	rBV2	355	456	0.03%	0.004%
21	4.128	865	867	868	rBV2	82	41	0.00%	0.000%
22	4.137	868	870	872	rVV	149	68	0.00%	0.001%
23	4.218	893	895	898	rVB	311	120	0.01%	0.001%
24	4.250	902	905	907	rBV2	182	146	0.01%	0.001%
25	4.314	922	925	927	rBV	184	105	0.01%	0.001%
26	4.366	938	941	944	rBV2	196	162	0.01%	0.002%
27	4.533	987	993	995	rBV	256	229	0.01%	0.002%
28	4.620	1007	1020	1053	rBV	145031	372600	24.20%	3.466%
29	5.060	1140	1157	1179	rBV	288292	629861	40.91%	5.860%
30	5.279	1220	1225	1226	rBV3	898	663	0.04%	0.006%
31	5.369	1249	1253	1255	rBV4	723	660	0.04%	0.006%
32	5.568	1310	1315	1321	rBV2	323	369	0.02%	0.003%
33	5.623	1329	1332	1334	rVB2	242	136	0.01%	0.001%
34	5.639	1335	1337	1338	rBV2	103	42	0.00%	0.000%
35	5.722	1341	1363	1385	rBV2	557151	1539646	100.00%	14.324%
36	6.044	1456	1463	1465	rBV3	349	469	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
 Data File : VU051132.D
 Acq On : 05 Oct 2022 17:34
 Operator : JC/MD
 Sample : N4853-16
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW838

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	6.076	1471	1473	1474	rBV2	165	49	0.00%	0.000%
38	6.121	1482	1487	1491	rBV2	440	544	0.04%	0.005%
39	6.153	1495	1497	1500	rBV2	350	189	0.01%	0.002%
40	6.247	1512	1526	1545	rBV	423354	805840	52.34%	7.497%
41	6.536	1606	1616	1624	rVB6	3030	5493	0.36%	0.051%
42	6.632	1644	1646	1649	rVB	607	236	0.02%	0.002%
43	6.690	1649	1664	1682	rBV	374965	732684	47.59%	6.816%
44	6.954	1745	1746	1748	rBV	123	58	0.00%	0.001%
45	6.970	1748	1751	1752	rBV	356	176	0.01%	0.002%
46	7.018	1763	1766	1770	rVB2	177	115	0.01%	0.001%
47	7.079	1780	1785	1789	rBV2	374	361	0.02%	0.003%
48	7.253	1836	1839	1843	rBV2	254	196	0.01%	0.002%
49	7.291	1849	1851	1853	rBV	105	65	0.00%	0.001%
50	7.359	1869	1872	1875	rBV2	592	439	0.03%	0.004%
51	7.388	1879	1881	1884	rVB3	268	172	0.01%	0.002%
52	7.475	1903	1908	1910	rBV	253	191	0.01%	0.002%
53	7.494	1910	1914	1918	rBV2	428	333	0.02%	0.003%
54	7.565	1924	1936	1951	rBV	153881	270684	17.58%	2.518%
55	7.803	2002	2010	2012	rBV4	1014	954	0.06%	0.009%
56	7.896	2025	2039	2057	rBV	608569	1039469	67.51%	9.670%
57	8.179	2115	2127	2143	rBV	107540	185850	12.07%	1.729%
58	8.552	2233	2243	2256	rVB3	26473	44916	2.92%	0.418%
59	8.632	2256	2268	2305	rBV3	352947	794508	51.60%	7.392%
60	9.015	2384	2387	2391	rVB2	297	214	0.01%	0.002%
61	9.037	2391	2394	2398	rBV2	524	326	0.02%	0.003%
62	9.224	2450	2452	2455	rBV2	193	108	0.01%	0.001%
63	9.324	2478	2483	2488	rBV	381	473	0.03%	0.004%
64	9.417	2498	2512	2536	rBV	630921	1039188	67.50%	9.668%
65	9.600	2567	2569	2573	rBV2	353	207	0.01%	0.002%
66	9.642	2578	2582	2585	rBV2	636	405	0.03%	0.004%
67	9.697	2593	2599	2601	rBV4	1058	1041	0.07%	0.010%
68	9.748	2610	2615	2619	rVB3	419	454	0.03%	0.004%
69	9.912	2664	2666	2674	rVB2	484	468	0.03%	0.004%
70	9.951	2674	2678	2680	rBV	285	209	0.01%	0.002%
71	9.967	2680	2683	2685	rBV	208	106	0.01%	0.001%
72	10.291	2781	2784	2787	rBV	315	180	0.01%	0.002%
73	10.635	2888	2891	2894	rBV	373	257	0.02%	0.002%
74	10.651	2894	2896	2904	rVV	343	312	0.02%	0.003%
75	10.754	2915	2928	2948	rBV	543796	873416	56.73%	8.126%
76	11.809	3244	3256	3278	rBV	421190	686795	44.61%	6.389%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
Data File : VU051132.D
Acq On : 05 Oct 2022 17:34
Operator : JC/MD
Sample : N4853-16
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW838

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Title : VOC Analysis

77	12.069	3328	3337	3354	rVB6	6216	12671	0.82%	0.118%
78	12.192	3362	3375	3403	rBV	477713	787747	51.16%	7.329%
79	12.921	3598	3602	3604	rBV	449	439	0.03%	0.004%




Sum of corrected areas: 10748926

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
Data File : VU051132.D
Acq On : 05 Oct 2022 17:34
Operator : JC/MD
Sample : N4853-16
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW838

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

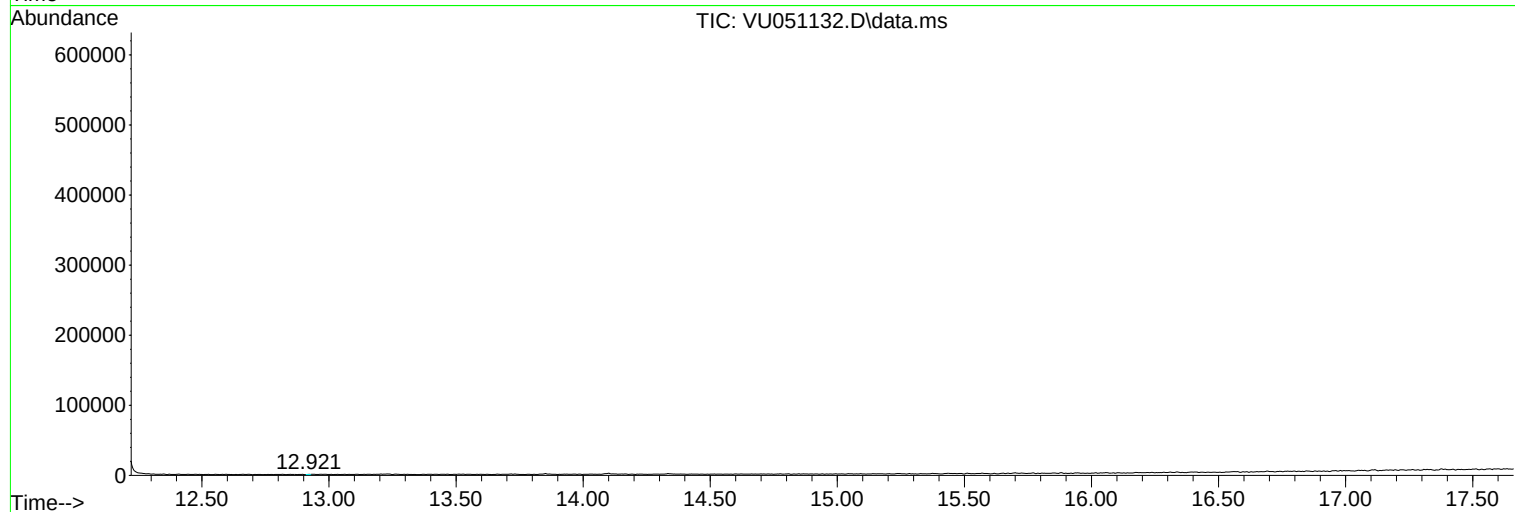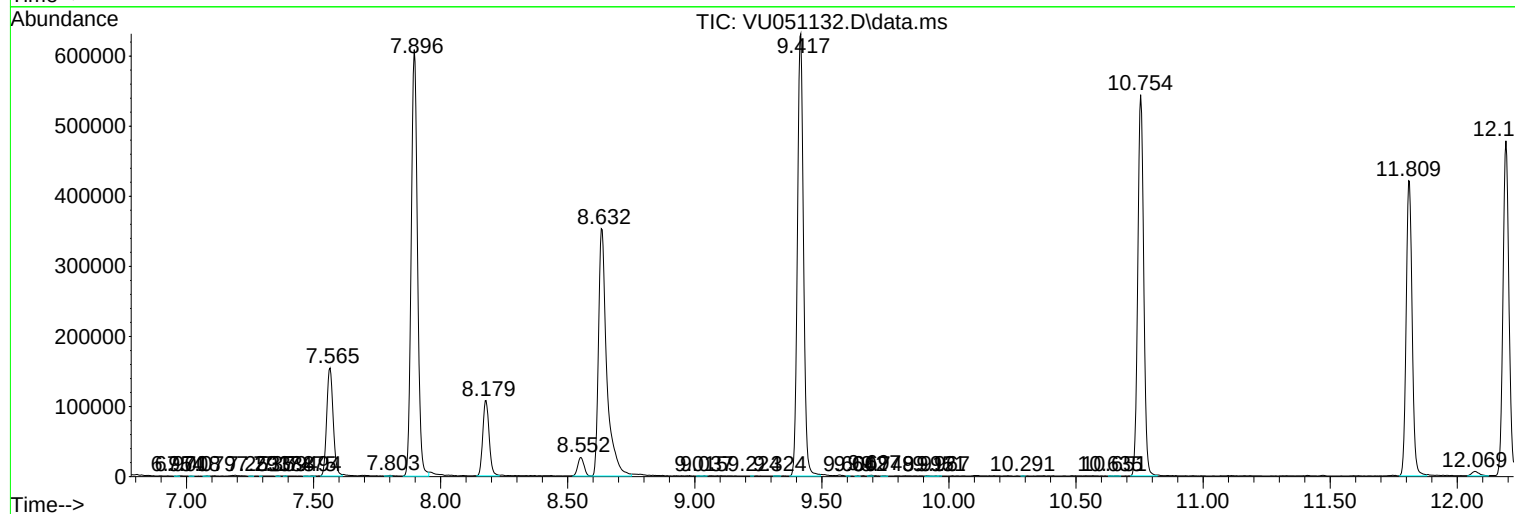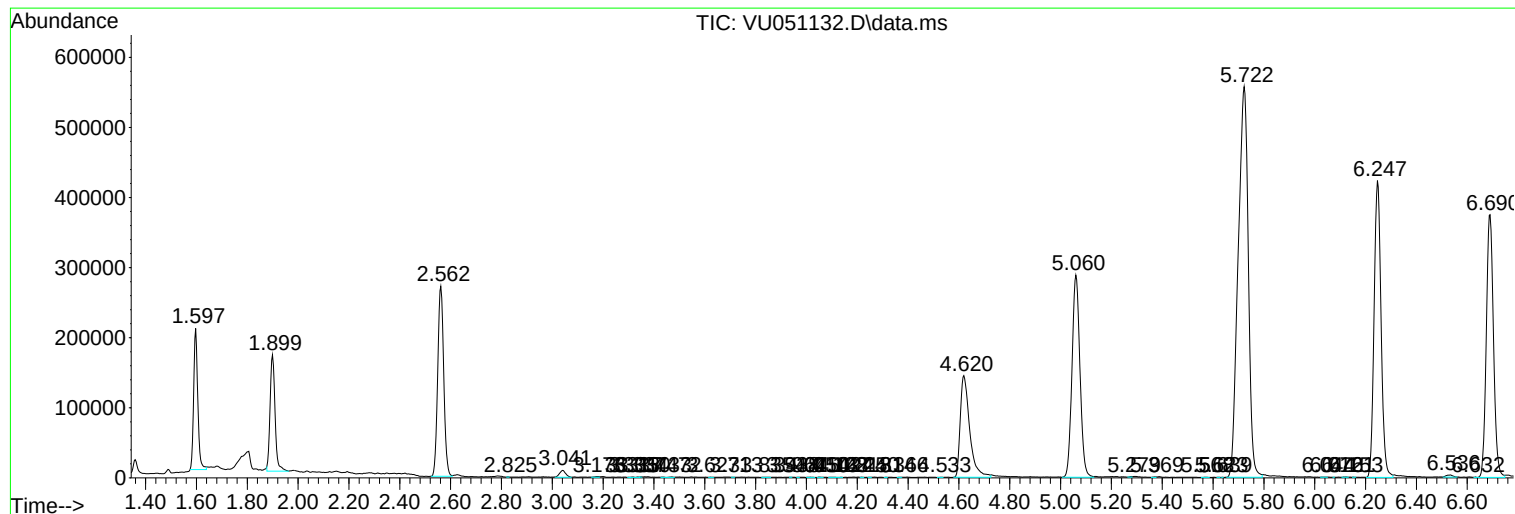

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
Data File : VU051132.D
Acq On : 05 Oct 2022 17:34
Operator : JC/MD
Sample : N4853-16
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW838

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
Data File : VU051132.D
Acq On : 05 Oct 2022 17:34
Operator : JC/MD
Sample : N4853-16
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW838

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc