

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
 Data File : VU051134.D
 Acq On : 05 Oct 2022 18:22
 Operator : JC/MD
 Sample : N4853-18
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW841

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

Signal : TIC: VU051134.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	92	rBV	190753	218523	10.02%	1.725%
2	1.900	165	174	194	rVB	162375	223135	10.23%	1.762%
3	2.562	367	380	394	rBV	262540	429238	19.68%	3.389%
4	2.681	415	417	422	rVB2	529	372	0.02%	0.003%
5	2.755	437	440	443	rBV3	367	301	0.01%	0.002%
6	2.861	469	473	476	rBV2	465	396	0.02%	0.003%
7	2.957	500	503	507	rBV3	445	273	0.01%	0.002%
8	3.038	519	528	547	rBV3	8317	14940	0.69%	0.118%
9	3.125	552	555	559	rBV2	369	293	0.01%	0.002%
10	3.157	560	565	566	rBV	590	442	0.02%	0.003%
11	3.353	623	626	628	rBV2	423	308	0.01%	0.002%
12	3.546	678	686	688	rBV	262	290	0.01%	0.002%
13	3.896	793	795	800	rVB	445	356	0.02%	0.003%
14	3.944	807	810	814	rVB	385	295	0.01%	0.002%
15	4.125	862	866	870	rBV2	352	279	0.01%	0.002%
16	4.314	922	925	933	rVB2	272	281	0.01%	0.002%
17	4.401	948	952	956	rBV2	349	332	0.02%	0.003%
18	4.427	956	960	965	rVB	480	470	0.02%	0.004%
19	4.539	989	995	1000	rBV	426	455	0.02%	0.004%
20	4.620	1008	1020	1062	rBV	142048	369010	16.92%	2.913%
21	4.790	1071	1073	1076	rVB2	534	276	0.01%	0.002%
22	4.906	1106	1109	1112	rVB	542	287	0.01%	0.002%
23	5.060	1140	1157	1178	rVV	281675	617291	28.31%	4.873%
24	5.282	1221	1226	1228	rBV4	643	606	0.03%	0.005%
25	5.385	1254	1258	1266	rVB4	681	827	0.04%	0.007%
26	5.456	1276	1280	1282	rBV	427	286	0.01%	0.002%
27	5.723	1337	1363	1388	rBV2	547987	1507739	69.14%	11.903%
28	5.960	1434	1437	1442	rVB4	409	326	0.01%	0.003%
29	5.989	1442	1446	1453	rVB3	839	827	0.04%	0.007%
30	6.025	1453	1457	1459	rBV3	531	365	0.02%	0.003%
31	6.163	1495	1500	1504	rBV	297	292	0.01%	0.002%
32	6.247	1508	1526	1550	rBV	423043	799863	36.68%	6.315%
33	6.420	1576	1580	1582	rBV4	537	367	0.02%	0.003%
34	6.526	1606	1613	1626	rBV9	3601	7343	0.34%	0.058%
35	6.690	1649	1664	1683	rVV	365886	718542	32.95%	5.673%
36	6.903	1727	1730	1733	rBV	809	641	0.03%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
 Data File : VU051134.D
 Acq On : 05 Oct 2022 18:22
 Operator : JC/MD
 Sample : N4853-18
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW841

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	7.102	1787	1792	1797	rBV4	608	670	0.03%	0.005%
38	7.192	1811	1820	1825	rBV6	1467	1974	0.09%	0.016%
39	7.211	1825	1826	1831	rVB	677	340	0.02%	0.003%
40	7.378	1874	1878	1881	rBV2	368	331	0.02%	0.003%
41	7.565	1922	1936	1962	rBV	150735	266614	12.23%	2.105%
42	7.694	1972	1976	1982	rVB4	1062	1171	0.05%	0.009%
43	7.784	2001	2004	2008	rBV4	377	317	0.01%	0.003%
44	7.896	2025	2039	2057	rBV	580688	1002886	45.99%	7.917%
45	8.179	2115	2127	2144	rBV	104939	181013	8.30%	1.429%
46	8.253	2149	2150	2154	rVV2	749	510	0.02%	0.004%
47	8.272	2154	2156	2161	rVB2	772	522	0.02%	0.004%
48	8.385	2188	2191	2193	rBV2	430	275	0.01%	0.002%
49	8.552	2229	2243	2258	rBV	1303201	2180599	100.00%	17.215%
50	8.632	2258	2268	2313	rVB2	364092	826856	37.92%	6.528%
51	8.922	2355	2358	2361	rVB2	634	370	0.02%	0.003%
52	8.983	2374	2377	2382	rVB3	779	753	0.03%	0.006%
53	9.012	2382	2386	2387	rBV2	497	295	0.01%	0.002%
54	9.025	2387	2390	2392	rBV2	532	304	0.01%	0.002%
55	9.157	2428	2431	2434	rVV3	537	361	0.02%	0.003%
56	9.179	2434	2438	2443	rVV3	470	390	0.02%	0.003%
57	9.272	2463	2467	2471	rVV3	463	479	0.02%	0.004%
58	9.417	2497	2512	2541	rBV	603398	1014316	46.52%	8.008%
59	9.558	2553	2556	2557	rBV	606	303	0.01%	0.002%
60	9.603	2567	2570	2573	rVV4	440	299	0.01%	0.002%
61	9.693	2593	2598	2607	rVB5	1668	2044	0.09%	0.016%
62	9.774	2621	2623	2626	rBV	400	294	0.01%	0.002%
63	9.838	2641	2643	2647	rVB2	508	307	0.01%	0.002%
64	9.874	2649	2654	2659	rBV2	472	622	0.03%	0.005%
65	10.041	2698	2706	2707	rBV2	356	367	0.02%	0.003%
66	10.095	2718	2723	2725	rBV2	1117	982	0.05%	0.008%
67	10.259	2770	2774	2776	rBV	335	273	0.01%	0.002%
68	10.320	2790	2793	2800	rVB3	454	437	0.02%	0.003%
69	10.488	2843	2845	2848	rVB2	701	364	0.02%	0.003%
70	10.584	2869	2875	2877	rBV2	462	517	0.02%	0.004%
71	10.629	2884	2889	2894	rBV3	290	340	0.02%	0.003%
72	10.709	2909	2914	2916	rBV	445	422	0.02%	0.003%
73	10.755	2916	2928	2947	rBV	526237	851954	39.07%	6.726%
74	10.886	2965	2969	2971	rBV2	527	444	0.02%	0.004%
75	11.044	3015	3018	3021	rBV	341	332	0.02%	0.003%
76	11.086	3028	3031	3033	rBV2	474	342	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
 Data File : VU051134.D
 Acq On : 05 Oct 2022 18:22
 Operator : JC/MD
 Sample : N4853-18
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW841

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	11.115	3038	3040	3047	rVB2	579	416	0.02%	0.003%
78	11.176	3055	3059	3061	rBV2	397	364	0.02%	0.003%
79	11.340	3106	3110	3117	rVV	381	384	0.02%	0.003%
80	11.430	3136	3138	3143	rVB	632	382	0.02%	0.003%
81	11.468	3146	3150	3156	rVB5	694	807	0.04%	0.006%
82	11.526	3165	3168	3172	rBV	318	279	0.01%	0.002%
83	11.590	3184	3188	3191	rBV2	456	347	0.02%	0.003%
84	11.642	3200	3204	3208	rVB2	378	282	0.01%	0.002%
85	11.713	3219	3226	3230	rBV2	671	963	0.04%	0.008%
86	11.809	3244	3256	3282	rBV	393278	645383	29.60%	5.095%
87	12.063	3327	3335	3346	rBV4	8466	15342	0.70%	0.121%
88	12.192	3362	3375	3395	rBV	446093	738267	33.86%	5.828%
89	12.571	3490	3493	3496	rBV2	530	409	0.02%	0.003%
90	12.590	3497	3499	3505	rVB2	480	407	0.02%	0.003%
91	12.825	3567	3572	3576	rBV3	757	617	0.03%	0.005%
92	12.980	3617	3620	3622	rBV	392	291	0.01%	0.002%
93	13.037	3631	3638	3642	rBV4	626	820	0.04%	0.006%
94	13.147	3669	3672	3678	rBB2	534	422	0.02%	0.003%
95	13.224	3694	3696	3699	rVV3	502	318	0.01%	0.003%
96	13.568	3798	3803	3805	rBV3	498	513	0.02%	0.004%
97	13.912	3908	3910	3914	rBV2	342	304	0.01%	0.002%
98	14.304	4029	4032	4034	rBV4	580	306	0.01%	0.002%
99	14.327	4037	4039	4046	rVB3	913	1057	0.05%	0.008%
100	14.687	4148	4151	4154	rBV2	685	509	0.02%	0.004%




Sum of corrected areas: 12667045

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
Data File : VU051134.D
Acq On : 05 Oct 2022 18:22
Operator : JC/MD
Sample : N4853-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW841

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

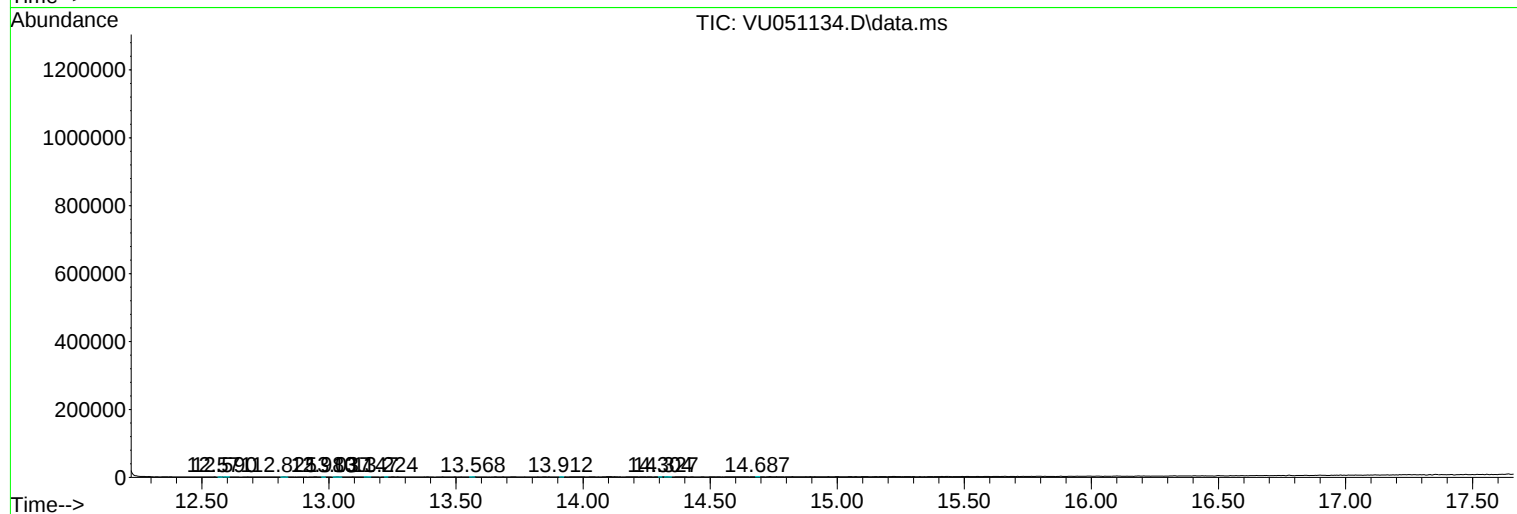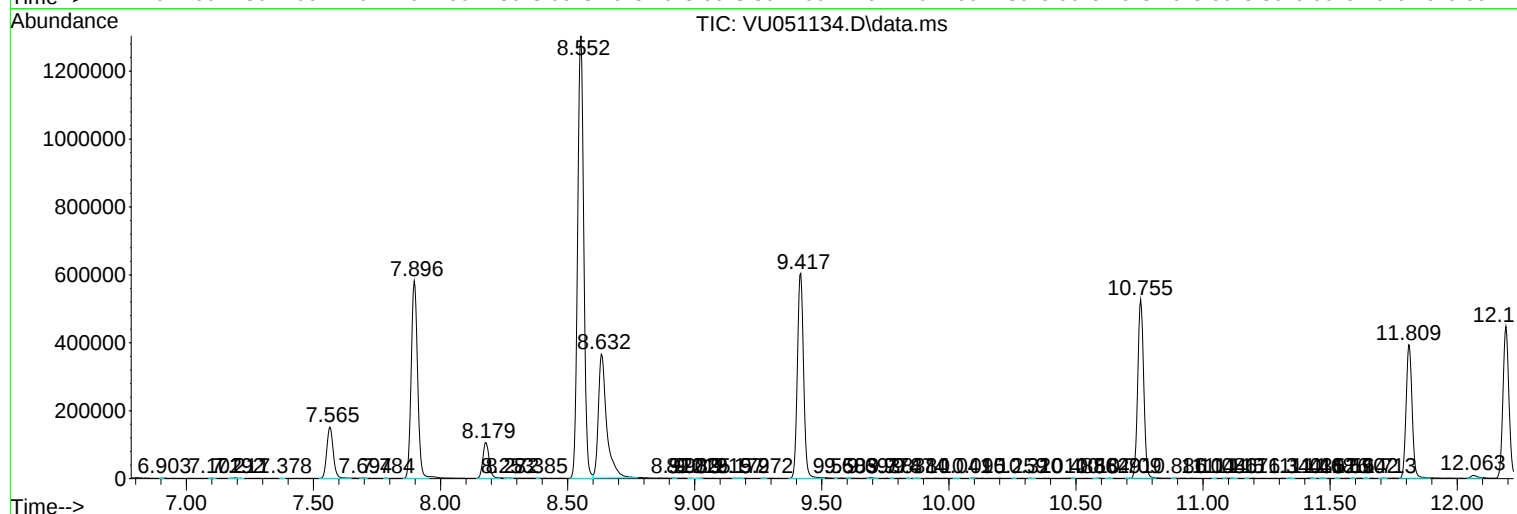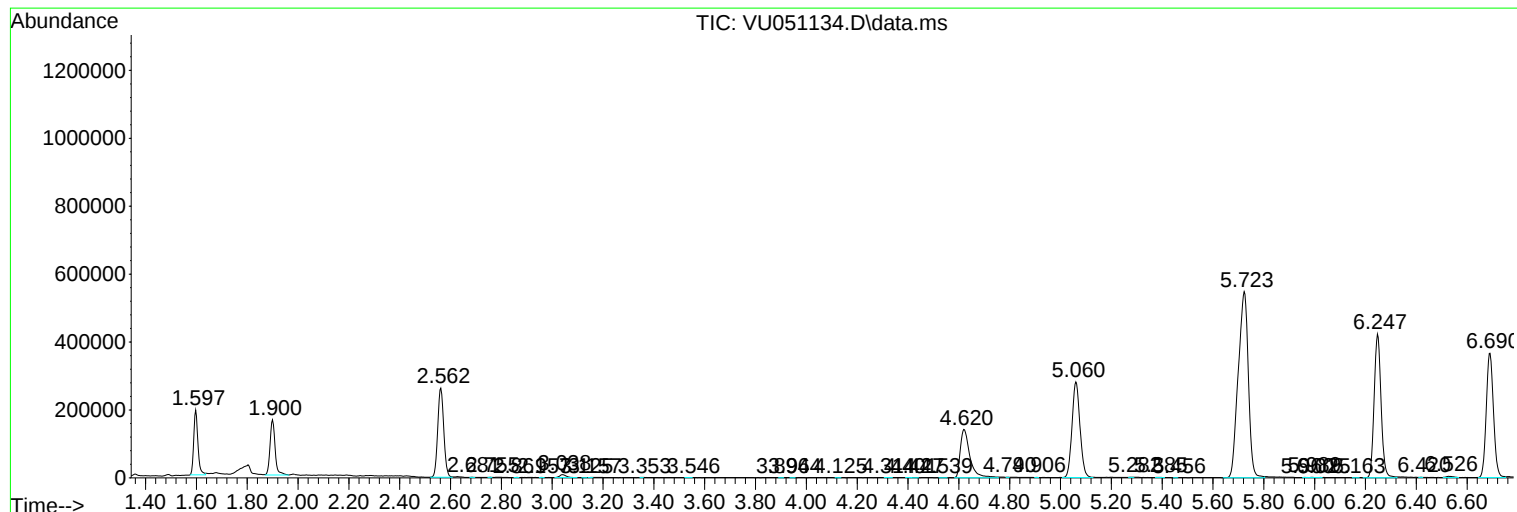

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
Data File : VU051134.D
Acq On : 05 Oct 2022 18:22
Operator : JC/MD
Sample : N4853-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW841

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
Data File : VU051134.D
Acq On : 05 Oct 2022 18:22
Operator : JC/MD
Sample : N4853-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW841

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc