

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
 Data File : VU051141.D
 Acq On : 05 Oct 2022 21:31
 Operator : JC/MD
 Sample : VU1005WBL02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK198

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M

Title : VOC Analysis

Signal : TIC: VU051141.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	93	rBV	231747	272337	14.42%	2.076%
2	1.900	166	174	199	rVB	198755	275934	14.61%	2.104%
3	2.562	367	380	396	rBV	355226	576015	30.49%	4.392%
4	2.755	437	440	443	rBV3	440	319	0.02%	0.002%
5	2.781	444	448	450	rBV2	1584	1275	0.07%	0.010%
6	2.941	494	498	502	rBV3	1025	869	0.05%	0.007%
7	3.044	521	530	536	rBV4	2665	3947	0.21%	0.030%
8	3.086	541	543	549	rVB2	384	310	0.02%	0.002%
9	3.118	549	553	557	rBV3	346	396	0.02%	0.003%
10	3.183	561	573	589	rVB3	2707	6366	0.34%	0.049%
11	3.257	592	596	598	rBV	417	335	0.02%	0.003%
12	3.337	615	621	622	rBV2	692	532	0.03%	0.004%
13	3.353	622	626	628	rVV3	1053	944	0.05%	0.007%
14	3.375	631	633	638	rVB3	486	318	0.02%	0.002%
15	3.491	666	669	675	rVB2	341	329	0.02%	0.003%
16	4.041	838	840	848	rVV3	498	406	0.02%	0.003%
17	4.170	877	880	889	rVB2	385	429	0.02%	0.003%
18	4.536	990	994	997	rBV2	653	584	0.03%	0.004%
19	4.620	1007	1020	1049	rBV	180880	454660	24.07%	3.467%
20	4.961	1122	1126	1129	rBV2	560	488	0.03%	0.004%
21	5.060	1140	1157	1185	rBV	346941	764852	40.49%	5.832%
22	5.157	1185	1187	1193	rBV3	500	435	0.02%	0.003%
23	5.282	1223	1226	1228	rBV3	731	561	0.03%	0.004%
24	5.369	1249	1253	1254	rBV	600	412	0.02%	0.003%
25	5.514	1293	1298	1300	rBV2	338	331	0.02%	0.003%
26	5.723	1341	1363	1393	rBV2	697905	1889042	100.00%	14.403%
27	6.038	1459	1461	1465	rVB4	504	342	0.02%	0.003%
28	6.125	1485	1488	1494	rVB2	558	498	0.03%	0.004%
29	6.163	1494	1500	1501	rBV	330	331	0.02%	0.003%
30	6.247	1510	1526	1549	rBV	485660	920705	48.74%	7.020%
31	6.420	1578	1580	1582	rBV3	767	448	0.02%	0.003%
32	6.530	1605	1614	1624	rBV6	4589	8360	0.44%	0.064%
33	6.687	1646	1663	1682	rBV	453677	886950	46.95%	6.763%
34	6.899	1726	1729	1733	rVB2	769	609	0.03%	0.005%
35	6.925	1733	1737	1740	rBV2	463	387	0.02%	0.003%
36	7.102	1789	1792	1797	rBV3	364	329	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
 Data File : VU051141.D
 Acq On : 05 Oct 2022 21:31
 Operator : JC/MD
 Sample : VU1005WBL02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK198

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	7.192	1811	1820	1824	rBV6	1954	3056	0.16%	0.023%
38	7.453	1895	1901	1906	rBV2	535	485	0.03%	0.004%
39	7.488	1907	1912	1916	rVB2	369	337	0.02%	0.003%
40	7.565	1922	1936	1960	rBV	202377	363961	19.27%	2.775%
41	7.793	2003	2007	2011	rBV3	1053	1031	0.05%	0.008%
42	7.896	2025	2039	2056	rBV	760902	1324564	70.12%	10.099%
43	8.179	2108	2127	2150	rBV	143365	251587	13.32%	1.918%
44	8.411	2197	2199	2204	rVB2	488	352	0.02%	0.003%
45	8.552	2233	2243	2251	rBV8	2792	4803	0.25%	0.037%
46	8.633	2255	2268	2308	rBV2	439202	984139	52.10%	7.504%
47	8.928	2355	2360	2366	rBV4	729	903	0.05%	0.007%
48	9.092	2407	2411	2415	rBV2	405	434	0.02%	0.003%
49	9.288	2468	2472	2474	rBV3	372	300	0.02%	0.002%
50	9.337	2483	2487	2491	rBV3	363	316	0.02%	0.002%
51	9.414	2498	2511	2539	rBV	705411	1178940	62.41%	8.989%
52	9.565	2555	2558	2566	rVB5	1197	1527	0.08%	0.012%
53	9.700	2592	2600	2607	rBV3	1542	2255	0.12%	0.017%
54	10.105	2717	2726	2729	rBV4	1250	1721	0.09%	0.013%
55	10.163	2740	2744	2747	rBV3	717	604	0.03%	0.005%
56	10.372	2803	2809	2811	rBV2	494	532	0.03%	0.004%
57	10.485	2838	2844	2850	rVV	807	958	0.05%	0.007%
58	10.575	2869	2872	2877	rBV2	454	370	0.02%	0.003%
59	10.642	2891	2893	2898	rVB2	511	459	0.02%	0.003%
60	10.671	2898	2902	2905	rBV2	392	329	0.02%	0.003%
61	10.755	2914	2928	2948	rBV	657139	1040745	55.09%	7.935%
62	10.919	2976	2979	2983	rBV	298	308	0.02%	0.002%
63	11.118	3039	3041	3043	rBV2	686	378	0.02%	0.003%
64	11.282	3090	3092	3098	rVV2	506	410	0.02%	0.003%
65	11.311	3098	3101	3107	rVB2	408	331	0.02%	0.003%
66	11.468	3145	3150	3157	rVV3	1206	1680	0.09%	0.013%
67	11.523	3162	3167	3171	rBV	506	503	0.03%	0.004%
68	11.610	3191	3194	3198	rBV	558	498	0.03%	0.004%
69	11.668	3207	3212	3215	rBV2	316	330	0.02%	0.003%
70	11.690	3215	3219	3221	rBV2	346	316	0.02%	0.002%
71	11.748	3230	3237	3243	rBV3	2120	2669	0.14%	0.020%
72	11.809	3244	3256	3277	rBV	497811	806263	42.68%	6.147%
73	11.964	3301	3304	3311	rVB4	654	565	0.03%	0.004%
74	12.038	3323	3327	3330	rBV2	522	526	0.03%	0.004%
75	12.108	3346	3349	3352	rBV2	428	303	0.02%	0.002%
76	12.192	3362	3375	3395	rBV	616040	1016902	53.83%	7.753%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
 Data File : VU051141.D
 Acq On : 05 Oct 2022 21:31
 Operator : JC/MD
 Sample : VU1005WBL02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK198

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	12.459	3456	3458	3462	rVB2	501	343	0.02%	0.003%
78	12.761	3548	3552	3555	rVV3	542	396	0.02%	0.003%
79	12.816	3564	3569	3570	rBV	555	429	0.02%	0.003%
80	12.874	3580	3587	3593	rVB3	623	781	0.04%	0.006%
81	12.906	3593	3597	3599	rBV	493	418	0.02%	0.003%
82	12.999	3620	3626	3633	rBV4	1307	1542	0.08%	0.012%
83	13.227	3690	3697	3704	rVB5	2019	3176	0.17%	0.024%
84	13.427	3754	3759	3761	rBV4	463	494	0.03%	0.004%
85	13.529	3789	3791	3797	rVB3	476	446	0.02%	0.003%
86	13.562	3798	3801	3806	rBV2	368	392	0.02%	0.003%
87	13.661	3829	3832	3834	rBV2	508	382	0.02%	0.003%
88	13.803	3874	3876	3881	rVB	581	448	0.02%	0.003%
89	13.845	3881	3889	3899	rBV6	4720	7990	0.42%	0.061%
90	14.028	3944	3946	3949	rBV3	523	363	0.02%	0.003%
91	14.092	3957	3966	3978	rBV	9388	15948	0.84%	0.122%
92	14.246	4011	4014	4016	rBV2	465	353	0.02%	0.003%
93	14.333	4033	4041	4053	rVV4	5474	9719	0.51%	0.074%
94	14.565	4110	4113	4115	rBV	598	464	0.02%	0.004%
95	14.697	4152	4154	4159	rBV2	645	516	0.03%	0.004%
96	15.166	4297	4300	4303	rBV3	536	466	0.02%	0.004%
97	15.301	4340	4342	4345	rBV3	639	440	0.02%	0.003%
98	15.340	4351	4354	4355	rBV2	819	452	0.02%	0.003%
99	15.623	4438	4442	4444	rBV3	1001	920	0.05%	0.007%
100	15.999	4556	4559	4560	rBV3	936	576	0.03%	0.004%




Sum of corrected areas: 13115529

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
Data File : VU051141.D
Acq On : 05 Oct 2022 21:31
Operator : JC/MD
Sample : VU1005WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK198

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

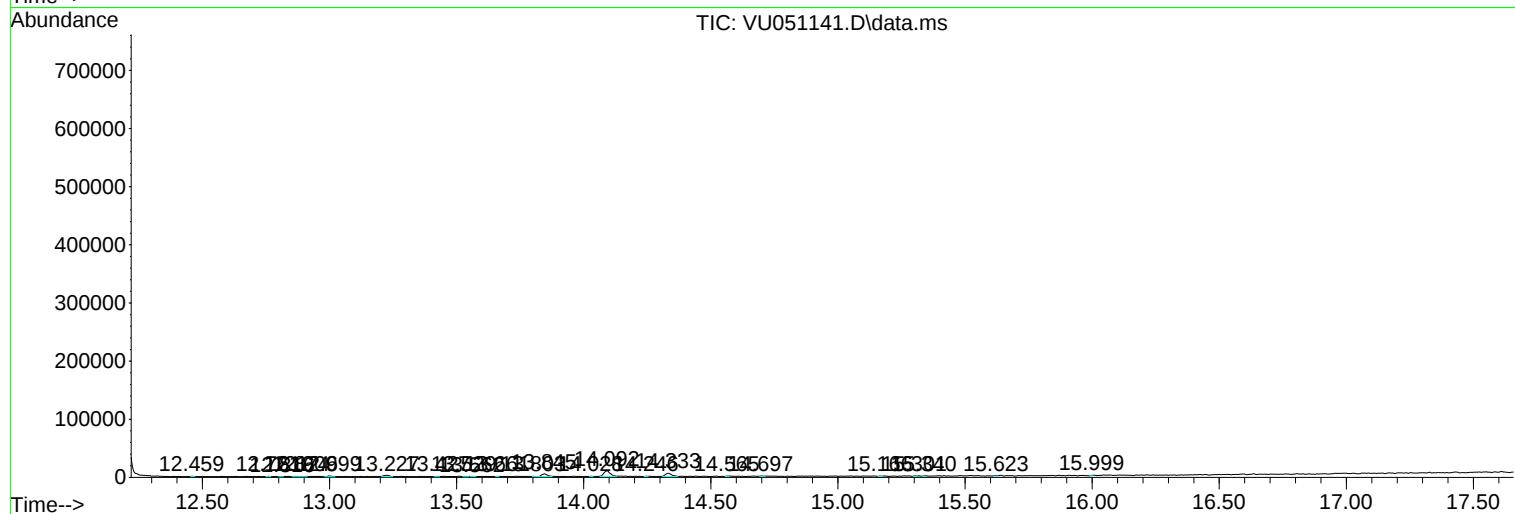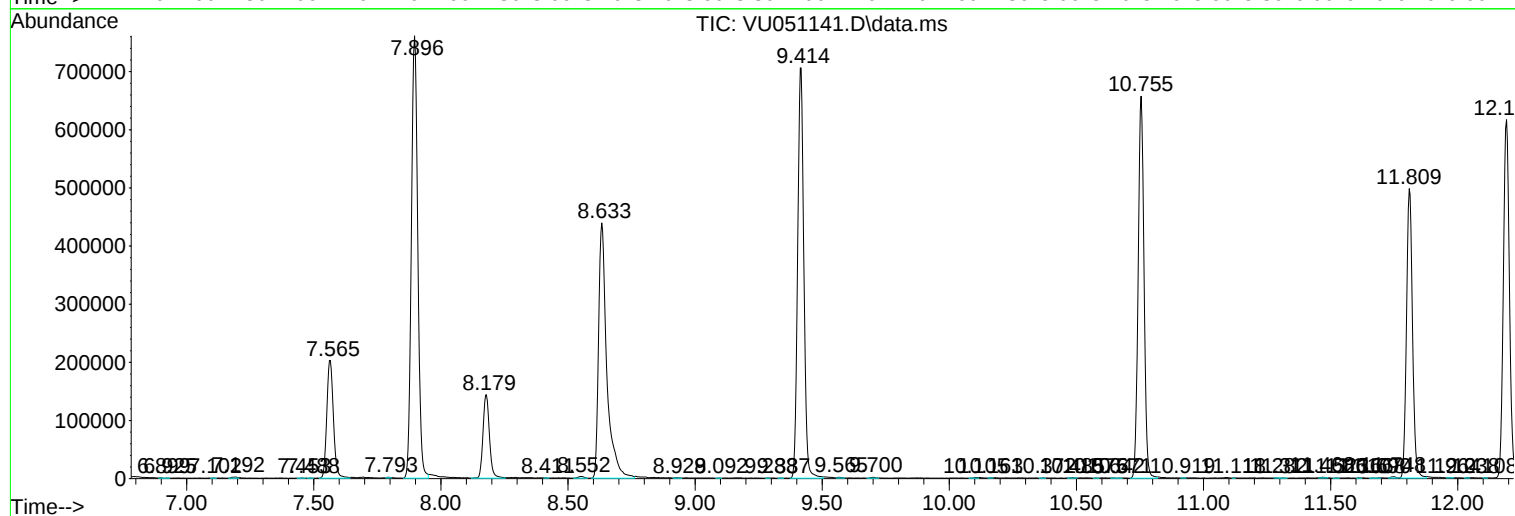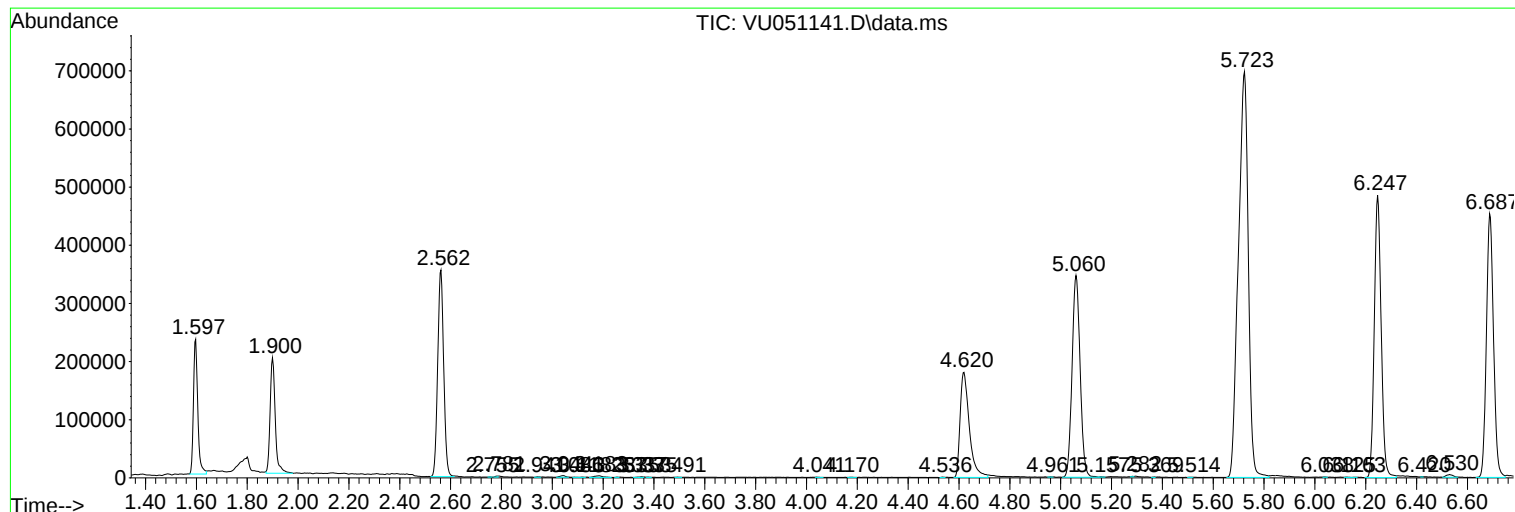

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
Data File : VU051141.D
Acq On : 05 Oct 2022 21:31
Operator : JC/MD
Sample : VU1005WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK198

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
Data File : VU051141.D
Acq On : 05 Oct 2022 21:31
Operator : JC/MD
Sample : VU1005WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK198

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------