

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
 Data File : VU051147.D
 Acq On : 05 Oct 2022 23:53
 Operator : JC/MD
 Sample : N4890-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY0E3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

Signal : TIC: VU051147.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	95	rVB	229977	258710	2.14%	0.918%
2	1.896	165	173	200	rVB	197519	269376	2.23%	0.955%
3	2.559	367	379	392	rBV	357731	586663	4.86%	2.081%
4	2.626	392	400	416	rVB	39243	67486	0.56%	0.239%
5	2.761	438	442	444	rBV3	974	663	0.01%	0.002%
6	2.781	444	448	450	rBV4	907	681	0.01%	0.002%
7	2.867	471	475	479	rVB3	458	387	0.00%	0.001%
8	2.890	479	482	485	rVB3	755	429	0.00%	0.002%
9	2.938	492	497	501	rBV2	662	770	0.01%	0.003%
10	2.961	501	504	507	rVB3	583	411	0.00%	0.001%
11	2.996	511	515	519	rVB4	557	519	0.00%	0.002%
12	3.038	523	528	538	rVB6	2314	3199	0.03%	0.011%
13	3.176	561	571	572	rBV5	2493	2529	0.02%	0.009%
14	3.327	614	618	621	rBV2	697	484	0.00%	0.002%
15	3.883	787	791	793	rVV3	476	421	0.00%	0.001%
16	4.121	860	865	869	rVB2	440	410	0.00%	0.001%
17	4.282	907	915	919	rBV2	301	425	0.00%	0.002%
18	4.436	955	963	965	rBV3	808	1008	0.01%	0.004%
19	4.620	1007	1020	1046	rBV	203218	507458	4.20%	1.800%
20	5.060	1139	1157	1179	rBV	352899	772755	6.40%	2.741%
21	5.247	1212	1215	1217	rBV3	567	429	0.00%	0.002%
22	5.440	1270	1275	1277	rBV2	515	425	0.00%	0.002%
23	5.462	1279	1282	1290	rVB2	525	384	0.00%	0.001%
24	5.723	1341	1363	1387	rBV2	745068	2006049	16.62%	7.115%
25	5.912	1420	1422	1427	rVB4	800	572	0.00%	0.002%
26	5.973	1437	1441	1442	rBV4	911	615	0.01%	0.002%
27	6.034	1457	1460	1464	rBV3	779	561	0.00%	0.002%
28	6.247	1511	1526	1548	rBV	592823	1122883	9.30%	3.983%
29	6.530	1604	1614	1624	rBV5	5159	10471	0.09%	0.037%
30	6.616	1639	1641	1647	rVB5	762	604	0.01%	0.002%
31	6.687	1647	1663	1679	rBV	476767	930266	7.70%	3.299%
32	6.977	1750	1753	1762	rVB7	1199	1510	0.01%	0.005%
33	7.038	1767	1772	1775	rBV3	478	491	0.00%	0.002%
34	7.115	1791	1796	1798	rBV3	847	739	0.01%	0.003%
35	7.182	1810	1817	1819	rBV7	2010	2446	0.02%	0.009%
36	7.237	1831	1834	1837	rVB3	993	652	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
 Data File : VU051147.D
 Acq On : 05 Oct 2022 23:53
 Operator : JC/MD
 Sample : N4890-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY0E3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

37	7.449	1896	1900	1905	rVB3	375	480	0.00%	0.002%
38	7.565	1923	1936	1953	rBV	231420	409470	3.39%	1.452%
39	7.687	1969	1974	1986	rVB8	1530	2904	0.02%	0.010%
40	7.793	2001	2007	2014	rVB5	1837	2482	0.02%	0.009%
41	7.896	2025	2039	2049	rBV	870101	1499151	12.42%	5.317%
42	7.967	2049	2061	2106	rVB	7105435	12073647	100.00%	42.822%
43	8.176	2117	2126	2142	rVB	165196	279148	2.31%	0.990%
44	8.468	2214	2217	2224	rVB5	1175	1144	0.01%	0.004%
45	8.549	2237	2242	2248	rVB5	2011	2446	0.02%	0.009%
46	8.632	2254	2268	2308	rBV3	535124	1146678	9.50%	4.067%
47	9.018	2383	2388	2391	rBV4	506	456	0.00%	0.002%
48	9.041	2391	2395	2399	rBV2	589	561	0.00%	0.002%
49	9.128	2418	2422	2427	rVB4	533	423	0.00%	0.002%
50	9.153	2427	2430	2433	rVV2	652	495	0.00%	0.002%
51	9.205	2443	2446	2449	rVV2	563	412	0.00%	0.001%
52	9.237	2454	2456	2462	rVB3	587	557	0.00%	0.002%
53	9.417	2498	2512	2536	rBV	811159	1361232	11.27%	4.828%
54	9.568	2548	2559	2576	rBV	158335	256264	2.12%	0.909%
55	9.690	2583	2597	2616	rBV	473038	773868	6.41%	2.745%
56	9.861	2646	2650	2655	rVB3	809	747	0.01%	0.003%
57	9.983	2685	2688	2694	rBV3	726	680	0.01%	0.002%
58	10.099	2711	2724	2737	rBV	94648	155350	1.29%	0.551%
59	10.240	2765	2768	2771	rBV4	768	608	0.01%	0.002%
60	10.356	2801	2804	2806	rBV2	671	441	0.00%	0.002%
61	10.481	2834	2843	2854	rBV	5355	8620	0.07%	0.031%
62	10.626	2884	2888	2890	rBV3	792	428	0.00%	0.002%
63	10.755	2913	2928	2954	rBV	699461	1124085	9.31%	3.987%
64	10.848	2954	2957	2962	rVB5	666	575	0.00%	0.002%
65	10.902	2962	2974	2985	rBV3	6635	11869	0.10%	0.042%
66	10.999	2996	3004	3023	rVB2	7795	17317	0.14%	0.061%
67	11.089	3025	3032	3043	rVB3	5079	8021	0.07%	0.028%
68	11.134	3044	3046	3050	rVB2	733	525	0.00%	0.002%
69	11.230	3066	3076	3087	rBV3	12564	20837	0.17%	0.074%
70	11.291	3089	3095	3105	rVV3	3481	5728	0.05%	0.020%
71	11.372	3115	3120	3123	rBV3	568	514	0.00%	0.002%
72	11.468	3139	3150	3168	rBV2	19647	34366	0.28%	0.122%
73	11.555	3170	3177	3190	rVB5	5799	8973	0.07%	0.032%
74	11.636	3198	3202	3213	rVB6	1363	2143	0.02%	0.008%
75	11.693	3213	3220	3223	rBV4	506	610	0.01%	0.002%
76	11.751	3229	3238	3244	rBV6	4704	7462	0.06%	0.026%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
 Data File : VU051147.D
 Acq On : 05 Oct 2022 23:53
 Operator : JC/MD
 Sample : N4890-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EY0E3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis

77	11.809	3244	3256	3272	rBV	679552	1081805	8.96%	3.837%
78	11.893	3277	3282	3295	rVB3	10622	17143	0.14%	0.061%
79	11.967	3302	3305	3308	rBV4	525	445	0.00%	0.002%
80	12.063	3327	3335	3342	rBV3	9499	16368	0.14%	0.058%
81	12.192	3361	3375	3399	rBV	761712	1234190	10.22%	4.377%
82	12.369	3427	3430	3431	rBV2	1322	762	0.01%	0.003%
83	12.533	3478	3481	3484	rBV3	780	716	0.01%	0.003%
84	12.571	3487	3493	3502	rVV6	3704	5854	0.05%	0.021%
85	12.610	3503	3505	3510	rVB5	866	773	0.01%	0.003%
86	12.671	3515	3524	3526	rBV4	973	1429	0.01%	0.005%
87	12.687	3526	3529	3535	rVV4	1132	1432	0.01%	0.005%
88	12.780	3555	3558	3562	rBV4	729	458	0.00%	0.002%
89	12.835	3572	3575	3578	rBV3	1037	902	0.01%	0.003%
90	12.877	3584	3588	3602	rVB8	2388	3822	0.03%	0.014%
91	12.973	3612	3618	3628	rBV6	2616	4125	0.03%	0.015%
92	13.025	3629	3634	3644	rVB5	2013	2754	0.02%	0.010%
93	13.221	3691	3695	3701	rBV4	968	1100	0.01%	0.004%
94	13.391	3740	3748	3750	rBV3	719	950	0.01%	0.003%
95	13.452	3759	3767	3779	rVB4	5367	8891	0.07%	0.032%
96	13.626	3814	3821	3830	rVB7	2615	3966	0.03%	0.014%
97	13.725	3850	3852	3858	rVB4	574	509	0.00%	0.002%
98	14.092	3957	3966	3978	rBV2	17691	30052	0.25%	0.107%
99	14.680	4146	4149	4150	rBV2	724	389	0.00%	0.001%
100	14.719	4159	4161	4165	rBV4	731	562	0.00%	0.002%




Sum of corrected areas: 28194995

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
Data File : VU051147.D
Acq On : 05 Oct 2022 23:53
Operator : JC/MD
Sample : N4890-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY0E3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

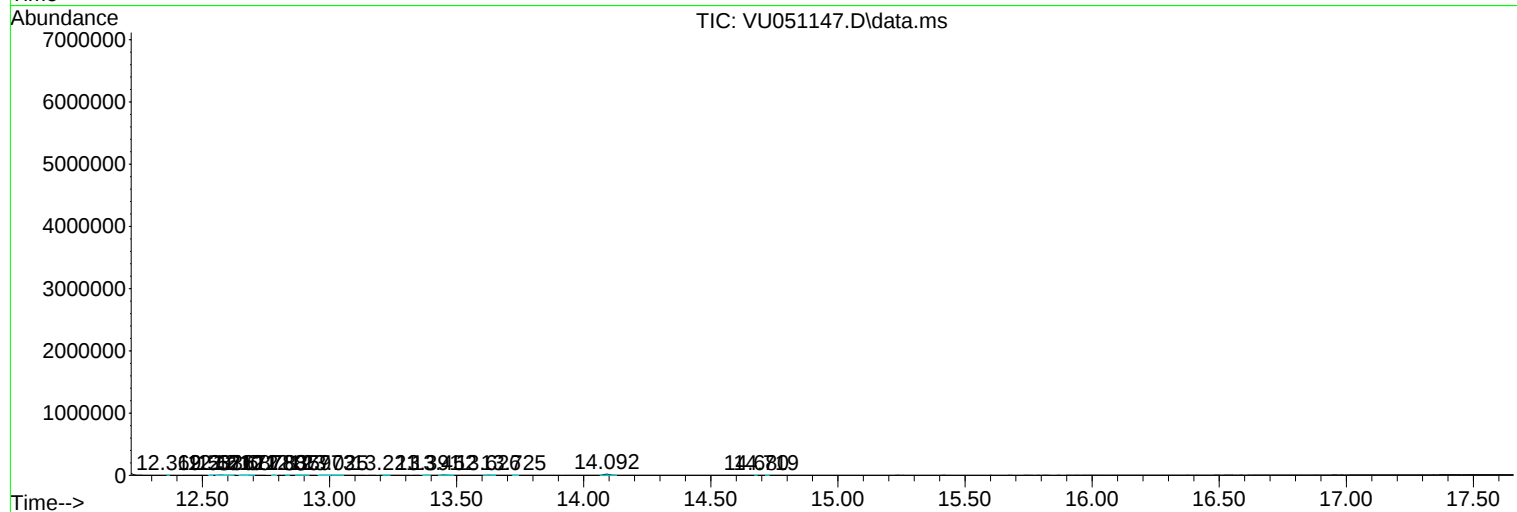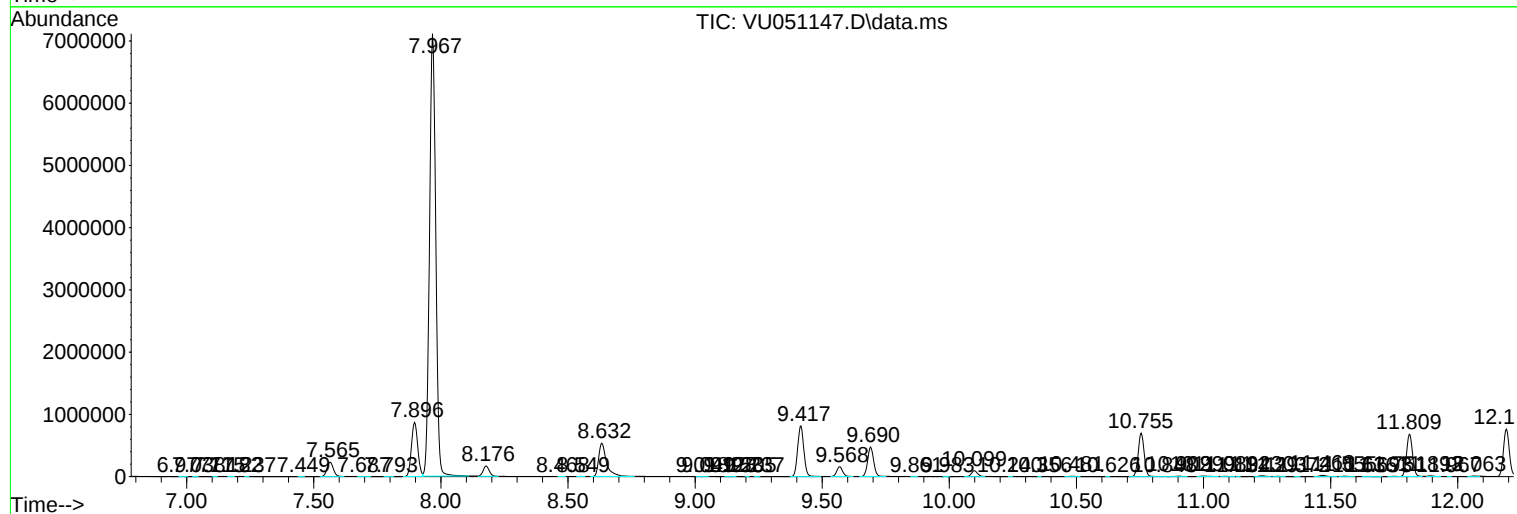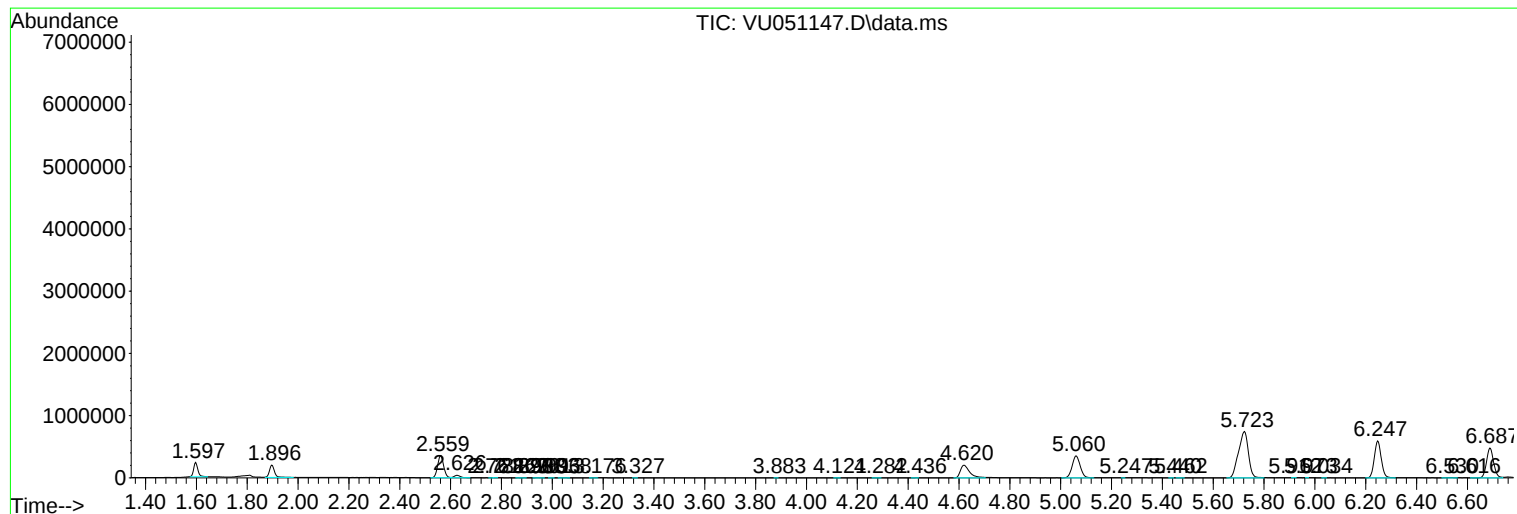

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
Data File : VU051147.D
Acq On : 05 Oct 2022 23:53
Operator : JC/MD
Sample : N4890-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY0E3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
Data File : VU051147.D
Acq On : 05 Oct 2022 23:53
Operator : JC/MD
Sample : N4890-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EY0E3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc