
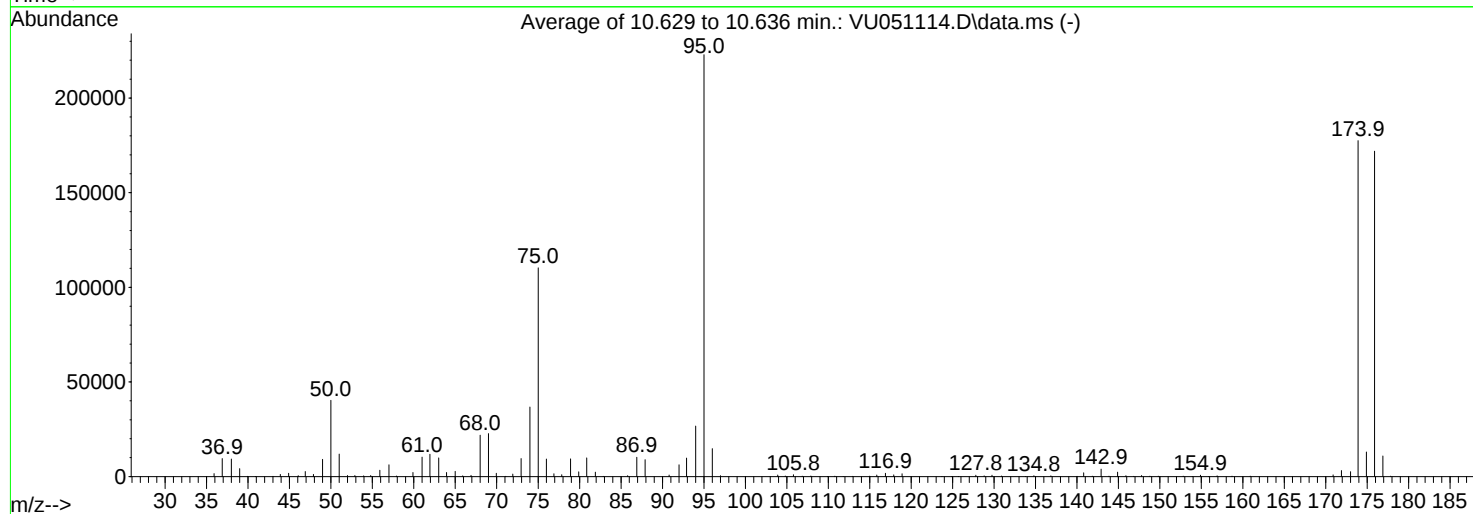


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU100522\
 Data File : VU051114.D
 Acq On : 05 Oct 2022 09:14
 Operator : JC/MD
 Sample : BFB136
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB136

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM092922WMA.M
 Title : VOC Analysis
 Last Update : Fri Oct 07 02:51:40 2022

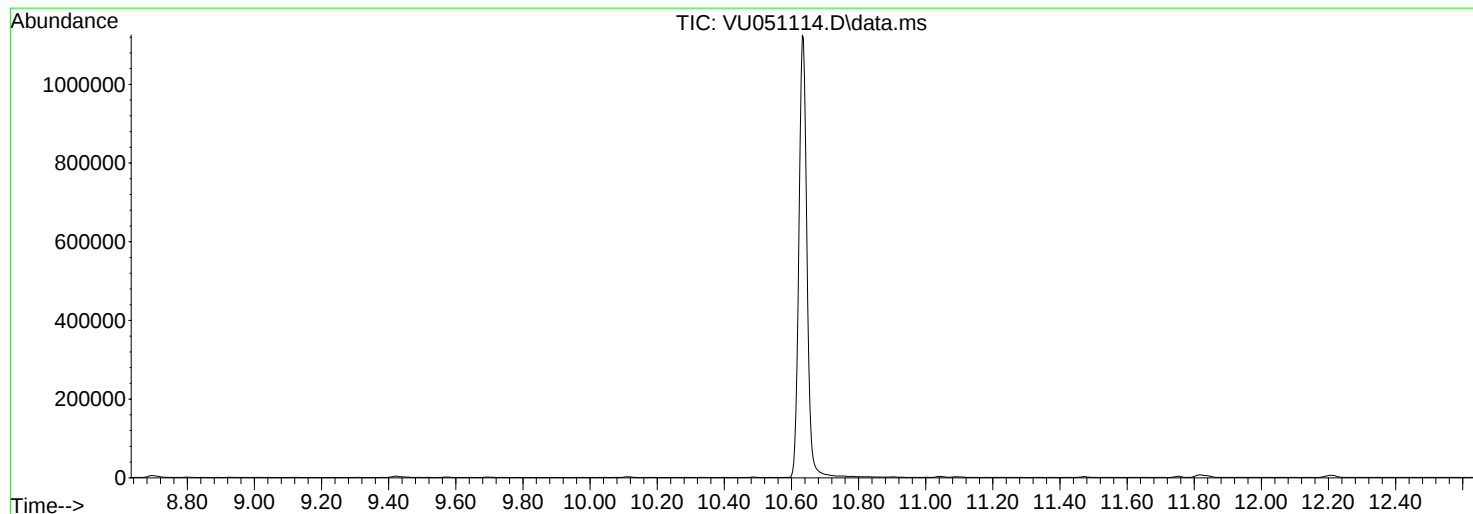

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	40267	PASS
75	95	30	80	49.5	110323	PASS
95	95	100	100	100.0	222869	PASS
96	95	5	9	6.6	14792	PASS
173	174	0.00	2	1.5	2585	PASS
174	95	50	120	79.6	177472	PASS
175	174	5	9	7.3	12981	PASS
176	174	95	101	96.9	171925	PASS
177	176	5	9	6.3	10855	PASS

m/z	Abundance
39.90	300.0
43.90	566.0

Instrument :
MSVOA_U
ClientSampleId :
BFB136

m/z	Abundance
35.90	1536.0
36.90	9206.0
38.00	9113.0
39.00	4050.0
40.00	395.0
43.00	127.0
44.00	1740.0
44.90	1581.0
46.00	470.0
46.90	2526.0
47.90	1189.0
49.00	8660.0
50.00	38560.0
51.00	11229.0
52.00	571.0
52.90	569.0
54.00	297.0
54.80	548.0
55.90	3247.0
57.00	5948.0
57.90	288.0
59.90	2012.0
61.00	9917.0
62.00	11585.0
63.00	9738.0
63.90	2032.0
65.00	2545.0
65.90	282.0
66.90	529.0
68.00	20880.0
69.00	21672.0
70.00	1675.0
71.10	159.0
72.00	1189.0
72.90	9511.0
74.00	35240.0
75.00	105224.0
76.00	9050.0
76.90	1567.0
77.80	900.0
78.90	9196.0
79.90	2160.0
80.90	9655.0
81.90	2119.0
82.80	189.0
85.80	508.0
86.90	9856.0
87.90	8357.0
90.80	751.0
92.00	5846.0
92.90	9310.0
94.00	24808.0
95.00	211008.0
96.00	13946.0
97.00	459.0
103.90	739.0
104.80	280.0
105.80	877.0
106.90	207.0
108.00	271.0
110.80	208.0
112.90	151.0
115.00	214.0
115.80	767.0
116.90	1721.0
117.90	811.0
118.90	1309.0
127.80	683.0
128.80	451.0
129.80	711.0
130.90	357.0
134.80	478.0
136.90	379.0
140.00	110.0
140.80	1749.0
141.80	234.0
142.90	3767.0
143.80	258.0
144.90	2339.0
145.90	421.0
146.90	124.0
147.80	517.0
148.80	191.0
149.70	225.0
152.80	238.0
154.90	673.0
156.90	361.0
158.60	165.0
160.90	186.0
170.90	877.0
171.90	2834.0
173.00	2556.0

Instrument :
MSVOA_U
ClientSampleId :
BFB136

173.90	163776.0
174.90	12520.0
175.90	159616.0
176.90	10490.0
177.80	226.0

Instrument :
MSVOA_U
ClientSampleId :
BFB136

m/z	Abundance
35.90	1630.0
36.90	9851.0
38.00	9549.0
39.00	4376.0
40.10	480.0
43.00	171.0
44.00	1856.0
44.90	1756.0
46.00	465.0
46.90	2724.0
47.90	1191.0
49.00	9409.0
50.00	41696.0
51.00	12229.0
52.00	594.0
52.90	585.0
54.00	369.0
54.80	564.0
55.90	3444.0
57.00	6470.0
57.90	299.0
59.90	2225.0
61.00	10594.0
62.00	12103.0
63.00	10181.0
63.90	2254.0
65.00	2893.0
65.90	410.0
66.90	653.0
68.00	22416.0
69.00	23456.0
70.00	1725.0
71.10	121.0
72.00	1306.0
72.90	9731.0
74.00	37896.0
75.00	113944.0
76.00	9432.0
76.90	1534.0
77.90	964.0
78.90	9590.0
79.90	2517.0
80.80	10157.0
81.90	2393.0
82.80	183.0
85.80	508.0
86.90	10473.0
87.90	9140.0
90.80	840.0
92.00	6357.0
92.90	9905.0
94.00	27736.0
95.00	229760.0
96.00	15358.0
97.00	510.0
103.90	849.0
104.80	330.0
105.80	1002.0
106.80	261.0
107.90	298.0
110.80	253.0
111.80	108.0
112.90	145.0
115.00	268.0
115.80	874.0
116.90	1798.0
117.90	922.0
118.90	1474.0
123.70	131.0
127.80	802.0
128.80	443.0
129.70	769.0
130.90	357.0
134.80	501.0
136.90	382.0
140.00	156.0
140.80	2075.0
141.90	205.0
142.90	4077.0
143.90	214.0
144.90	2482.0
145.90	506.0
146.80	161.0
147.80	575.0
148.80	202.0
149.80	200.0
152.80	190.0
154.90	731.0
155.90	111.0
156.90	374.0
158.70	184.0
160.90	232.0

Instrument :
MSVOA_U
ClientSampleId :
BFB136

170.90	902.0
171.90	3275.0
173.00	2648.0
173.90	182976.0
174.90	13346.0
175.90	177280.0
176.90	11207.0
177.80	225.0

Instrument :
MSVOA_U
ClientSampleId :
BFB136

m/z	Abundance
35.90	1653.0
36.90	9520.0
38.00	9062.0
39.00	4249.0
40.00	544.0
40.90	125.0
43.00	184.0
43.90	1633.0
44.90	1785.0
46.10	390.0
46.90	2694.0
47.90	1121.0
49.00	9282.0
50.00	40544.0
51.00	12314.0
52.00	550.0
52.90	472.0
53.90	392.0
54.80	561.0
55.90	3247.0
57.00	6246.0
57.90	255.0
59.90	2257.0
61.00	10386.0
61.90	11708.0
63.00	9760.0
64.00	2332.0
65.00	2797.0
65.90	419.0
66.90	657.0
68.00	22168.0
69.00	23056.0
69.90	1689.0
71.90	1339.0
73.00	9299.0
74.00	37176.0
75.00	111800.0
76.00	9403.0
76.90	1371.0
77.90	954.0
78.90	9182.0
79.90	2708.0
80.80	9779.0
81.90	2419.0
82.90	152.0
85.80	437.0
86.90	10227.0
87.90	9224.0
90.80	876.0
92.00	6468.0
92.90	9970.0
94.00	27376.0
95.00	227840.0
96.00	15072.0
97.00	502.0
103.90	908.0
104.80	311.0
105.80	998.0
106.80	254.0
107.80	272.0
109.90	129.0
110.80	265.0
113.00	136.0
115.00	275.0
115.90	920.0
116.90	1766.0
117.90	965.0
118.90	1562.0
123.70	130.0
124.90	101.0
125.70	104.0
127.80	791.0
128.80	400.0
129.80	714.0
130.90	275.0
133.80	110.0
134.80	419.0
136.80	331.0
140.00	174.0
140.80	2217.0
141.90	185.0
142.90	4049.0
143.80	179.0
144.90	2226.0
145.90	536.0
146.80	171.0
147.80	568.0
148.80	174.0
149.90	181.0
152.90	119.0
153.90	108.0
154.90	675.0

Instrument :
MSVOA_U
ClientSampleId :
BFB136

155.90	125.0
156.90	372.0
158.80	234.0
160.90	215.0
170.90	840.0
171.90	3473.0
173.00	2552.0
173.90	185664.0
174.90	13078.0
175.90	178880.0
176.90	10868.0
177.90	213.0

Instrument :
MSVOA_U
ClientSampleId :
BFB136