

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101124\
 Data File : VU061113.D
 Acq On : 11 Oct 2024 13:00
 Operator : MD/SY
 Sample : P4380-21
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E27G6

Manual Integrations
 APPROVED

Reviewed By :Mahesh Dadoda 10/14/2024
 Supervised By :Semsettin Yesilyurt 10/14/2024

Quant Time: Oct 14 04:18:44 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100124WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Oct 11 06:46:55 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.277	114	154857	5.000	ug/L	0.04
28) Chlorobenzene-d5	9.418	117	144606	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	69727	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.605	65	40181	3.629	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	72.600%
7) Chloroethane-d5	1.930	69	35286	4.258	ug/L	0.02
Spiked Amount	5.000	Range	65 - 130	Recovery	=	85.200%
11) 1,1-Dichloroethene-d2	2.573	65	19572	4.007	ug/L	0.01
Spiked Amount	5.000	Range	60 - 125	Recovery	=	80.200%
20) 2-Butanone-d5	4.734	46	112709	42.499	ug/L	0.11
Spiked Amount	50.000	Range	40 - 130	Recovery	=	85.000%
24) Chloroform-d	5.091	84	87916	4.506	ug/L	0.04
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.200%
26) 1,2-Dichloroethane-d4	5.743	65	45408	4.390	ug/L	0.05
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.800%
32) Benzene-d6	5.763	84	171435	4.496	ug/L	0.04
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.000%
36) 1,2-Dichloropropane-d6	6.714	67	58609	4.681	ug/L	0.03
Spiked Amount	5.000	Range	60 - 140	Recovery	=	93.600%
41) Toluene-d8	7.907	98	156873	4.402	ug/L	0.02
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.000%
43) trans-1,3-Dichloroprop...	8.187	79	22018	4.112	ug/L	0.01
Spiked Amount	5.000	Range	55 - 130	Recovery	=	82.200%
46) 2-Hexanone-d5	8.644	63	106469	48.044	ug/L	0.02
Spiked Amount	50.000	Range	45 - 130	Recovery	=	96.080%
56) 1,1,2,2-Tetrachloroeth...	10.753	84	41651	4.536	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	90.800%
66) 1,2-Dichlorobenzene-d4	12.187	152	53991	4.843	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	96.800%
Target Compounds						
3) Chloromethane	1.525	50	1562	0.143	ug/L	91
8) Chloroethane	1.930	64	35156	5.297	ug/L #	52
14) Carbon disulfide	2.795	76	6550	0.216	ug/L #	84
42) Toluene	7.984	91	5008	0.110	ug/L	98
62) 1,3,5-Trimethylbenzene	11.084	105	5401	0.131	ug/L	93
63) 1,2,4-Trimethylbenzene	11.470	105	2933m	0.071	ug/L	
70) 1,2,4-trichlorobenzene	13.833	180	7708	0.715	ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101124\
Data File : VU061113.D
Acq On : 11 Oct 2024 13:00
Operator : MD/SY
Sample : P4380-21
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1


Instrument :
MSVOA_U
ClientSampleId :
E27G6

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 10/14/2024
Supervised By :Semsettin Yesilyurt 10/14/2024


Quant Time: Oct 14 04:18:44 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100124WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Oct 11 06:46:55 2024
Response via : Initial Calibration

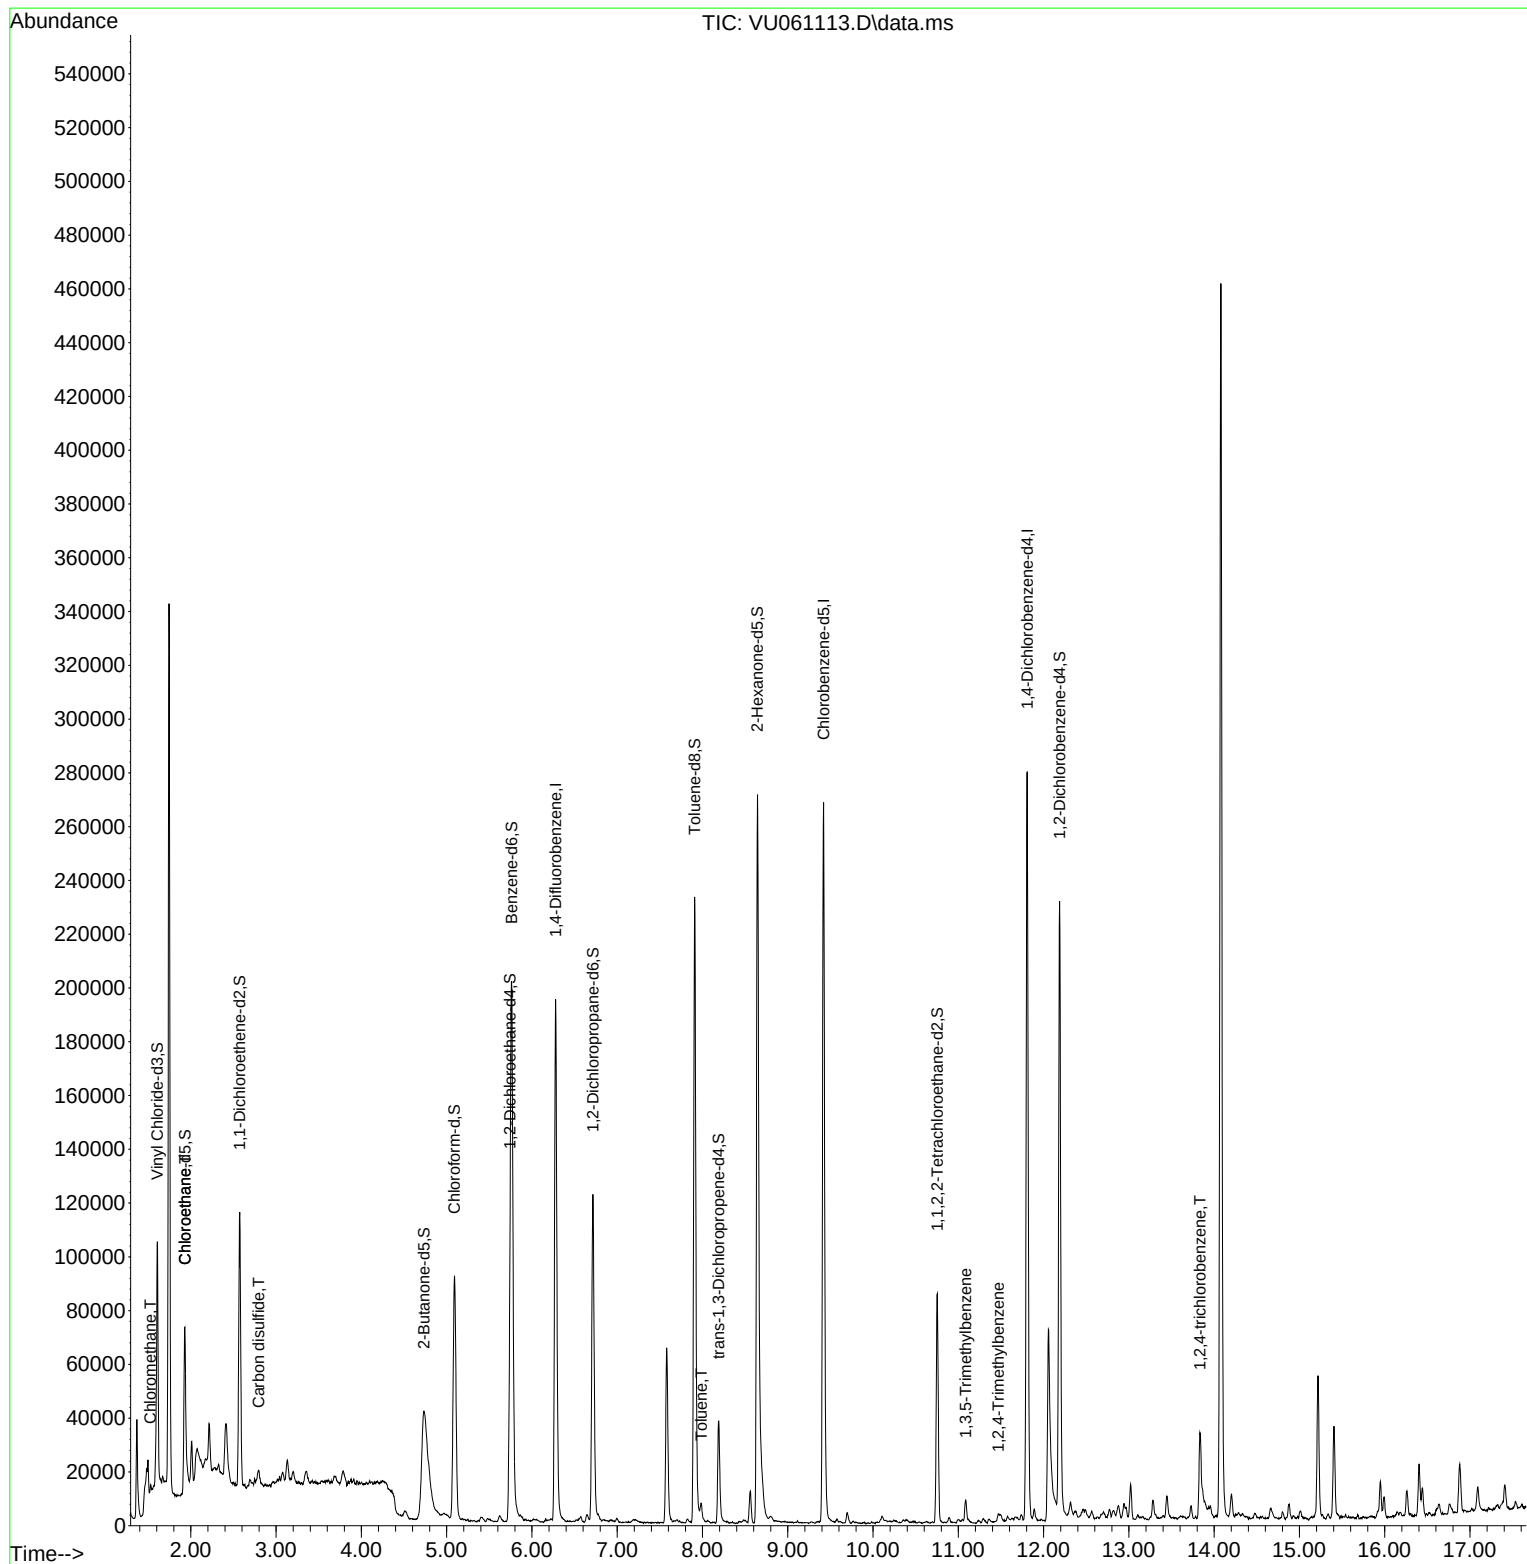

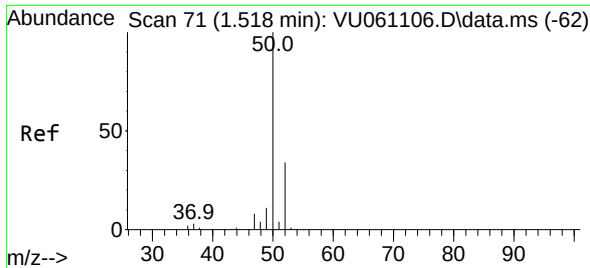

#3
Chloromethane
Concen: 0.143 ug/L
RT: 1.525 min Scan# 71
Delta R.T. 0.007 min
Lab File: VU061113.D
Acq: 11 Oct 2024 13:00




Instrument :
MSVOA_U
ClientSampleId :
E27G6

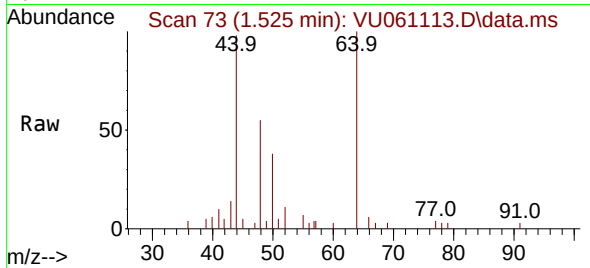

Tgt Ion: 50 Resp: 1562
Ion Ratio Lower Upper
50 100
52 30.0 24.4 45.4




Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 10/14/2024
Supervised By :Semsettin Yesilyurt 10/14/2024

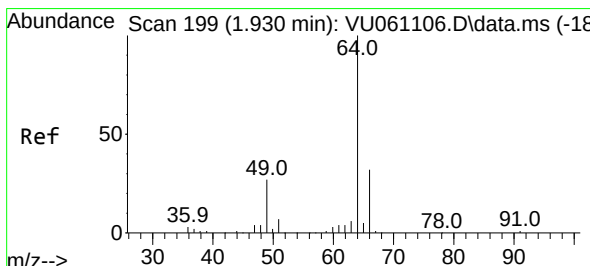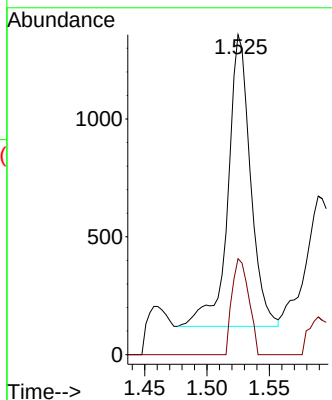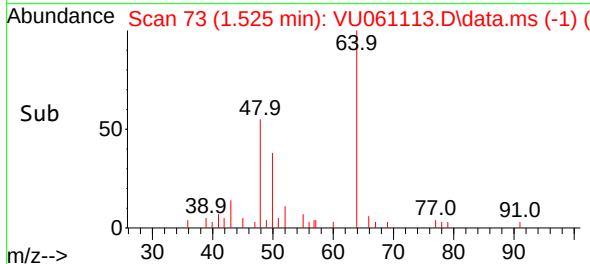

#8
Chloroethane
Concen: 5.297 ug/L
RT: 1.930 min Scan# 199
Delta R.T. 0.000 min
Lab File: VU061113.D
Acq: 11 Oct 2024 13:00


Tgt Ion: 64 Resp: 35156
Ion Ratio Lower Upper
64 100
66 5.0 22.3 41.3#

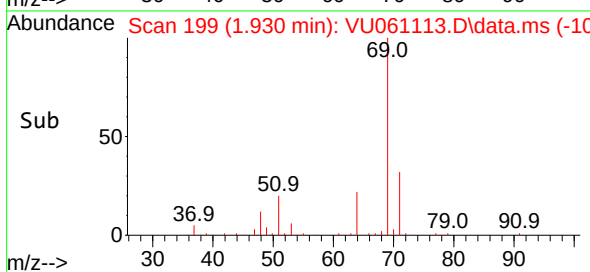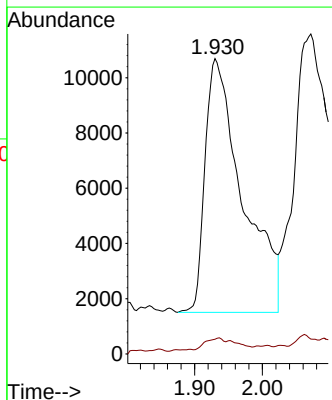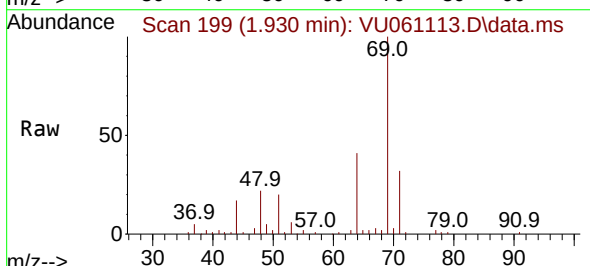

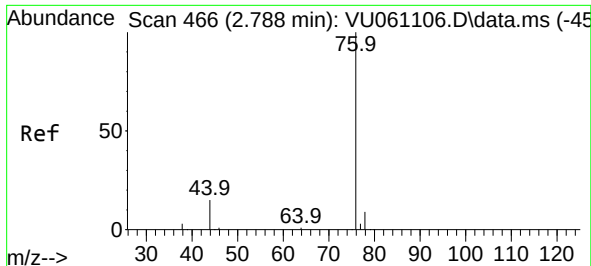

#14
Carbon disulfide
Concen: 0.216 ug/L
RT: 2.795 min Scan# 40
Delta R.T. 0.007 min
Lab File: VU061113.D
Acq: 11 Oct 2024 13:00




Instrument :
MSVOA_U
ClientSampleId :
E27G6

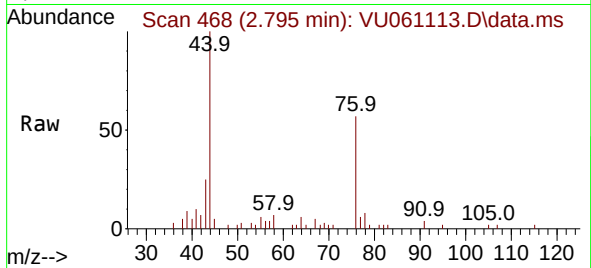

Tgt Ion: 76 Resp: 6550
Ion Ratio Lower Upper
76 100
78 14.7 7.1 10.7




Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 10/14/2024
Supervised By :Semsettin Yesilyurt 10/14/2024

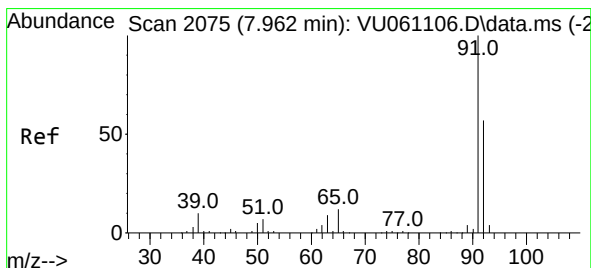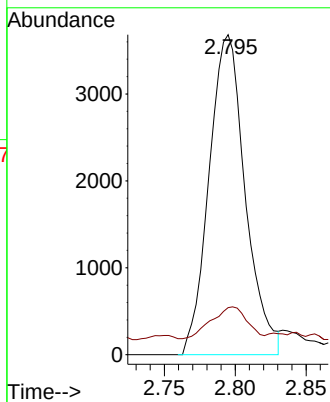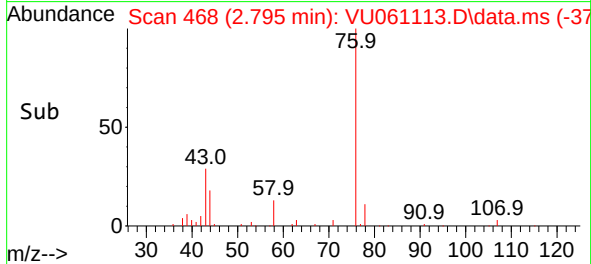

#42
Toluene
Concen: 0.110 ug/L
RT: 7.984 min Scan# 2082
Delta R.T. 0.023 min
Lab File: VU061113.D
Acq: 11 Oct 2024 13:00

Tgt Ion: 91 Resp: 5008
Ion Ratio Lower Upper
91 100
92 56.3 40.5 75.3

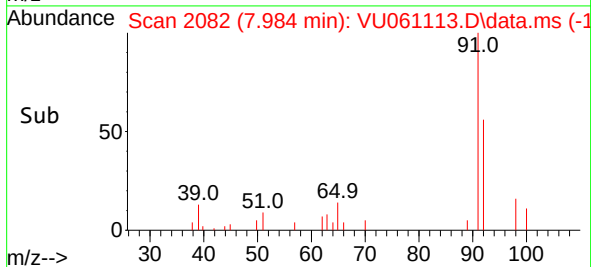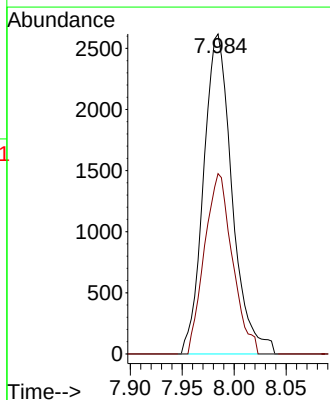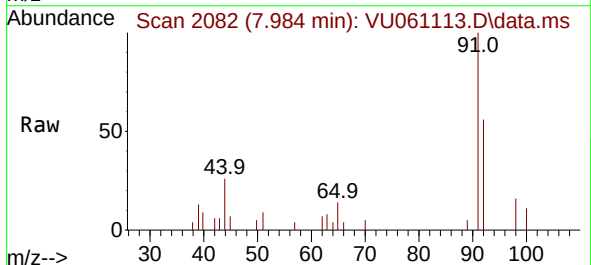

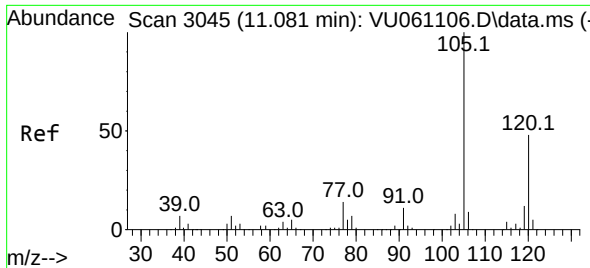





#62
1,3,5-Trimethylbenzene
Concen: 0.131 ug/L
RT: 11.084 min Scan# 3045
Delta R.T. 0.003 min
Lab File: VU061113.D
Acq: 11 Oct 2024 13:00

Instrument :
MSVOA_U
ClientSampleId :
E27G6

Tgt Ion:105 Resp: 540
Ion Ratio Lower Upper
105 100
120 43.5 38.5 57.7




Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 10/14/2024
Supervised By :Semsettin Yesilyurt 10/14/2024

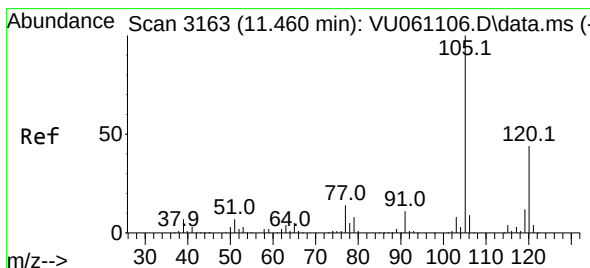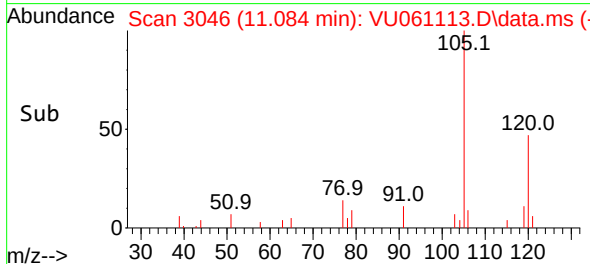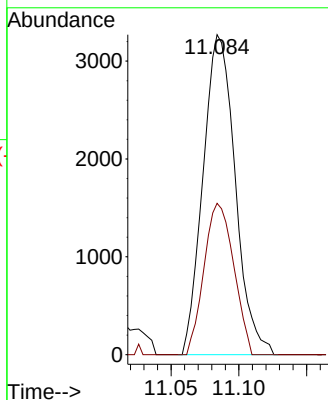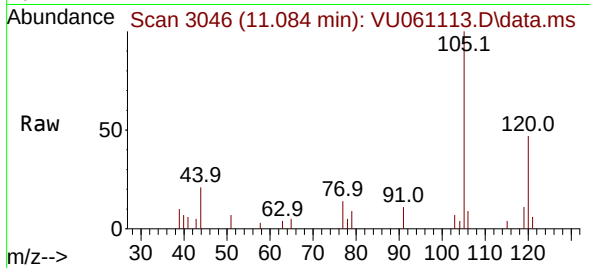

#63
1,2,4-Trimethylbenzene
Concen: 0.071 ug/L m
RT: 11.470 min Scan# 3166
Delta R.T. 0.010 min
Lab File: VU061113.D
Acq: 11 Oct 2024 13:00


Tgt Ion:105 Resp: 2933
Ion Ratio Lower Upper
105 100
120 80.1 36.1 54.1#

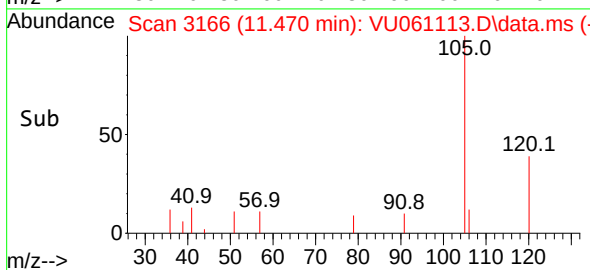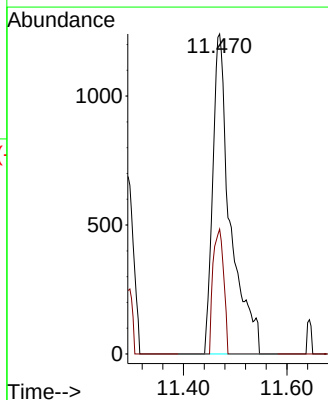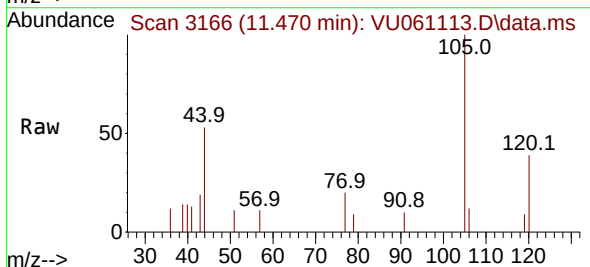

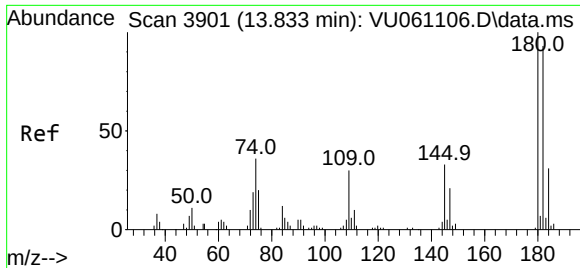

#70
 1,2,4-trichlorobenzene
 Concen: 0.715 ug/L
 RT: 13.833 min Scan# 3901
 Delta R.T. -0.003 min
 Lab File: VU061113.D
 Acq: 11 Oct 2024 13:00

Instrument :
 MSVOA_U
 ClientSampleId :
 E27G6

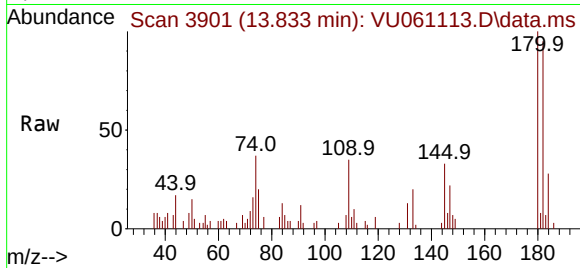

Tgt Ion:180 Resp: 7708
 Ion Ratio Lower Upper
 180 100
 182 93.7 77.4 116.2
 145 33.6 22.9 34.3

Manual Integrations
 APPROVED

Reviewed By :Mahesh Dadoda 10/14/2024
 Supervised By :Semsettin Yesilyurt 10/14/2024

