

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101124\
 Data File : VU061116.D
 Acq On : 11 Oct 2024 14:13
 Operator : MD/SY
 Sample : VIBLK148
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK148

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100124WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU061116.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	86	95	110	rBV	60712	69569	12.01%	1.491%
2	1.911	184	193	202	rBV	49819	66522	11.48%	1.426%
3	2.560	384	395	412	rBV	97304	159159	27.47%	3.411%
4	4.624	1023	1037	1074	rBV	78701	227755	39.31%	4.881%
5	5.052	1154	1170	1192	rBV	92483	211747	36.54%	4.538%
6	5.718	1357	1377	1412	rBV2	188441	496867	85.75%	10.648%
7	6.242	1527	1540	1572	rBV	200731	396542	68.43%	8.498%
8	6.682	1661	1677	1707	rBV	120627	243358	42.00%	5.215%
9	7.560	1936	1950	1972	rBV2	63260	116936	20.18%	2.506%
10	7.891	2039	2053	2078	rBV	229263	415148	71.65%	8.896%
11	8.174	2127	2141	2168	rBV	36707	69629	12.02%	1.492%
12	8.627	2266	2282	2325	rBV	284393	579445	100.00%	12.417%
13	9.409	2513	2525	2564	rBV	274531	484219	83.57%	10.377%
14	10.750	2929	2942	2960	rBV	85293	142454	24.58%	3.053%
15	11.804	3256	3270	3292	rBV	286891	475247	82.02%	10.184%
16	12.187	3377	3389	3412	rBV	212026	356736	61.57%	7.645%
17	14.084	3968	3979	4006	rVB	69810	126981	21.91%	2.721%
18	15.228	4325	4335	4350	rBV	10625	19218	3.32%	0.412%
19	15.412	4381	4392	4404	rBV	5419	8956	1.55%	0.192%




Sum of corrected areas: 4666488

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101124\
Data File : VU061116.D
Acq On : 11 Oct 2024 14:13
Operator : MD/SY
Sample : VIBLK148
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK148

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100124WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

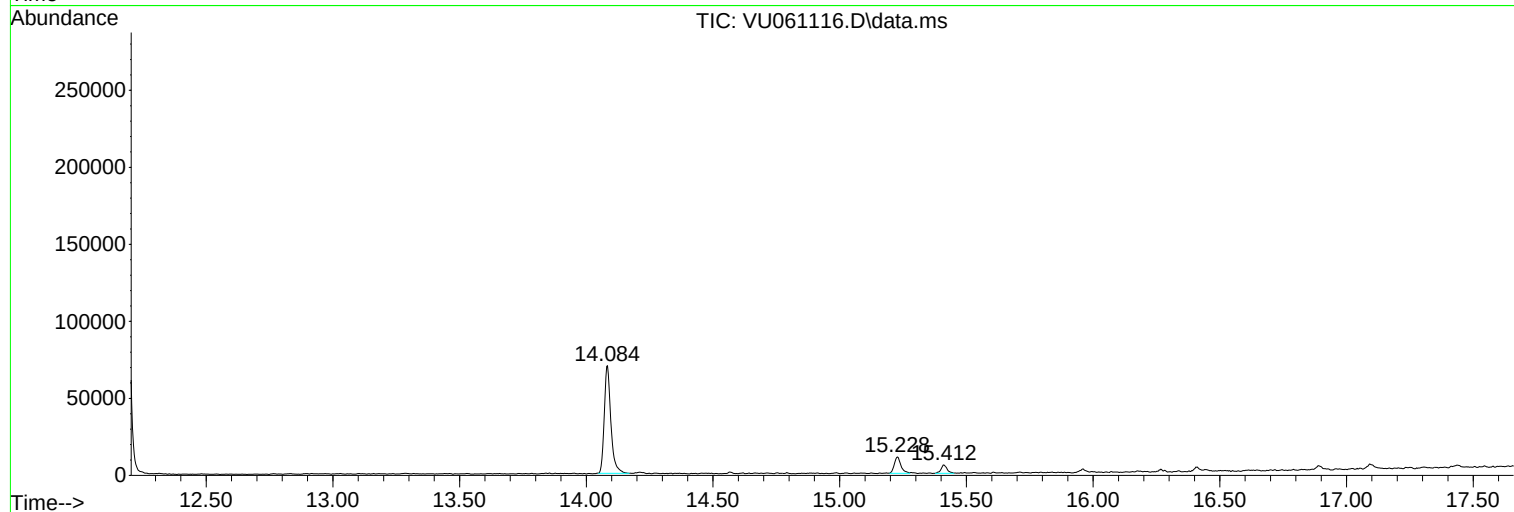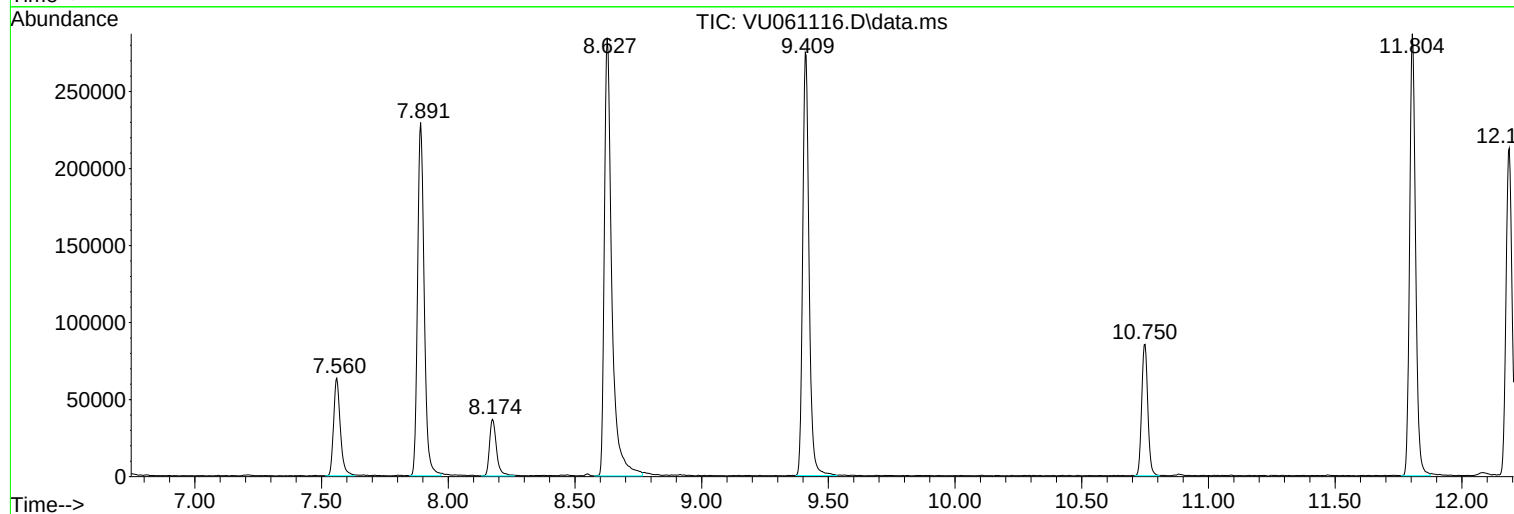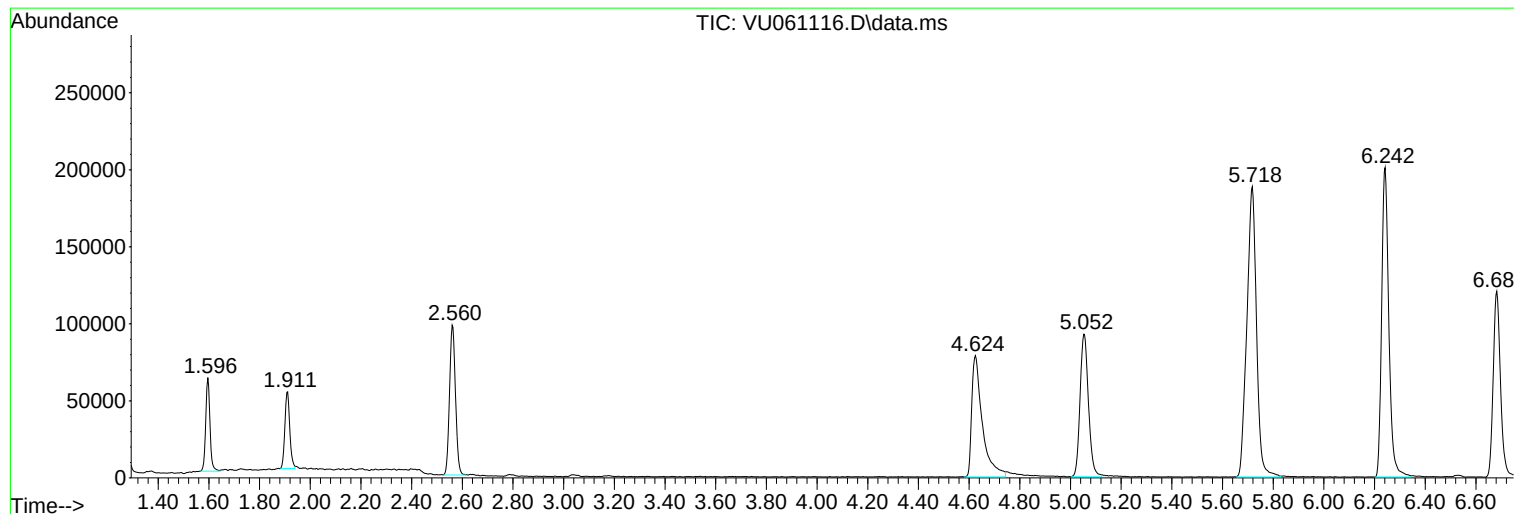

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101124\
Data File : VU061116.D
Acq On : 11 Oct 2024 14:13
Operator : MD/SY
Sample : VIBLK148
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK148










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100124WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 1H-Indene, 1-methylene- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.084	1.34 ug/L	126981	1,4-Dichlorobenzene-d4	11.804

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Naphthalene	128	C10H8	000091-20-3	95
2			1H-Indene, 1-methylene-	128	C10H8	002471-84-3	95
3			Naphthalene	128	C10H8	000091-20-3	94
4			Azulene	128	C10H8	000275-51-4	91
5			Azulene	128	C10H8	000275-51-4	91

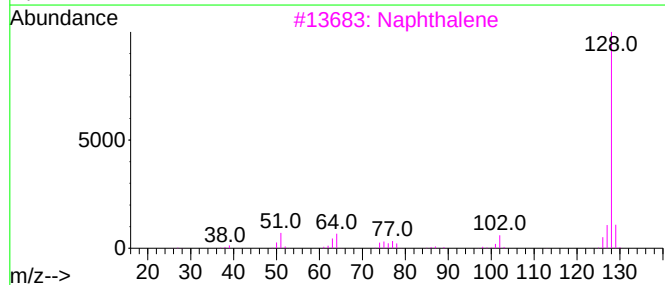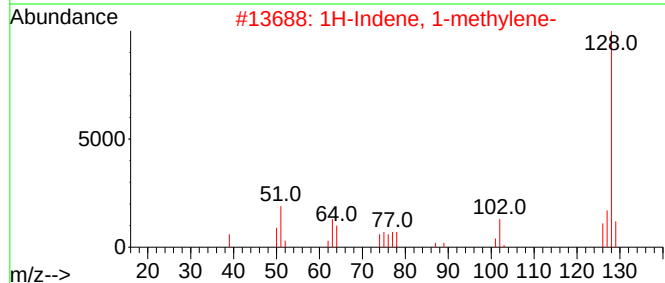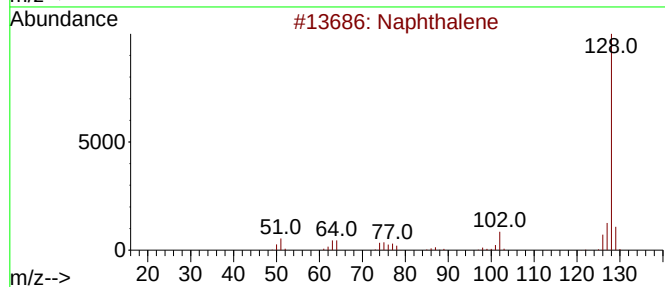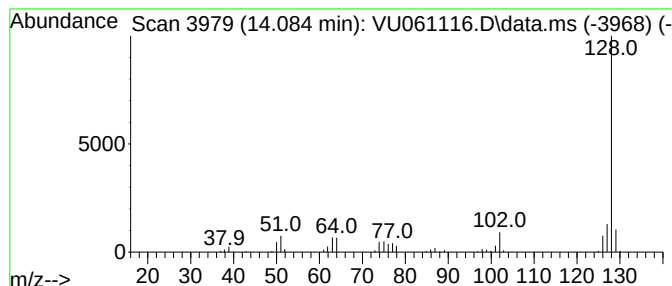

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101124\
Data File : VU061116.D
Acq On : 11 Oct 2024 14:13
Operator : MD/SY
Sample : VIBLK148
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK148

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR100124WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
1H-Indene, 1-me...	14.084	1.3	ug/L	126981	3	11.804	475247	5.0