

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101824\
 Data File : VU061157.D
 Acq On : 18 Oct 2024 11:34
 Operator : MD/SY
 Sample : VU1018WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU1018WBL01

Quant Time: Oct 18 23:57:57 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U101724DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Fri Oct 18 02:52:28 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.110	96	27857	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.634	95	12725	0.860	ug/l	0.00
Spiked Amount 1.000			Recovery	=	86.000%	
68) 1,2-Dichlorobenzene-d4	12.190	152	12051	0.826	ug/l	0.00
Spiked Amount 1.000			Recovery	=	83.000%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU101824\
Data File : VU061157.D
Acq On : 18 Oct 2024 11:34
Operator : MD/SY
Sample : VU1018WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU1018WBL01

Quant Time: Oct 18 23:57:57 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U101724DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Fri Oct 18 02:52:28 2024
Response via : Initial Calibration




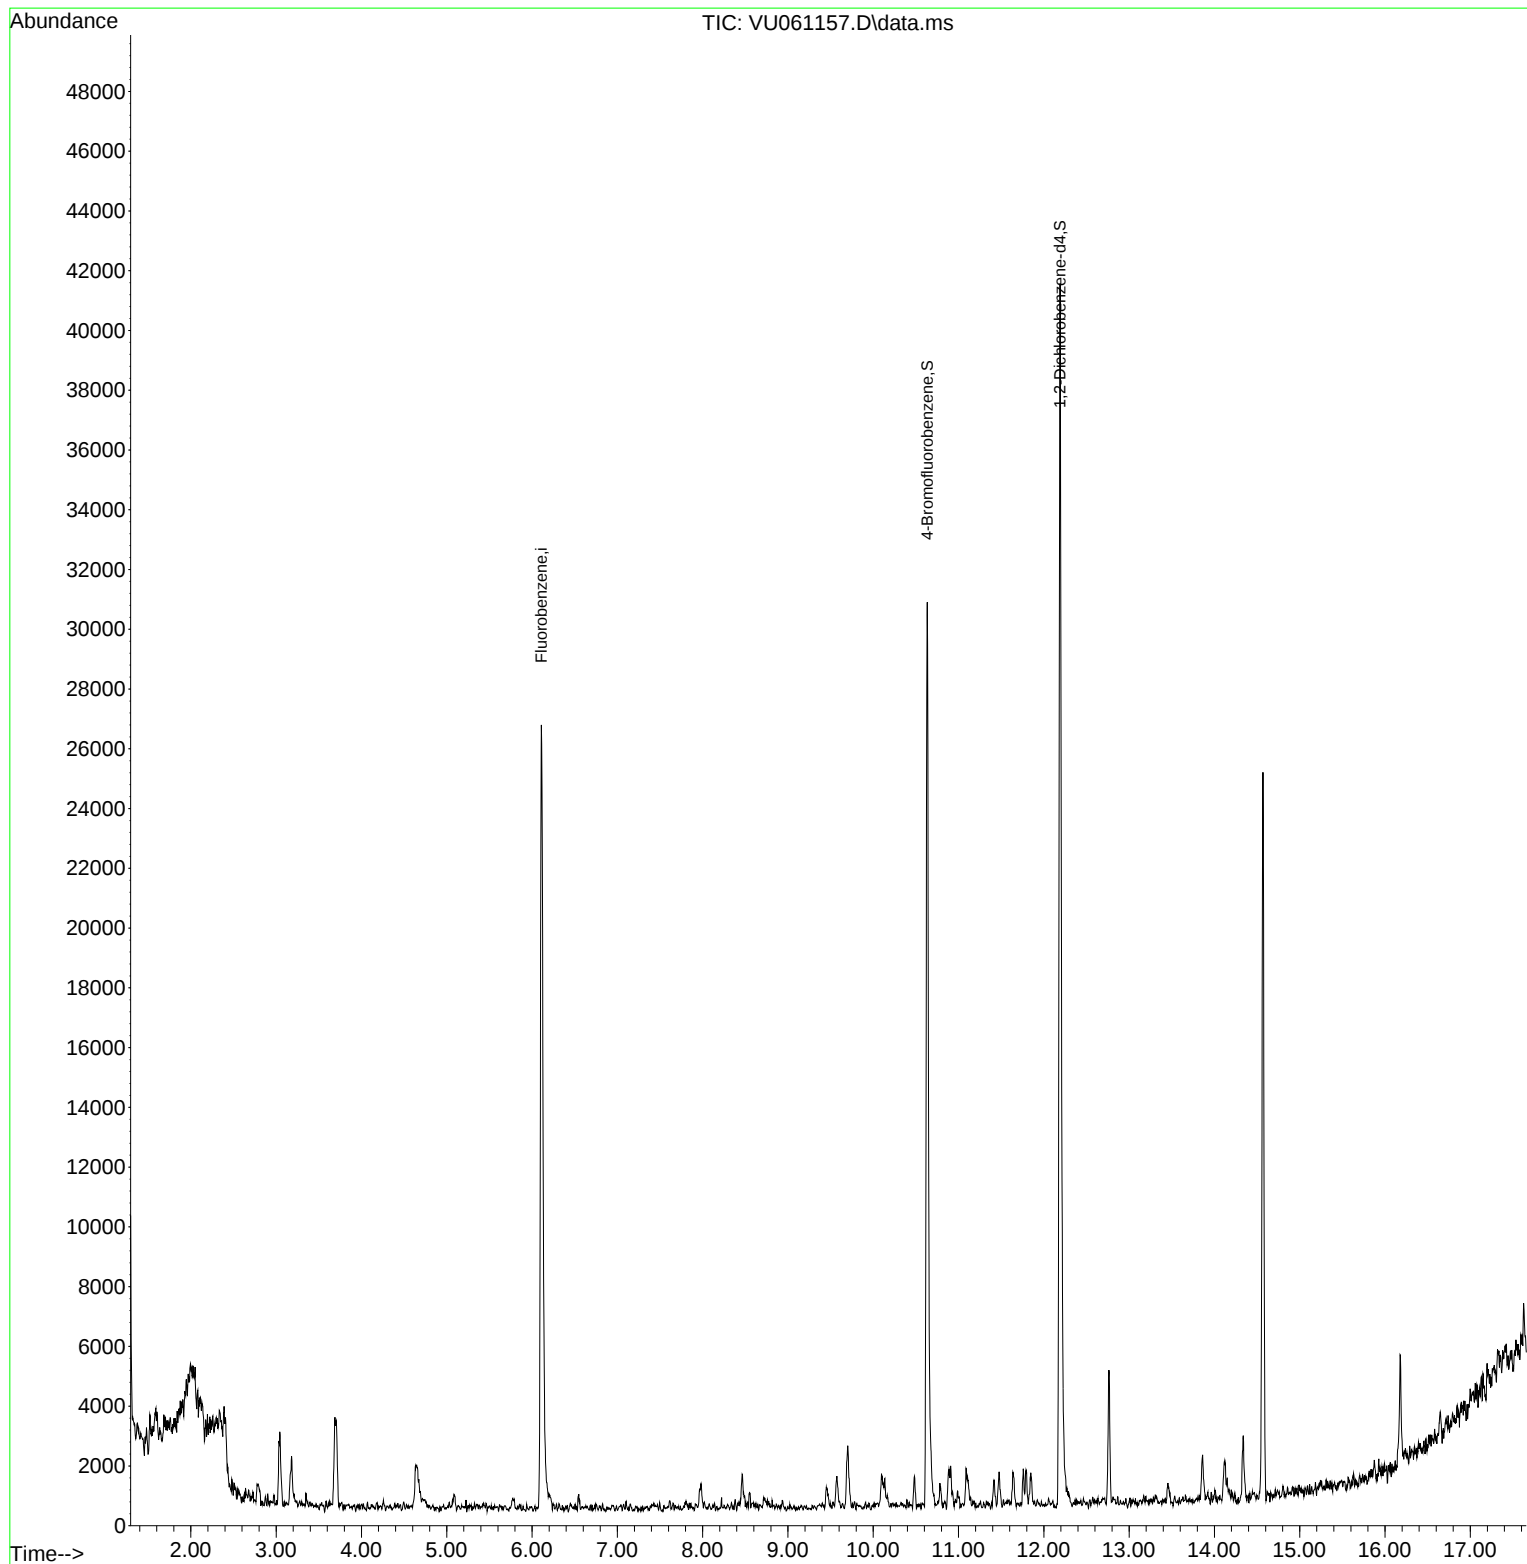


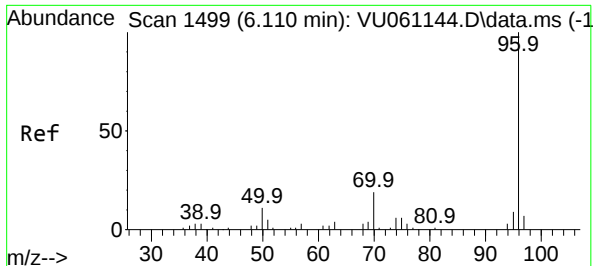

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.110 min Scan# 1499
Delta R.T. -0.000 min
Lab File: VU061157.D
Acq: 18 Oct 2024 11:34




Instrument :
MSVOA_U
ClientSampleId :
VU1018WBL01


Tgt Ion:	96	Resp:	27857
Ion Ratio	Lower	Upper	
96	100		
70	17.9	16.1	24.1
95	9.3	0.0	0.0#
97	6.1	0.0	0.0#

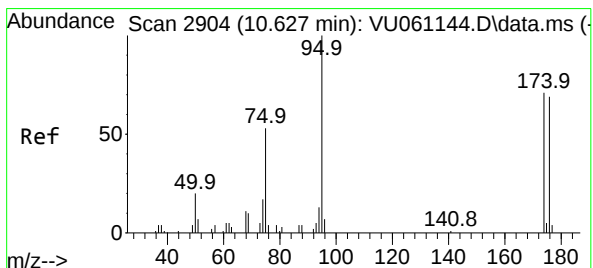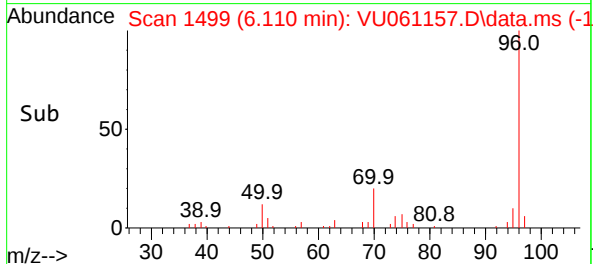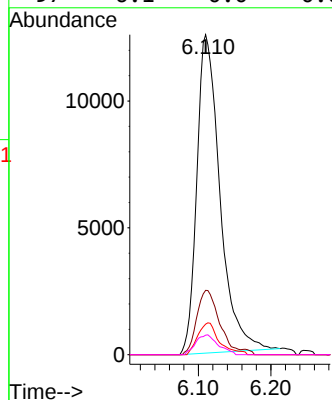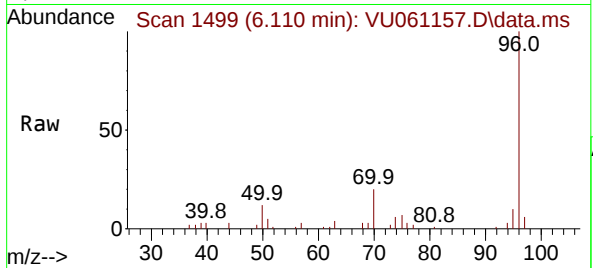

#57
4-Bromofluorobenzene
Concen: 0.860 ug/l
RT: 10.634 min Scan# 2906
Delta R.T. 0.006 min
Lab File: VU061157.D
Acq: 18 Oct 2024 11:34

Tgt Ion:	95	Resp:	12725
Ion Ratio	Lower	Upper	
95	100		
174	74.0	55.4	83.0
176	73.4	54.4	81.6

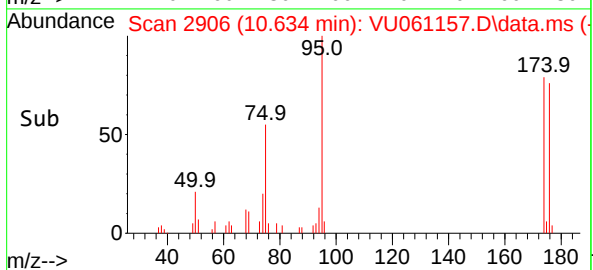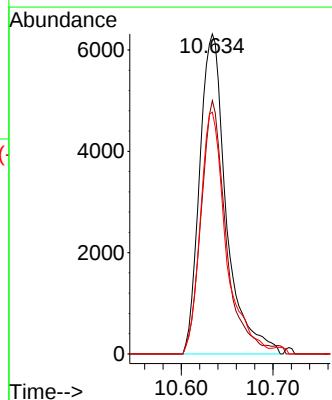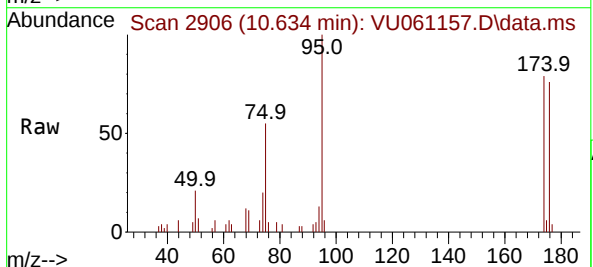

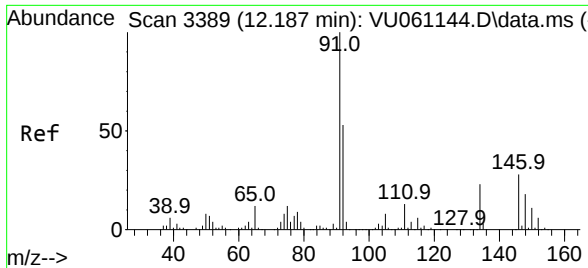

#68
 1,2-Dichlorobenzene-d4
 Concen: 0.826 ug/l
 RT: 12.190 min Scan# 31
 Delta R.T. 0.003 min
 Lab File: VU061157.D
 Acq: 18 Oct 2024 11:34

Instrument :
 MSVOA_U
 ClientSampleId :
 VU1018WBL01

Tgt Ion:	152	Resp:	12051
Ion	Ratio	Lower	Upper
152	100		
115	68.1	0.0	275.0
150	158.3	0.0	668.8

